
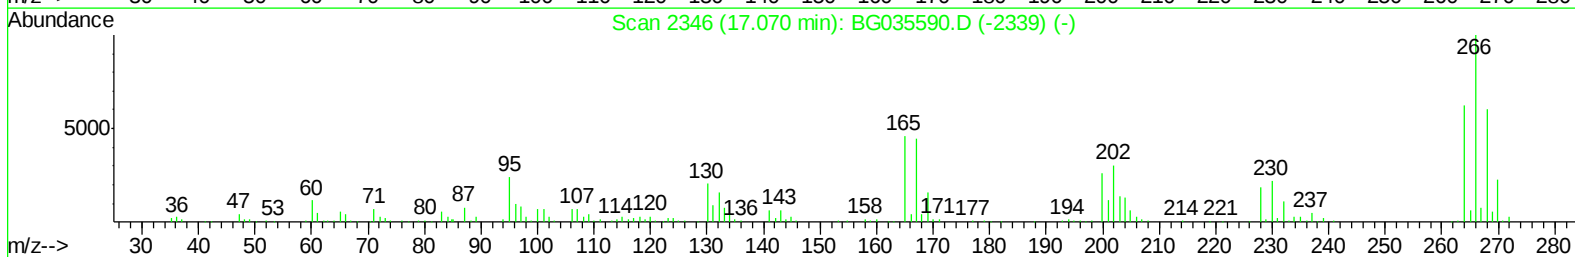
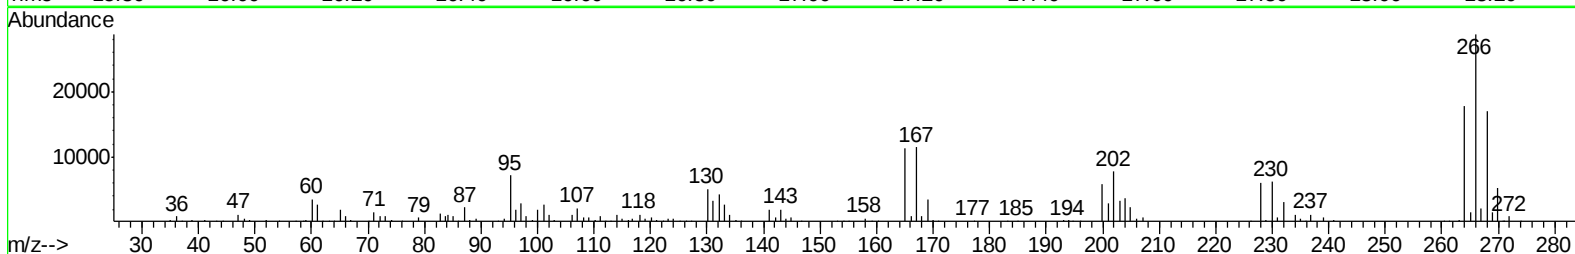


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071618\
Data File : BG035661.D
Acq On : 16 Jul 2018 9:28
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 09:04:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 12 14:43:32 2018
Response via : Initial Calibration

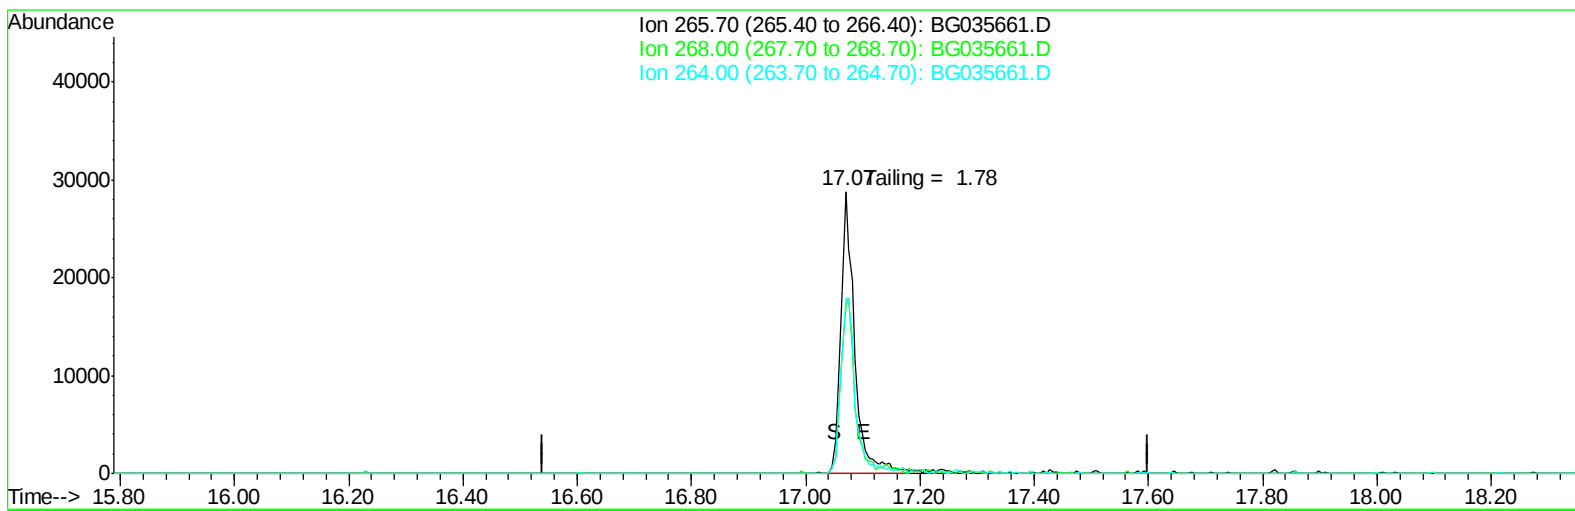

TIC: BG035661.D

(69) Pentachlorophenol (C)




17.070min (-17.070) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	63.90	0.00#
264.00	62.00	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071618\
 Data File : BG035661.D
 Acq On : 16 Jul 2018 9:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 09:04:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 12 14:43:32 2018
 Response via : Initial Calibration

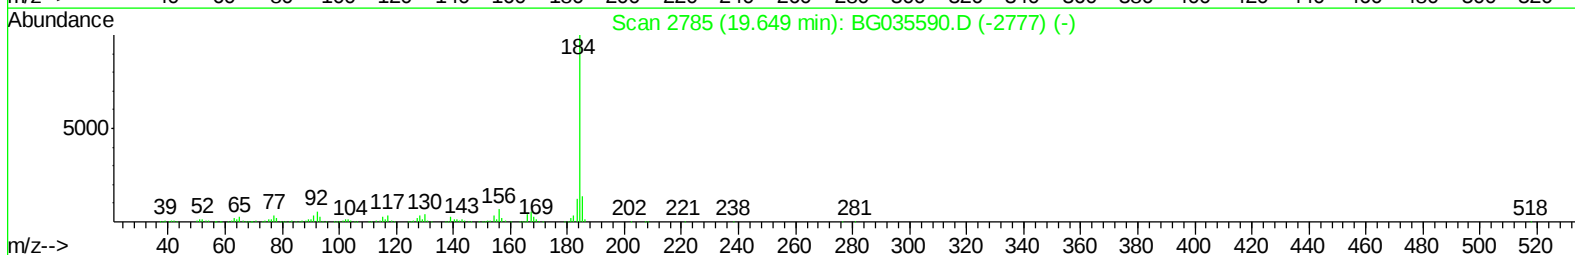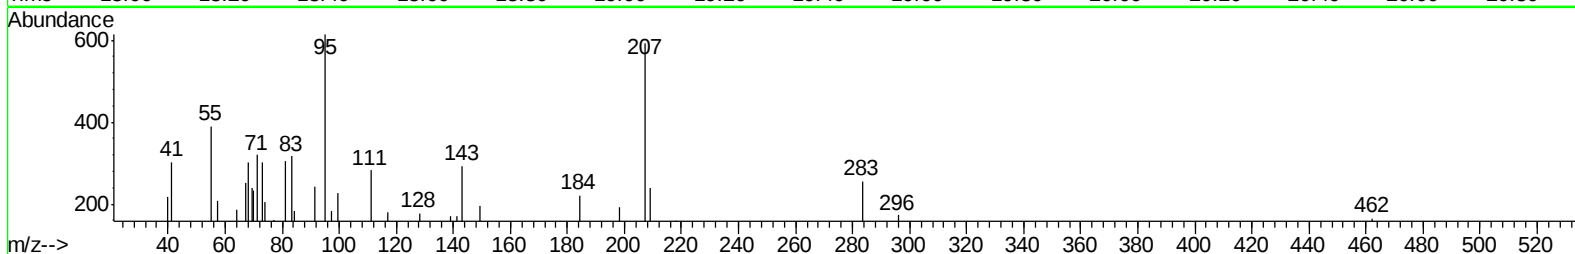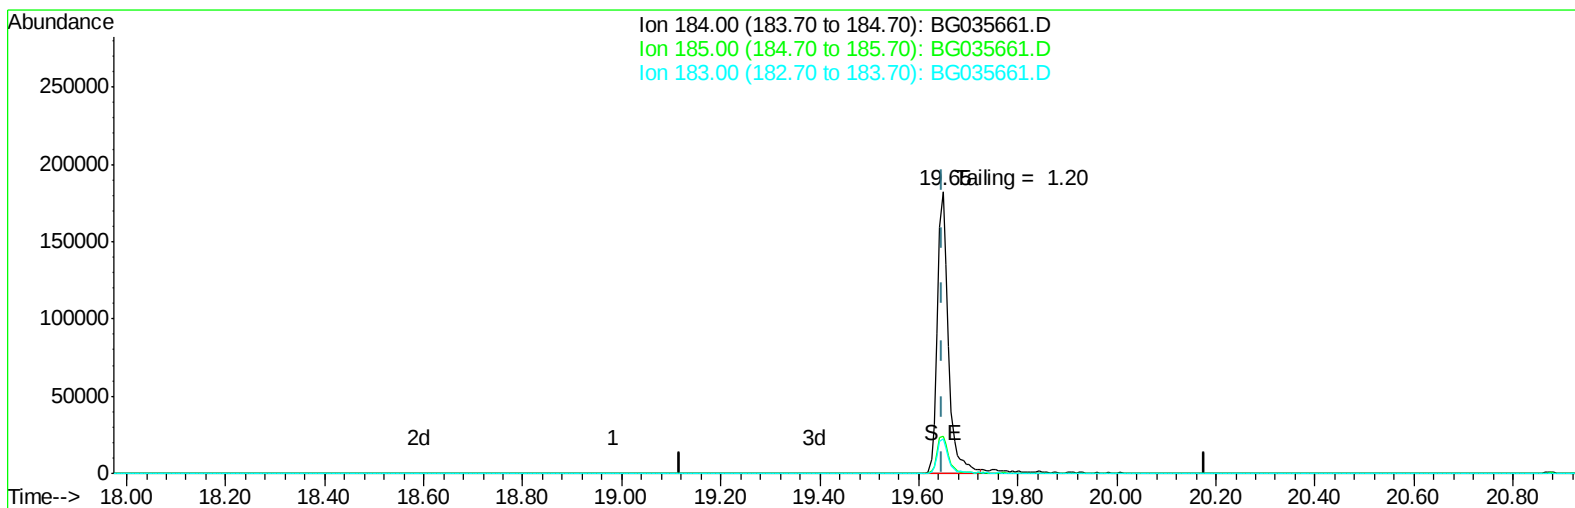

TIC: BG035661.D

(76) Benzidine

18.984min (-0.664) 1.14ng

response 78

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00