


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071618\
 Data File : BG035661.D
 Acq On : 16 Jul 2018 9:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

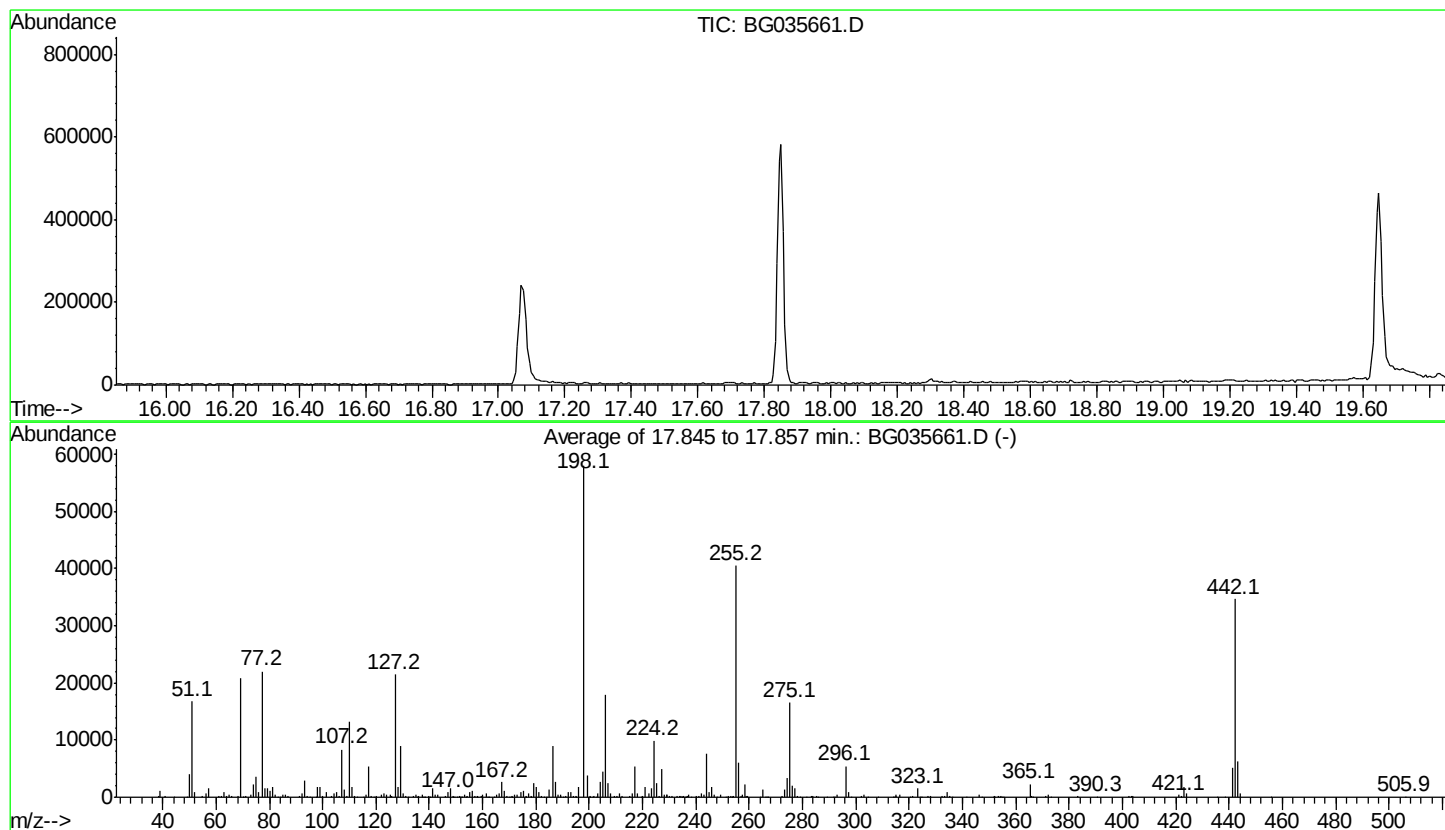

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	16780	PASS
68	69	0.00	2	0.9	193	PASS
69	198	0.00	100	35.9	20858	PASS
70	69	0.00	2	0.4	80	PASS
127	198	10	80	37.0	21444	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58032	PASS
199	198	5	9	6.6	3835	PASS
275	198	10	60	28.5	16553	PASS
365	198	1	100	3.9	2272	PASS
441	198	0.01	100	9.0	5204	PASS
442	198	50	100	59.8	34677	PASS
443	442	15	24	18.2	6327	PASS