

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071619\
 Data File : BG041678.D
 Acq On : 17 Jul 2019 3:53
 Operator : HP/JU
 Sample : PB121423BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB121423BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.192	14	17	29	rVB	78612	128203	1.59%	0.319%
2	5.612	421	429	441	rBV	1936580	3126548	38.71%	7.781%
3	7.199	689	699	713	rBV	2014105	3474325	43.02%	8.647%
4	7.580	756	764	777	rBV	1919768	3334512	41.29%	8.299%
5	8.051	837	844	853	rVB	371123	644949	7.99%	1.605%
6	8.374	891	899	910	rBV	1482256	2551111	31.59%	6.349%
7	9.202	1032	1040	1052	rBV	1163255	2080388	25.76%	5.178%
8	10.853	1311	1321	1331	rVB	524337	927743	11.49%	2.309%
9	13.297	1729	1737	1745	rBV	3184788	4986502	61.75%	12.410%
10	14.666	1963	1970	1978	rBV2	848979	1313540	16.26%	3.269%
11	16.141	2214	2221	2243	rBV	2248631	3584969	44.39%	8.922%
12	17.398	2426	2435	2447	rBV2	1111986	1745686	21.62%	4.345%
13	20.007	2873	2879	2886	rBV	5930845	8075955	100.00%	20.099%
14	21.652	3152	3159	3169	rBV	1236676	1997577	24.73%	4.971%
15	24.002	3554	3559	3567	rVB3	40043	83814	1.04%	0.209%
16	24.843	3692	3702	3714	rVV2	726648	2033756	25.18%	5.061%
17	24.954	3716	3721	3732	rVB3	36306	91375	1.13%	0.227%


Sum of corrected areas: 40180953

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071619\
Data File : BG041678.D
Acq On : 17 Jul 2019 3:53
Operator : HP/JU
Sample : PB121423BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB121423BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

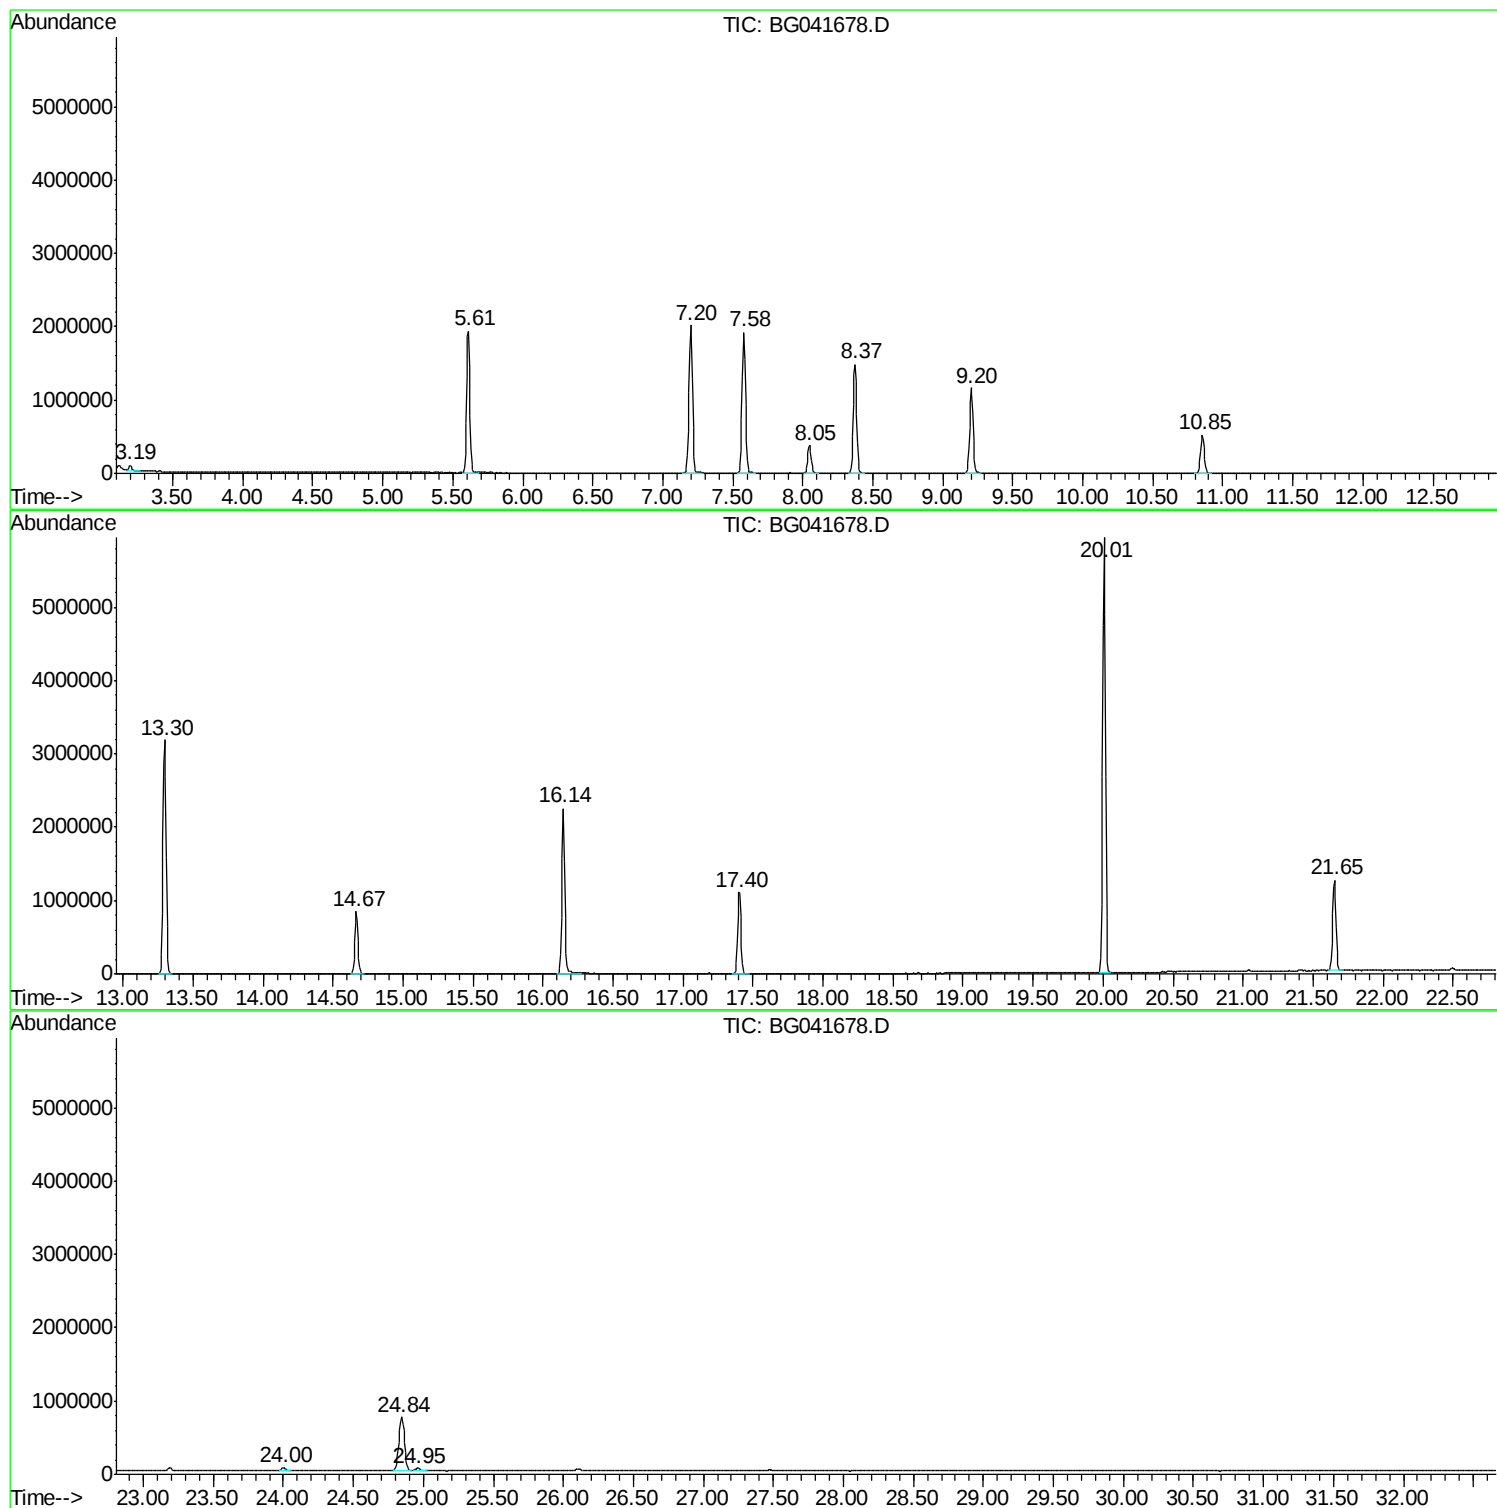

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071619\\
Data_File : BG041678.D
Acq_On : 17 Jul 2019 3:533
Operator : HP/JUU
Sample : PB121423BLL
Misc :
ALS_Vial : 20 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
PB121423BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
