


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071619\
Data File : BG041657.D
Acq On : 16 Jul 2019 7:48
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 15 16:16:21 2019

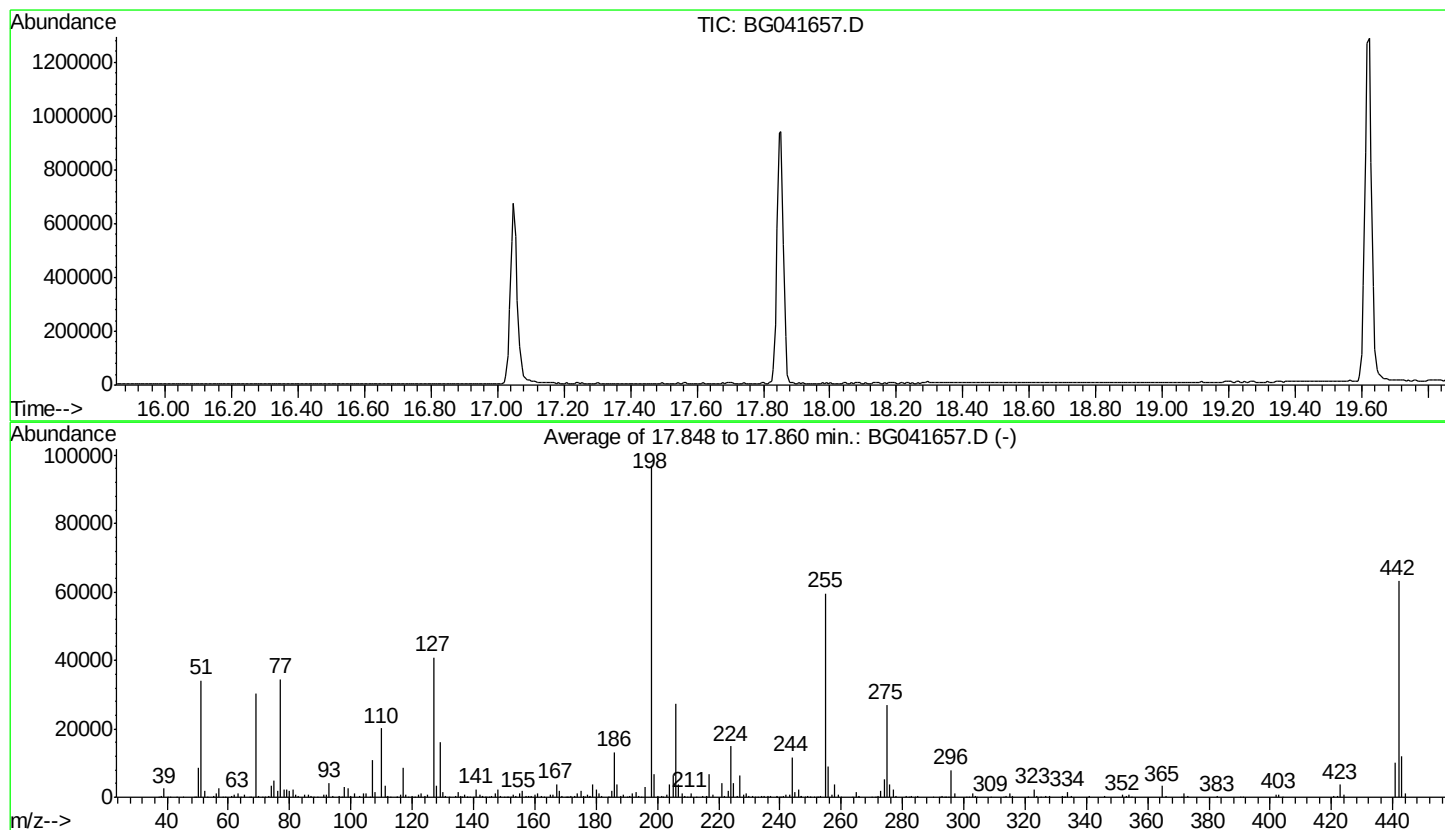

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	34178	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.4	30478	PASS
70	69	0.00	2	1.0	307	PASS
127	198	10	80	42.2	40930	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	96925	PASS
199	198	5	9	6.9	6676	PASS
275	198	10	60	27.8	26970	PASS
365	198	1	100	3.5	3365	PASS
441	198	0.01	100	10.4	10046	PASS
442	198	50	100	65.4	63357	PASS
443	442	15	24	18.8	11927	PASS