


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071619\
 Data File : BG041675.D
 Acq On : 16 Jul 2019 20:11
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 15 16:16:21 2019

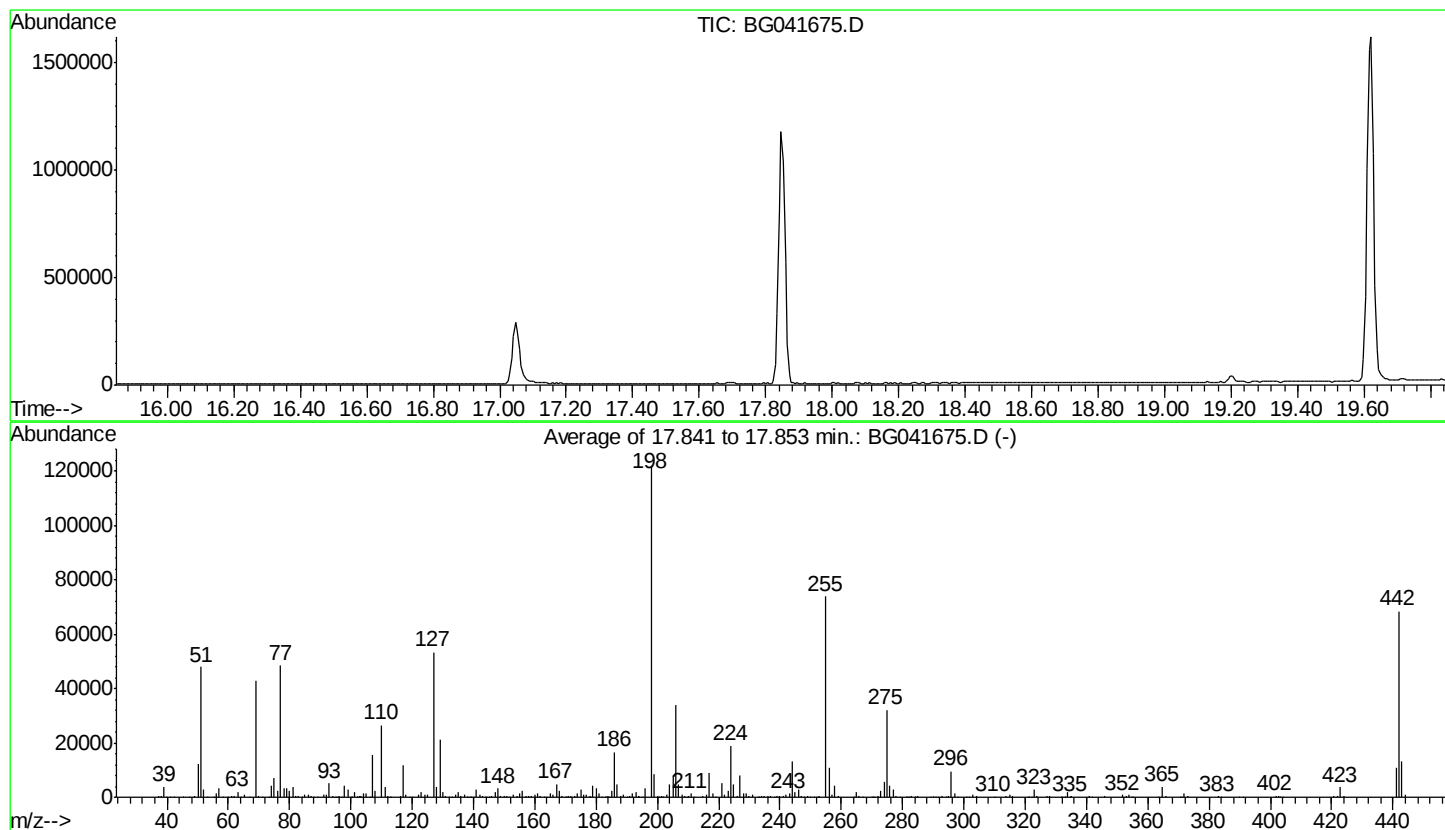

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	47930	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.0	42651	PASS
70	69	0.00	2	0.7	286	PASS
127	198	10	80	43.6	53210	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121954	PASS
199	198	5	9	7.0	8527	PASS
275	198	10	60	26.4	32149	PASS
365	198	1	100	3.2	3921	PASS
441	198	0.01	100	8.8	10742	PASS
442	198	50	100	56.1	68408	PASS
443	442	15	24	19.0	13022	PASS