

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071723\
 Data File : BG058284.D
 Acq On : 17 Jul 2023 15:52
 Operator : CG/JU
 Sample : SSTD01093
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010443

Quant Time: Jul 18 01:30:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 01:24:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	44148	20.000	ng/u1	0.00
20) Naphthalene-d8	10.703	136	201529	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.540	164	146267	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.284	188	362299	20.000	ng/u1	0.00
79) Chrysene-d12	21.532	240	318521	20.000	ng/u1	0.00
88) Perylene-d12	24.663	264	370379	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.341	96	5253	4.167	ng/uL	0.00
4) Pyridine-d5	3.752	84	33955	8.871	ng/u1	0.00
7) Phenol-d5	7.066	99	40672	9.021	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.225	67	27459	10.106	ng/u1	0.00
11) 2-Chlorophenol-d4	7.430	132	29396	9.453	ng/u1	0.00
15) 4-Methylphenol-d8	8.606	113	31015	9.117	ng/u1	0.00
21) Nitrobenzene-d5	9.064	128	14720	8.962	ng/u1	0.00
24) 2-Nitrophenol-d4	9.781	143	16012	9.275	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.327	165	31694	9.570	ng/u1	0.00
31) 4-Chloroaniline-d4	10.838	131	49295	9.818	ng/u1	0.00
46) Dimethylphthalate-d6	13.940	166	119610	10.364	ng/u1	0.00
49) Acenaphthylene-d8	14.228	160	124659	9.899	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	15759	7.729	ng/u1	0.00
60) Fluorene-d10	15.527	176	100056	10.209	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.650	200	16323	8.297	ng/u1	0.00
73) Anthracene-d10	17.378	188	166700	9.916	ng/u1	0.00
81) Pyrene-d10	19.669	212	198446	9.892	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.446	264	182938	9.695	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.376	88	5889	3.781	ng/uL	93
5) Pyridine	3.770	79	38106	9.717	ng/u1	97
6) Benzaldehyde	7.043	77	11020	7.319	ng/u1	94
8) Phenol	7.090	94	43351	9.475	ng/u1	94
10) Bis(2-Chloroethyl)ether	7.319	93	34310	9.712	ng/u1	98
12) 2-Chlorophenol	7.466	128	31119	9.617	ng/u1	95
13) 2-Methylphenol	8.341	108	33516	9.328	ng/u1	93
14) 2,2'-oxybis(1-Chloropr...	8.429	45	57220	10.522	ng/u1	98
16) Acetophenone	8.723	105	58260	10.322	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.700	70	30957	10.260	ng/u1	98
18) 4-Methylphenol	8.670	108	36893	9.495	ng/u1	96
19) Hexachloroethane	8.982	117	12794	10.314	ng/u1	83
22) Nitrobenzene	9.105	77	40701	9.545	ng/u1	99
23) Isophorone	9.622	82	92703	10.189	ng/u1	100
25) 2-Nitrophenol	9.816	139	17403	9.395	ng/u1	98
26) 2,4-Dimethylphenol	9.875	107	39983	9.599	ng/u1	98
27) Bis(2-Chloroethoxy)met...	10.110	93	49371	9.629	ng/u1	97
29) 2,4-Dichlorophenol	10.351	162	29741	9.237	ng/u1	97
30) Naphthalene	10.756	128	112494	9.933	ng/u1	99
32) 4-Chloroaniline	10.862	127	50203	9.779	ng/u1	98
33) Hexachlorobutadiene	11.032	225	21872	9.595	ng/u1	96
34) Caprolactam	11.620	113	12745	9.845	ng/u1	92
35) 4-Chloro-3-methylphenol	11.990	107	37977	9.602	ng/u1	94
36) 2-Methylnaphthalene	12.360	142	75144	9.843	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071723\
 Data File : BG058284.D
 Acq On : 17 Jul 2023 15:52
 Operator : CG/JU
 Sample : SSTD01093
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SSTD010443

Quant Time: Jul 18 01:30:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 01:24:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.583	142	78386	10.239	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.730	216	44937	10.081	ng/ul	99
40) Hexachlorocyclopentadiene	12.707	237	18276	6.509	ng/ul	93
41) 2,4,6-Trichlorophenol	12.971	196	28322	9.375	ng/ul	95
42) 2,4,5-Trichlorophenol	13.041	196	29969	9.173	ng/ul	97
43) 1,1'-Biphenyl	13.371	154	106952	10.147	ng/ul	99
44) 2-Chloronaphthalene	13.412	162	83033	9.815	ng/ul	97
45) 2-Nitroaniline	13.617	65	26336	8.954	ng/ul	94
47) Dimethylphthalate	13.987	163	121207	10.454	ng/ul	98
48) 2,6-Dinitrotoluene	14.111	165	21736	9.133	ng/ul	95
50) Acenaphthylene	14.258	152	135872	9.991	ng/ul	99
51) 3-Nitroaniline	14.446	138	16195	8.052	ng/ul	93
52) Acenaphthene	14.598	153	93873	10.059	ng/ul	99
53) 2,4-Dinitrophenol	14.651	184	8164	6.580	ng/ul#	88
55) 4-Nitrophenol	14.751	109	11483	7.602	ng/ul	94
56) Dibenzofuran	14.933	168	135795	10.237	ng/ul	100
57) 2,4-Dinitrotoluene	14.898	165	31870	9.451	ng/ul	91
58) 2,3,4,6-Tetrachlorophenol	15.163	232	27865	9.369	ng/ul#	96
59) Diethylphthalate	15.345	149	125662	10.384	ng/ul	99
61) Fluorene	15.586	166	111874	10.278	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.574	204	58701	10.193	ng/ul	98
63) 4-Nitroaniline	15.603	138	10962	6.084	ng/ul	92
66) 4,6-Dinitro-2-methylph...	15.662	198	17026	8.463	ng/ul	98
67) N-Nitrosodiphenylamine	15.791	169	95399	9.894	ng/ul	99
68) 4-Bromophenyl-phenylether	16.467	248	39876	10.027	ng/ul	100
69) Hexachlorobenzene	16.590	284	44821	10.066	ng/ul	97
70) Atrazine	16.731	200	38633	9.798	ng/ul	98
71) Pentachlorophenol	16.937	266	20815	7.787	ng/ul	99
72) Phenanthrene	17.325	178	185963	10.091	ng/ul	99
74) Anthracene	17.413	178	185291	9.936	ng/ul	97
75) 1,2,3,4-Tetrachloroben...	13.335	216	48044	9.999	ng/ul	98
76) Pentachlorobenzene	14.857	250	51276	9.992	ng/ul	98
77) Carbazole	17.683	167	170785	10.126	ng/ul	98
78) Di-n-butylphthalate	18.235	149	204433	9.515	ng/ul	99
80) Fluoranthene	19.334	202	227063	9.768	ng/ul	99
82) Pyrene	19.698	202	235398	10.060	ng/ul	99
83) Butylbenzylphthalate	20.580	149	86882	9.157	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.432	252	74624	9.677	ng/ul	97
85) Benzo(a)anthracene	21.508	228	223292	9.763	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.414	149	126286	9.288	ng/ul	99
87) Chrysene	21.579	228	215318	10.043	ng/ul	99
89) Di-n-octyl phthalate	22.589	149	213649	9.388	ng/ul	100
90) Benzo(b)fluoranthene	23.664	252	226214	9.864	ng/ul	99
91) Benzo(k)fluoranthene	23.729	252	222600	9.903	ng/ul	99
93) Benzo(a)pyrene	24.510	252	198187	9.764	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	28.224	276	256186	9.505	ng/ul	98
95) Dibenzo(a,h)anthracene	28.282	278	212607	9.565	ng/ul	98
96) Benzo(g,h,i)perylene	29.340	276	208592	9.475	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA G

ClientSampleId :

SSTD010443


Quant Time: Jul 18 01:30:21 2023


Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Jul 18 01:24:07 2023

Response via : Initial Calibration





#2
1,4-Dioxane

Concen: 3.781 ng/uL

RT: 3.376 min Scan# 49

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion: 88 Resp: 5889

Ion Ratio Lower Upper

88 100

43 25.2 19.6 29.4

58 80.3 70.2 105.4

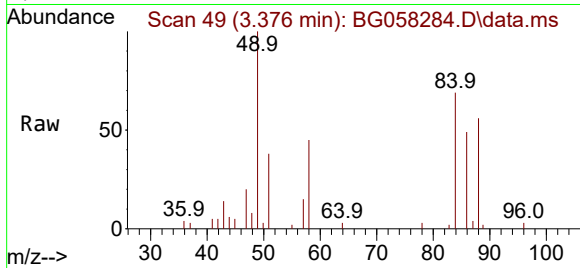

#5

Pyridine

Concen: 9.717 ng/uL

RT: 3.770 min Scan# 116

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion: 79 Resp: 38106


Ion Ratio Lower Upper

79 100

52 89.9 72.3 108.5

51 46.8 33.4 50.0




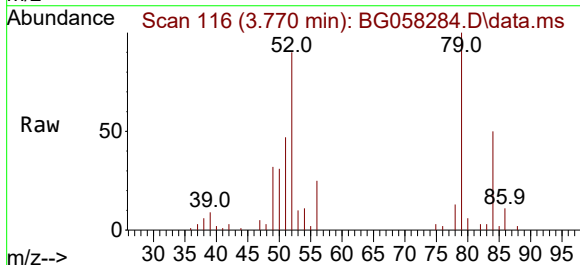




#6
Benzaldehyde
Concen: 7.319 ng/ul
RT: 7.043 min Scan# 61
Delta R.T. 0.008 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:	77	Resp:	11020
Ion	Ratio	Lower	Upper
77	100		
105	89.0	78.2	117.4
106	91.9	71.6	107.4



#8
Phenol
Concen: 9.475 ng/ul
RT: 7.090 min Scan# 681
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:	94	Resp:	43351
Ion	Ratio	Lower	Upper
94	100		
65	29.0	23.8	35.8
66	33.2	31.2	46.8



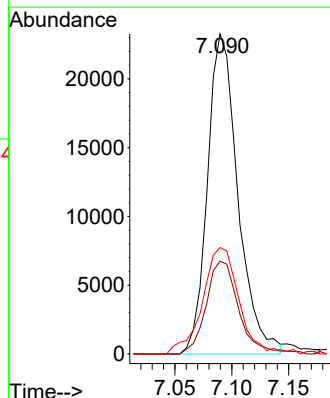





#10
Bis(2-Chloroethyl)ether
Concen: 9.712 ng/ul
RT: 7.319 min Scan# 720
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion: 93 Resp: 34310
Ion Ratio Lower Upper
93 100
63 87.1 67.7 101.5
95 32.8 27.0 40.6



#12
2-Chlorophenol
Concen: 9.617 ng/ul
RT: 7.466 min Scan# 745
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion: 128 Resp: 31119
Ion Ratio Lower Upper
128 100
64 59.5 45.6 68.4
130 36.6 25.2 37.8



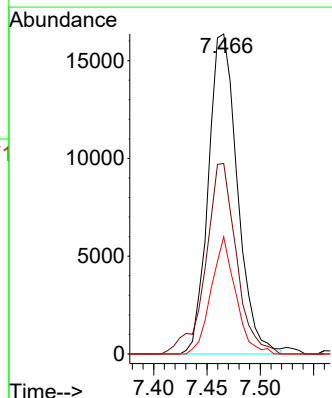





#13
2-Methylphenol
Concen: 9.328 ng/ul
RT: 8.341 min Scan# 894
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:108 Resp: 33516
Ion Ratio Lower Upper
108 100
107 83.2 71.5 107.3

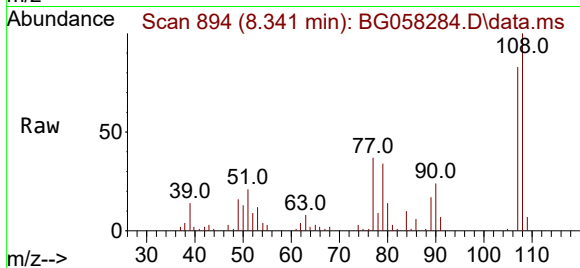

#14
2,2'-oxybis(1-Chloropropane)
Concen: 10.522 ng/ul
RT: 8.429 min Scan# 909
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion: 45 Resp: 57220
Ion Ratio Lower Upper
45 100
77 13.0 9.4 14.2
79 9.2 7.4 11.2




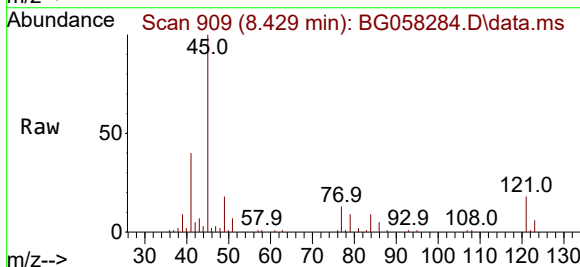




#16
Acetophenone
Concen: 10.322 ng/ul
RT: 8.723 min Scan# 91
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:105 Resp: 58260
Ion Ratio Lower Upper
105 100
77 75.5 60.7 91.1
51 30.1 23.5 35.3

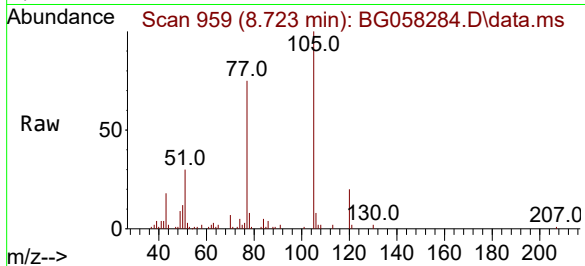

#17
N-Nitroso-di-n-propylamine
Concen: 10.260 ng/ul
RT: 8.700 min Scan# 955
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion: 70 Resp: 30957
Ion Ratio Lower Upper
70 100
42 58.9 46.6 69.8
101 7.5 7.3 10.9
130 19.0 14.2 21.2




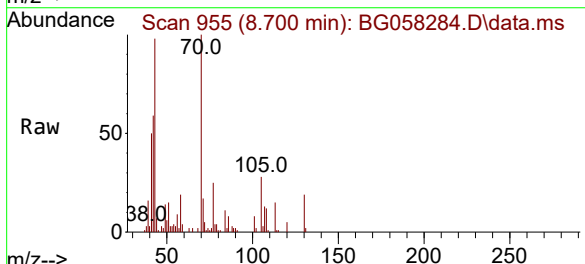




#18
4-Methylphenol
Concen: 9.495 ng/ul
RT: 8.670 min Scan# 91
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:108 Resp: 36893
Ion Ratio Lower Upper
108 100
107 108.9 90.6 136.0



#19
Hexachloroethane
Concen: 10.314 ng/ul
RT: 8.982 min Scan# 1003
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:117 Resp: 12794
Ion Ratio Lower Upper
117 100
201 104.7 103.6 155.4
199 67.1 60.1 90.1



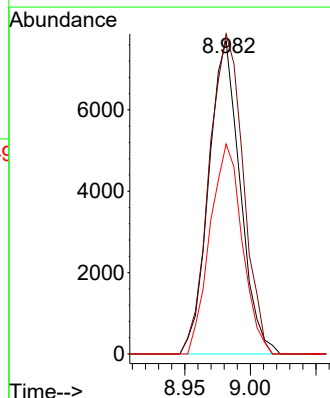
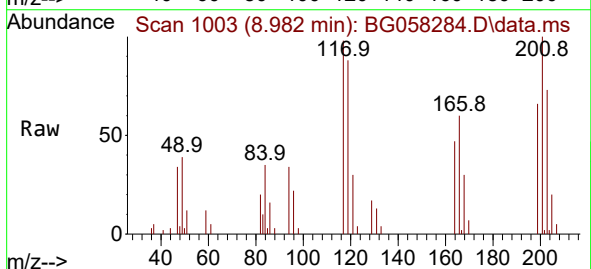




#22
Nitrobenzene
Concen: 9.545 ng/ul
RT: 9.105 min Scan# 1024
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion: 77 Resp: 40701
Ion Ratio Lower Upper
77 100
123 41.7 34.0 51.0
65 14.6 11.0 16.6



#23
Isophorone
Concen: 10.189 ng/ul
RT: 9.622 min Scan# 1112
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion: 82 Resp: 92703
Ion Ratio Lower Upper
82 100
95 6.5 5.1 7.7
138 14.9 11.9 17.9









#25
2-Nitrophenol
Concen: 9.395 ng/ul
RT: 9.816 min Scan# 1145
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:139 Resp: 17403
Ion Ratio Lower Upper
139 100
65 60.2 49.2 73.8
109 27.9 21.6 32.4



#26
2,4-Dimethylphenol
Concen: 9.599 ng/ul
RT: 9.875 min Scan# 1155
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:107 Resp: 39983
Ion Ratio Lower Upper
107 100
121 47.7 39.1 58.7
122 84.7 68.9 103.3





#27

Bis(2-Chloroethoxy)methane

Concen: 9.629 ng/ul

RT: 10.110 min Scan# 1195

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion: 93 Resp: 49371

Ion Ratio Lower Upper

93 100

95 33.8 25.8 38.8

123 10.4 9.3 13.9

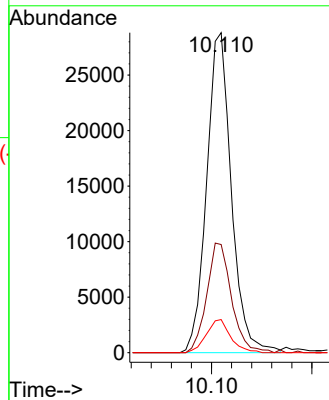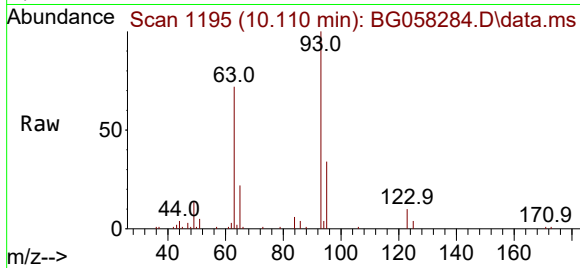

#29

2,4-Dichlorophenol

Concen: 9.237 ng/ul

RT: 10.351 min Scan# 1236

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion:162 Resp: 29741


Ion Ratio Lower Upper

162 100

164 69.8 58.4 87.6

98 38.3 29.6 44.4



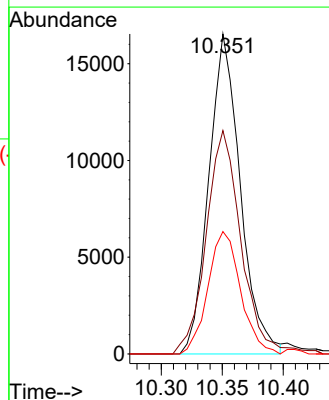
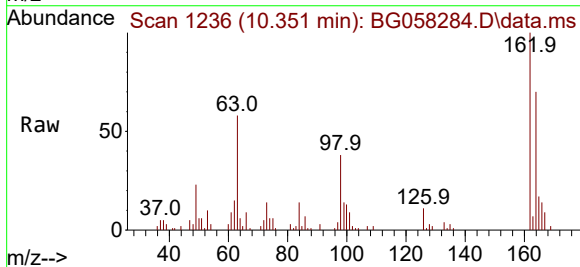




#30
Naphthalene
Concen: 9.933 ng/ul
RT: 10.756 min Scan# 11
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:128 Resp: 112494
Ion Ratio Lower Upper
128 100
129 10.6 8.8 13.2
127 13.1 10.8 16.2

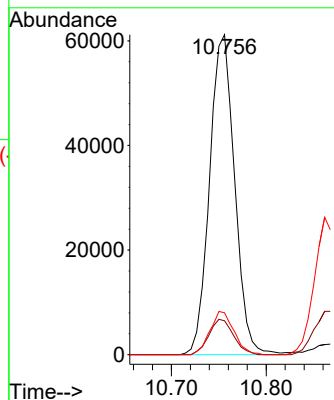

#32
4-Chloroaniline
Concen: 9.779 ng/ul
RT: 10.862 min Scan# 1323
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:127 Resp: 50203
Ion Ratio Lower Upper
127 100
129 31.6 26.1 39.1

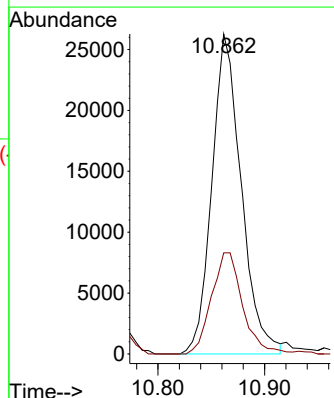



#33

Hexachlorobutadiene

Concen: 9.595 ng/ul

RT: 11.032 min Scan# 11

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:225 Resp: 21872

Ion Ratio Lower Upper

225 100

223 66.1 49.7 74.5

227 63.9 53.2 79.8

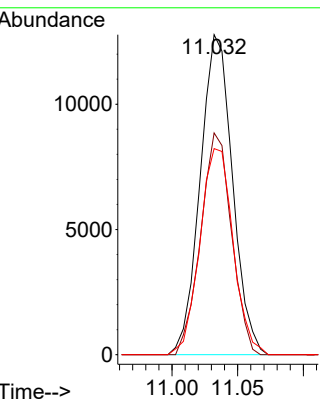

#34

Caprolactam

Concen: 9.845 ng/ul

RT: 11.620 min Scan# 1452

Delta R.T. -0.016 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion:113 Resp: 12745


Ion Ratio Lower Upper

113 100

55 221.7 179.8 269.6

56 143.9 132.2 198.4

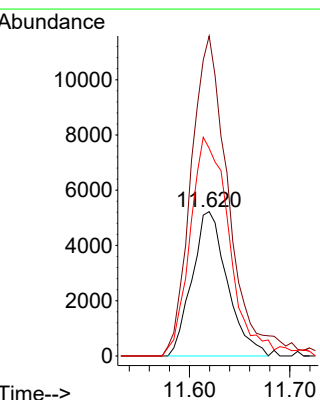



#35

4-Chloro-3-methylphenol

Concen: 9.602 ng/ul

RT: 11.990 min Scan# 1

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:107 Resp: 37977

Ion Ratio Lower Upper

107 100

144 23.9 19.0 28.6

142 76.8 55.8 83.6

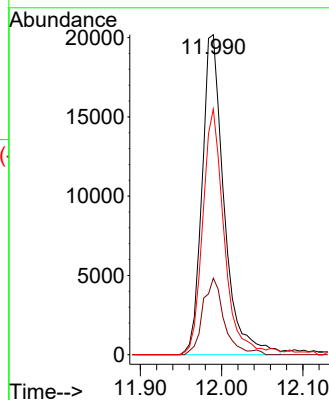

#36

2-Methylnaphthalene

Concen: 9.843 ng/ul

RT: 12.360 min Scan# 1578

Delta R.T. 0.002 min

Lab File: BG058284.D




Acq: 17 Jul 2023 15:52


Tgt Ion:142 Resp: 75144

Ion Ratio Lower Upper

142 100

141 91.1 72.6 108.8

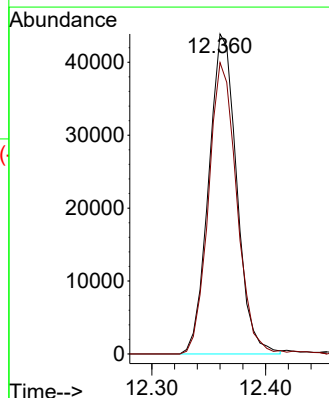



#37

1-Methylnaphthalene

Concen: 10.239 ng/ul

RT: 12.583 min Scan# 1

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:142 Resp: 78386

Ion Ratio Lower Upper

142 100

141 95.5 75.8 113.6

116 4.3 3.2 4.8



#39

1,2,4,5-Tetrachlorobenzene

Concen: 10.081 ng/ul

RT: 12.730 min Scan# 1641

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Tgt Ion:216 Resp: 44937




Ion Ratio Lower Upper


216 100

214 78.0 62.2 93.4

179 19.5 16.2 24.2

108 16.2 12.2 18.4









#40
Hexachlorocyclopentadiene
Concen: 6.509 ng/ul
RT: 12.707 min Scan# 1637
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:237 Resp: 18276
Ion Ratio Lower Upper
237 100
235 57.6 50.9 76.3
272 12.8 10.8 16.2



#41
2,4,6-Trichlorophenol
Concen: 9.375 ng/ul
RT: 12.971 min Scan# 1682
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:196 Resp: 28322
Ion Ratio Lower Upper
196 100
198 90.6 77.7 116.5
200 30.7 25.0 37.6









#42
2,4,5-Trichlorophenol
Concen: 9.173 ng/ul
RT: 13.041 min Scan# 1
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:196 Resp: 29969
Ion Ratio Lower Upper
196 100
198 95.5 74.8 112.2
200 27.8 24.4 36.6



#43
1,1'-Biphenyl
Concen: 10.147 ng/ul
RT: 13.371 min Scan# 1750
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:154 Resp: 106952
Ion Ratio Lower Upper
154 100
153 40.0 31.8 47.6
76 13.4 11.7 17.5

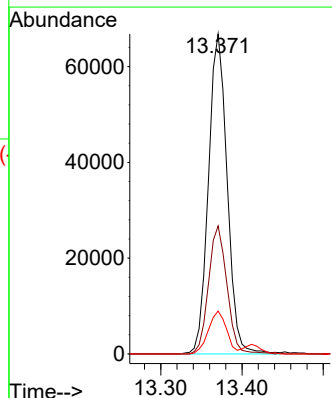



#44

2-Chloronaphthalene

Concen: 9.815 ng/ul

RT: 13.412 min Scan# 1

Delta R.T. -0.004 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:162 Resp: 83033

Ion Ratio Lower Upper

162 100

164 35.2 26.2 39.2

127 36.2 29.8 44.6

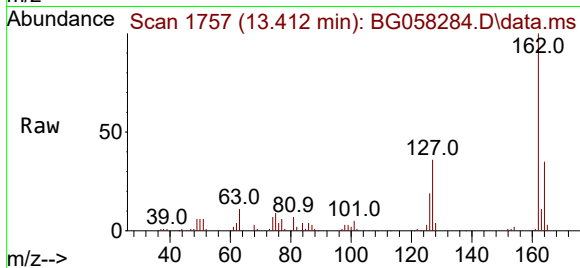

#45

2-Nitroaniline

Concen: 8.954 ng/ul

RT: 13.617 min Scan# 1792

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion: 65 Resp: 26336


Ion Ratio Lower Upper

65 100

92 68.1 51.4 77.2

138 83.8 71.6 107.4




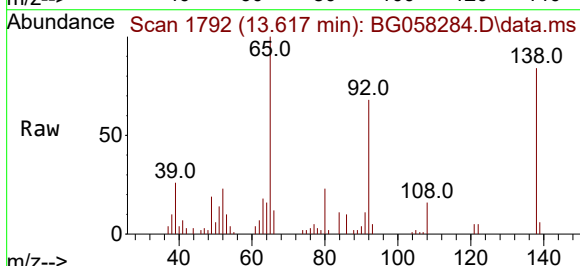




#47
Dimethylphthalate
Concen: 10.454 ng/ul
RT: 13.987 min Scan# 1855
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:163 Resp: 121207
Ion Ratio Lower Upper
163 100
194 3.8 2.6 3.8
164 10.8 8.2 12.2

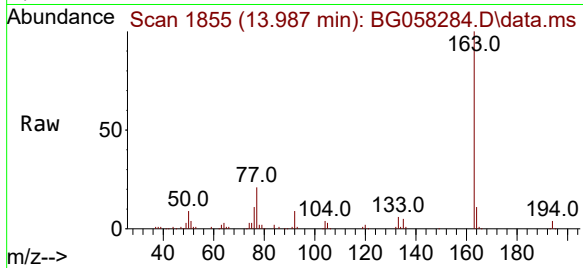

#48
2,6-Dinitrotoluene
Concen: 9.133 ng/ul
RT: 14.111 min Scan# 1876
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:165 Resp: 21736
Ion Ratio Lower Upper
165 100
89 64.6 48.9 73.3
121 23.4 16.2 24.4




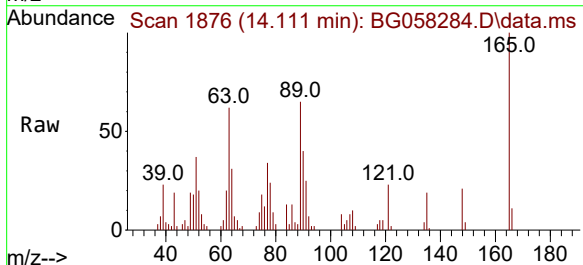




#50
Acenaphthylene
Concen: 9.991 ng/ul
RT: 14.258 min Scan# 1902
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:152 Resp: 135872
Ion Ratio Lower Upper
152 100
151 19.8 16.4 24.6
153 13.6 10.6 16.0



#51
3-Nitroaniline
Concen: 8.052 ng/ul
RT: 14.446 min Scan# 1933
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:138 Resp: 16195
Ion Ratio Lower Upper
138 100
108 11.8 8.6 13.0
92 126.2 108.4 162.6





#52

Acenaphthene

Concen: 10.059 ng/ul

RT: 14.598 min Scan# 1959

Delta R.T. -0.004 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:153 Resp: 93873

Ion Ratio Lower Upper

153 100

152 47.7 39.1 58.7

154 86.3 68.7 103.1

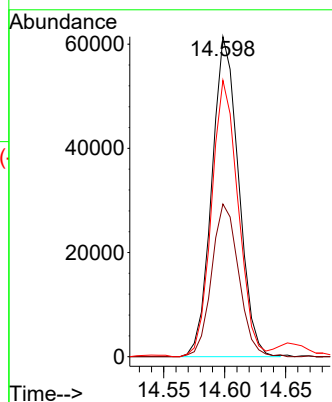

#53

2,4-Dinitrophenol

Concen: 6.580 ng/ul

RT: 14.651 min Scan# 1968

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion:184 Resp: 8164


Ion Ratio Lower Upper

184 100

63 80.5 52.9 79.3#

154 63.6 47.8 71.8









#55
4-Nitrophenol
Concen: 7.602 ng/ul
RT: 14.751 min Scan# 1985
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:109 Resp: 11483
Ion Ratio Lower Upper
109 100
139 138.2 100.3 150.5
65 152.7 120.6 180.8



#56
Dibenzofuran
Concen: 10.237 ng/ul
RT: 14.933 min Scan# 2016
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:168 Resp: 135795
Ion Ratio Lower Upper
168 100
139 34.9 27.8 41.8









#57
2,4-Dinitrotoluene
Concen: 9.451 ng/ul
RT: 14.898 min Scan# 2011
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:165 Resp: 31870
Ion Ratio Lower Upper
165 100
63 47.8 33.8 50.6
182 1.7 1.2 1.8



#58
2,3,4,6-Tetrachlorophenol
Concen: 9.369 ng/ul
RT: 15.163 min Scan# 2055
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:232 Resp: 27865
Ion Ratio Lower Upper
232 100
131 38.6 29.0 43.6
130 2.7 1.1 1.7#
166 30.8 23.0 34.6



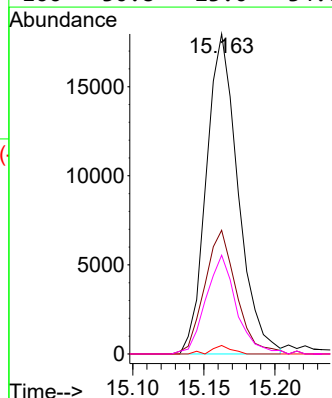



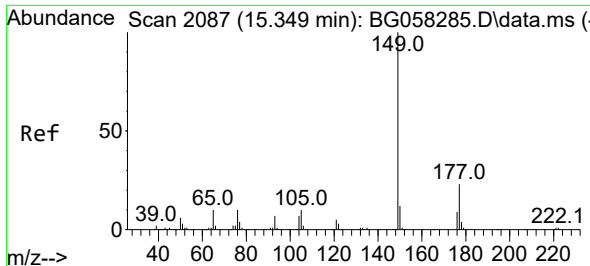

#59
Diethylphthalate
Concen: 10.384 ng/ul
RT: 15.345 min Scan# 2086
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:149 Resp: 125662
Ion Ratio Lower Upper
149 100
177 22.3 18.4 27.6
150 12.8 10.0 15.0

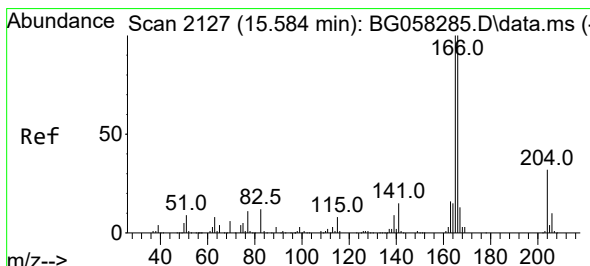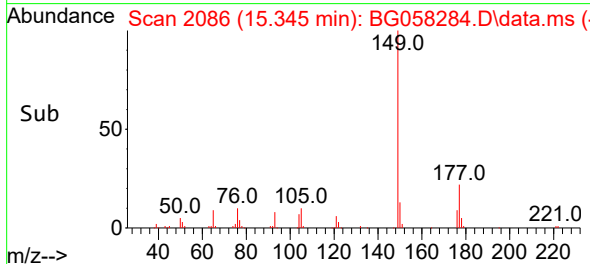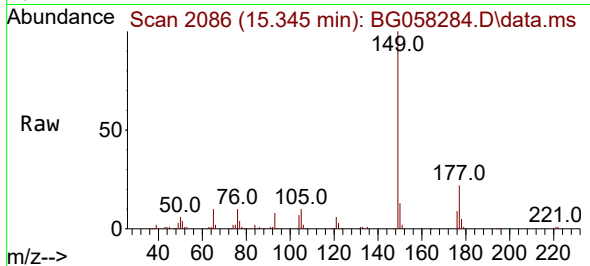

#61
Fluorene
Concen: 10.278 ng/ul
RT: 15.586 min Scan# 2127
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:166 Resp: 111874
Ion Ratio Lower Upper
166 100
165 98.2 80.2 120.2
167 13.9 10.5 15.7


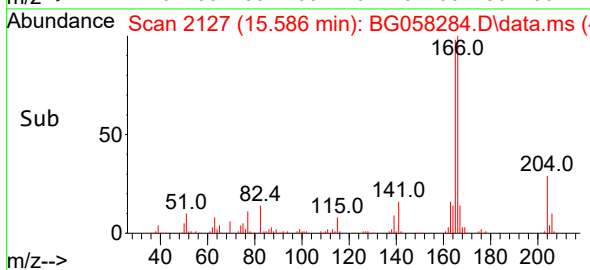

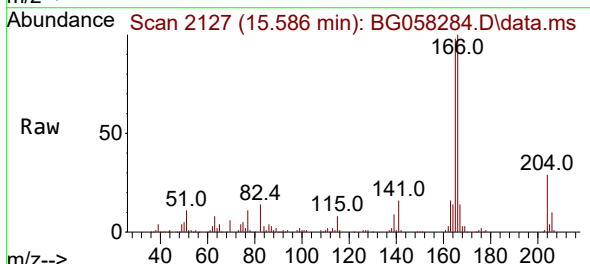




#62
4-Chlorophenyl-phenylether
Concen: 10.193 ng/ul
RT: 15.574 min Scan# 2125
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:204 Resp: 58701
Ion Ratio Lower Upper
204 100
206 34.5 26.0 39.0
141 53.7 42.2 63.2



#63
4-Nitroaniline
Concen: 6.084 ng/ul
RT: 15.603 min Scan# 2130
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:138 Resp: 10962
Ion Ratio Lower Upper
138 100
92 59.2 45.0 67.4
108 85.1 60.8 91.2



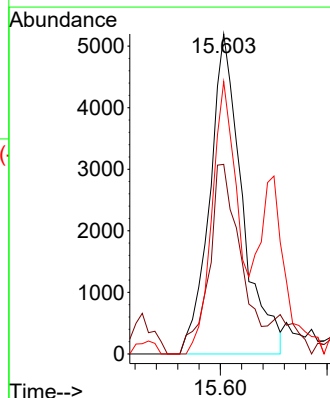





#66
 4,6-Dinitro-2-methylphenol
 Concen: 8.463 ng/ul
 RT: 15.662 min Scan# 2140
 Delta R.T. -0.004 min
 Lab File: BG058284.D
 Acq: 17 Jul 2023 15:52




Instrument :
 BNA_G
 ClientSampleId :
 SST010443


Tgt Ion:198 Resp: 17026
 Ion Ratio Lower Upper
 198 100
 182 4.1 3.4 5.2
 77 21.9 18.4 27.6

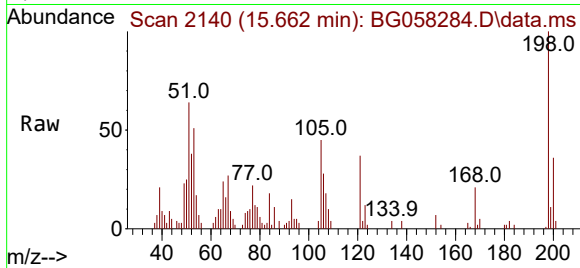

#67
 N-Nitrosodiphenylamine
 Concen: 9.894 ng/ul
 RT: 15.791 min Scan# 2162
 Delta R.T. 0.002 min
 Lab File: BG058284.D
 Acq: 17 Jul 2023 15:52

Tgt Ion:169 Resp: 95399
 Ion Ratio Lower Upper
 169 100
 168 69.3 55.7 83.5
 167 38.0 31.2 46.8



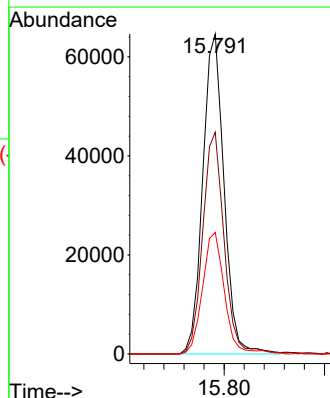
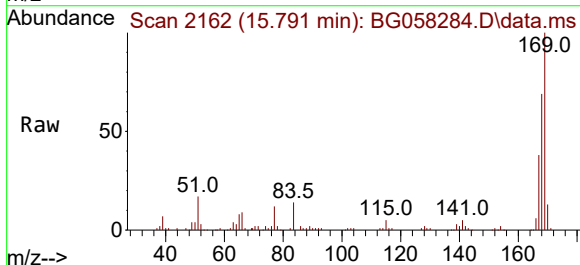




#68
4-Bromophenyl-phenylether
Concen: 10.027 ng/ul
RT: 16.467 min Scan# 21
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:248 Resp: 39876
Ion Ratio Lower Upper
248 100
250 92.3 73.8 110.6
141 60.4 48.2 72.2



#69
Hexachlorobenzene
Concen: 10.066 ng/ul
RT: 16.590 min Scan# 2298
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:284 Resp: 44821
Ion Ratio Lower Upper
284 100
142 27.5 20.5 30.7
249 29.7 25.2 37.8





#70

Atrazine

Concen: 9.798 ng/ul

RT: 16.731 min Scan# 21

Delta R.T. -0.004 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:200 Resp: 38633

Ion Ratio Lower Upper

200 100

173 27.1 19.8 29.8

215 45.7 36.2 54.4

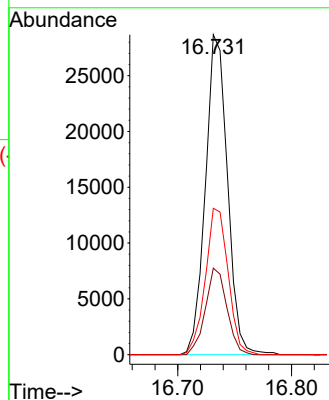

#71

Pentachlorophenol

Concen: 7.787 ng/ul

RT: 16.937 min Scan# 2357

Delta R.T. 0.008 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion:266 Resp: 20815


Ion Ratio Lower Upper

266 100

264 57.8 46.6 70.0

268 58.6 47.6 71.4

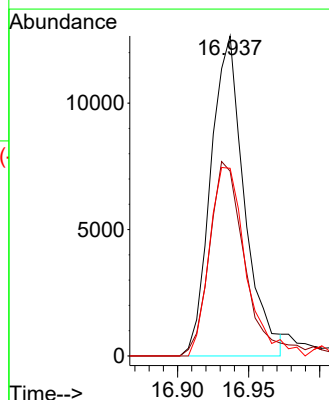



#72

Phenanthrene

Concen: 10.091 ng/ul

RT: 17.325 min Scan# 2423

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:178 Resp: 185963

Ion Ratio Lower Upper

178 100

179 15.9 11.9 17.9

176 19.9 15.8 23.8

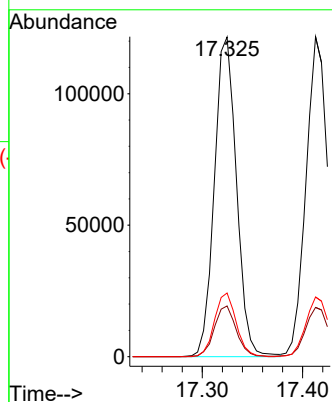

#74

Anthracene

Concen: 9.936 ng/ul

RT: 17.413 min Scan# 2438

Delta R.T. -0.004 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion:178 Resp: 185291


Ion Ratio Lower Upper

178 100

179 15.4 13.4 20.2

176 18.7 16.2 24.2









#75
1,2,3,4-Tetrachlorobenzene
Concen: 9.999 ng/uL
RT: 13.335 min Scan# 11
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:216 Resp: 48044
Ion Ratio Lower Upper
216 100
214 79.8 62.2 93.4
218 50.5 40.9 61.3

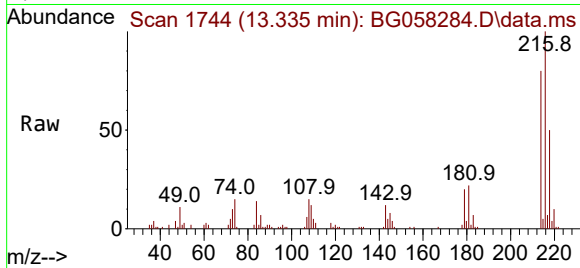

#76
Pentachlorobenzene
Concen: 9.992 ng/uL
RT: 14.857 min Scan# 2003
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:250 Resp: 51276
Ion Ratio Lower Upper
250 100
248 64.4 51.6 77.4
252 65.4 54.4 81.6



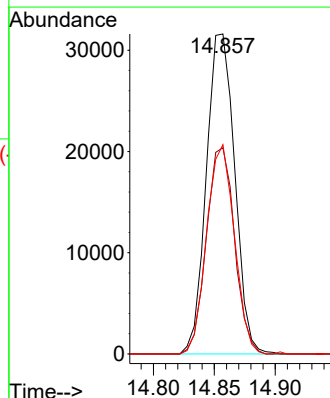
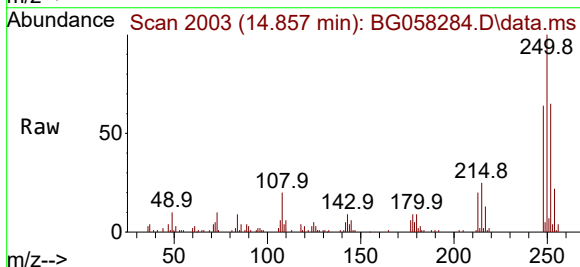




#77
 Carbazole
 Concen: 10.126 ng/ul
 RT: 17.683 min Scan# 2484
 Delta R.T. 0.002 min
 Lab File: BG058284.D
 Acq: 17 Jul 2023 15:52




Instrument :
 BNA_G
 ClientSampleId :
 SST010443


Tgt Ion:167 Resp: 170785
 Ion Ratio Lower Upper
 167 100
 166 23.4 17.8 26.8
 139 12.2 9.4 14.0

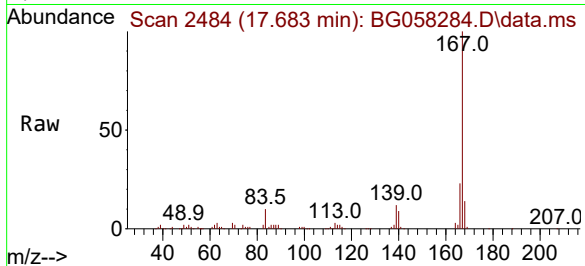

#78
 Di-n-butylphthalate
 Concen: 9.515 ng/ul
 RT: 18.235 min Scan# 2578
 Delta R.T. -0.004 min
 Lab File: BG058284.D
 Acq: 17 Jul 2023 15:52

Tgt Ion:149 Resp: 204433
 Ion Ratio Lower Upper
 149 100
 150 9.4 7.2 10.8
 104 4.7 3.9 5.9




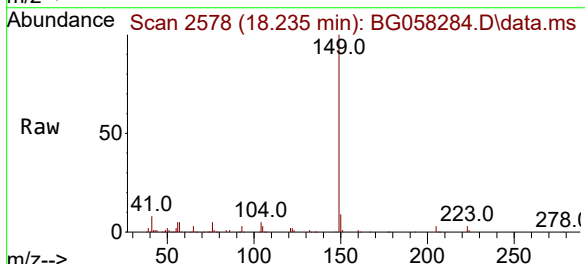


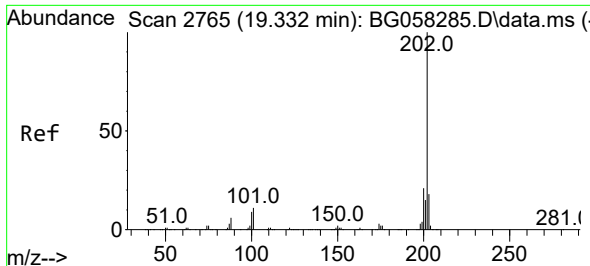

#80
Fluoranthene
Concen: 9.768 ng/ul
RT: 19.334 min Scan# 21
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:202 Resp: 227063
Ion Ratio Lower Upper
202 100
101 10.2 8.6 12.8
100 8.7 7.2 10.8

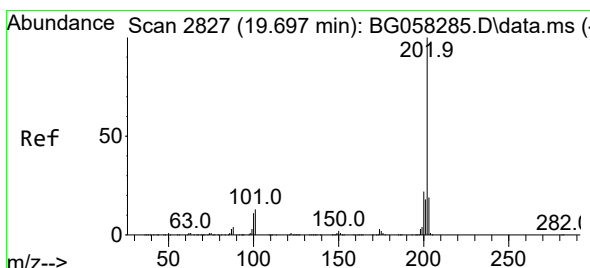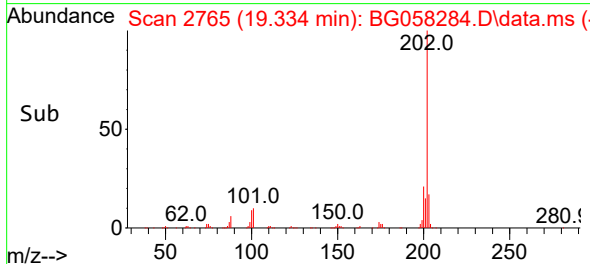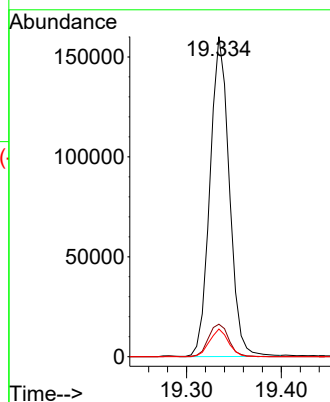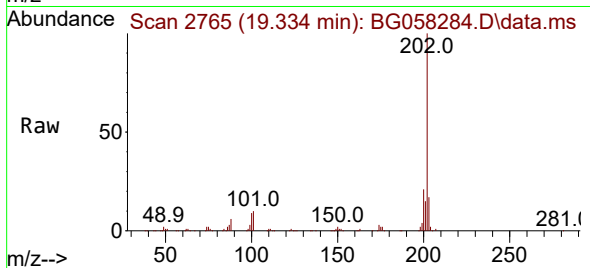

#82
Pyrene
Concen: 10.060 ng/ul
RT: 19.698 min Scan# 2827
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:202 Resp: 235398
Ion Ratio Lower Upper
202 100
101 12.1 10.2 15.2
100 10.8 8.9 13.3

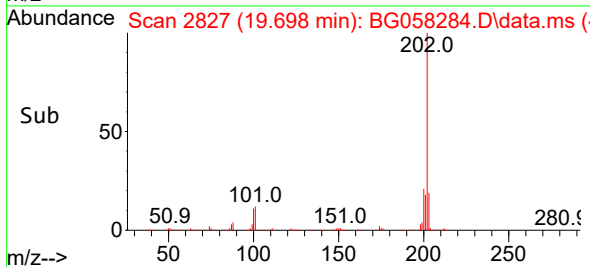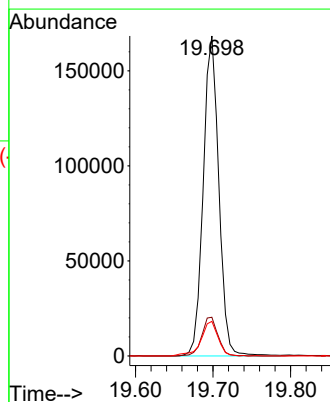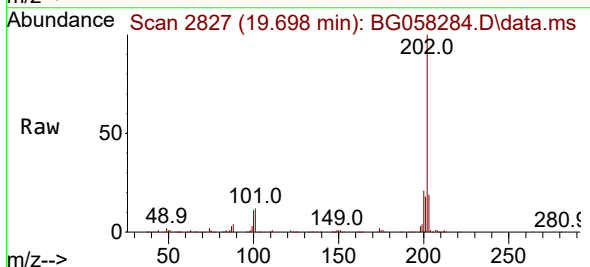



#83

Butylbenzylphthalate

Concen: 9.157 ng/ul

RT: 20.580 min Scan# 2977

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:149 Resp: 86882

Ion Ratio Lower Upper

149 100

91 71.4 59.9 89.9

206 19.7 16.9 25.3



#84

3,3'-Dichlorobenzidine

Concen: 9.677 ng/ul

RT: 21.432 min Scan# 3122

Delta R.T. 0.002 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion:252 Resp: 74624


Ion Ratio Lower Upper

252 100

254 65.1 50.5 75.7

126 9.2 6.5 9.7









#85
Benzo(a)anthracene
Concen: 9.763 ng/ul
RT: 21.508 min Scan# 3136
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:228 Resp: 223292
Ion Ratio Lower Upper
228 100
229 19.0 15.7 23.5
226 27.4 21.8 32.8

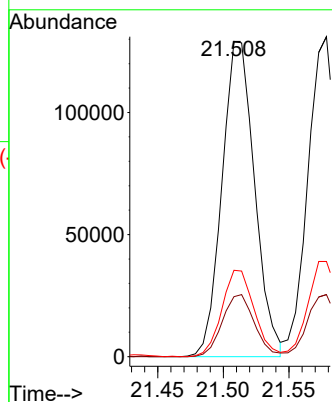

#86
Bis(2-ethylhexyl)phthalate
Concen: 9.288 ng/ul
RT: 21.414 min Scan# 3119
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:149 Resp: 126286
Ion Ratio Lower Upper
149 100
167 26.6 21.6 32.4
279 3.5 3.0 4.4



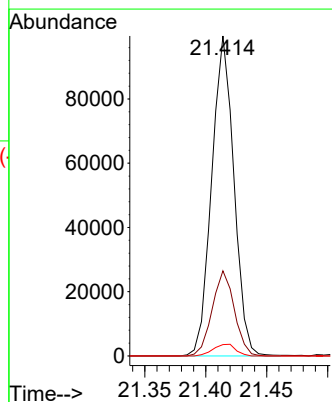





#87
Chrysene
Concen: 10.043 ng/ul
RT: 21.579 min Scan# 3147
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:228 Resp: 215318
Ion Ratio Lower Upper
228 100
226 29.7 24.0 36.0
229 19.4 15.8 23.8



#89
Di-n-octyl phthalate
Concen: 9.388 ng/ul
RT: 22.589 min Scan# 3319
Delta R.T. 0.002 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:149 Resp: 213649









#90
Benzo(b)fluoranthene
Concen: 9.864 ng/ul
RT: 23.664 min Scan# 3503
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52




Instrument :
BNA_G
ClientSampleId :
SSTD010443


Tgt Ion:252 Resp: 226214
Ion Ratio Lower Upper
252 100
253 22.5 17.9 26.9
125 9.0 6.7 10.1

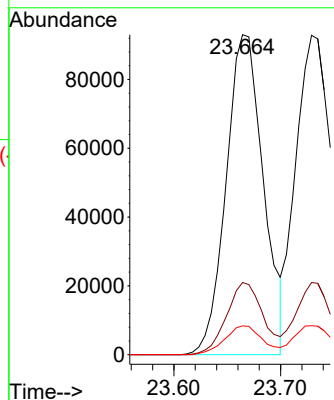

#91
Benzo(k)fluoranthene
Concen: 9.903 ng/ul
RT: 23.729 min Scan# 3513
Delta R.T. -0.004 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:252 Resp: 222600
Ion Ratio Lower Upper
252 100
253 22.6 18.3 27.5
125 9.1 7.4 11.0

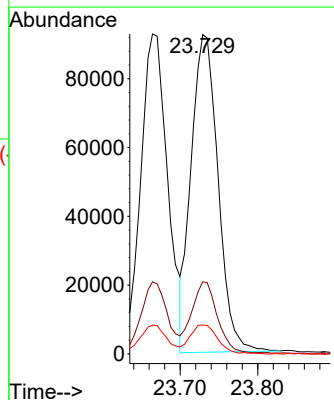



#93

Benzo(a)pyrene

Concen: 9.764 ng/ul

RT: 24.510 min Scan# 3

Delta R.T. -0.010 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52

Instrument :

BNA_G

ClientSampleId :

SSTD010443





Tgt Ion:252 Resp: 198187

Ion Ratio Lower Upper

252 100

253 21.3 17.4 26.0

125 8.4 7.7 11.5



#94

Indeno(1,2,3-cd)pyrene

Concen: 9.505 ng/ul

RT: 28.224 min Scan# 4278

Delta R.T. -0.004 min

Lab File: BG058284.D

Acq: 17 Jul 2023 15:52




Tgt Ion:276 Resp: 256186


Ion Ratio Lower Upper

276 100

138 17.3 13.8 20.6

277 25.3 19.2 28.8









#95
Dibenzo(a,h)anthracene
Concen: 9.565 ng/ul
RT: 28.282 min Scan# 41
Delta R.T. -0.010 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Instrument :
BNA_G
ClientSampleId :
SSTD010443

Tgt Ion:278 Resp: 212607
Ion Ratio Lower Upper
278 100
139 13.8 10.4 15.6
279 23.8 18.4 27.6

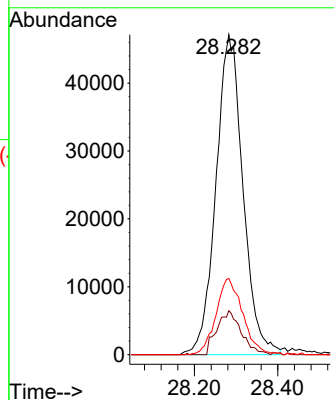

#96
Benzo(g,h,i)perylene
Concen: 9.475 ng/ul
RT: 29.340 min Scan# 4468
Delta R.T. -0.010 min
Lab File: BG058284.D
Acq: 17 Jul 2023 15:52

Tgt Ion:276 Resp: 208592
Ion Ratio Lower Upper
276 100
138 18.1 13.5 20.3
277 24.8 19.4 29.2

