
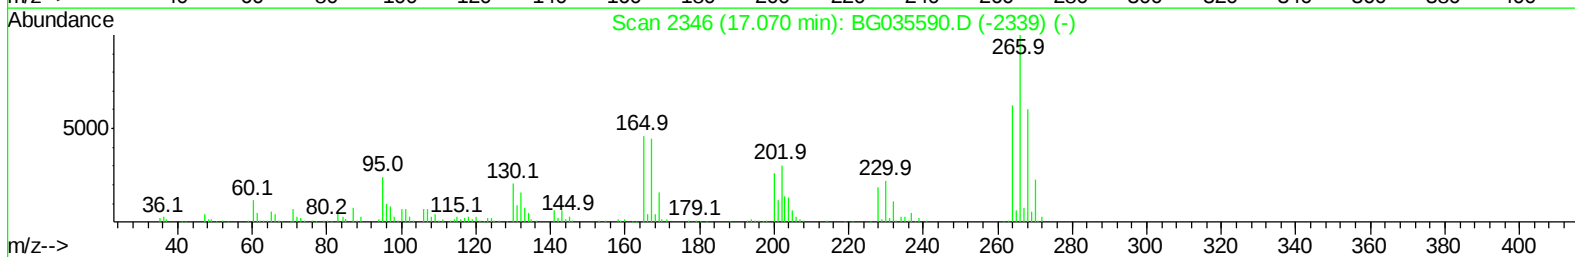
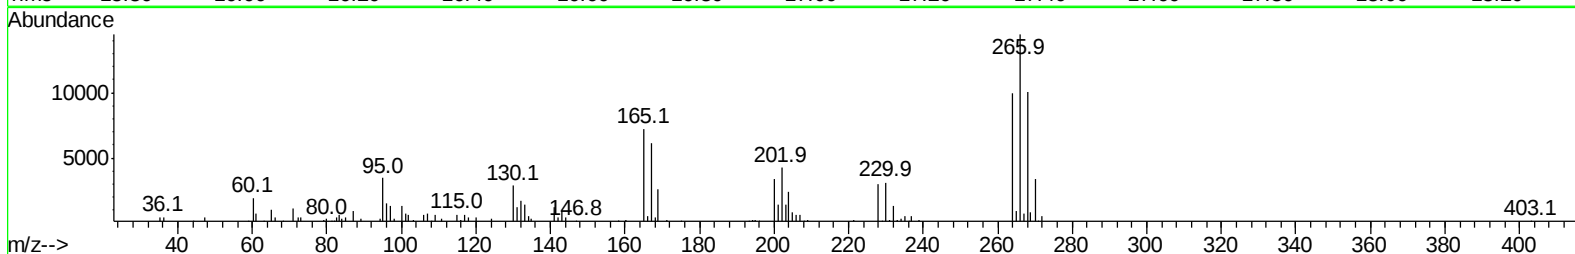


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071818\
Data File : BG035736.D
Acq On : 19 Jul 2018 3:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 05:01:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 17:45:13 2018
Response via : Initial Calibration

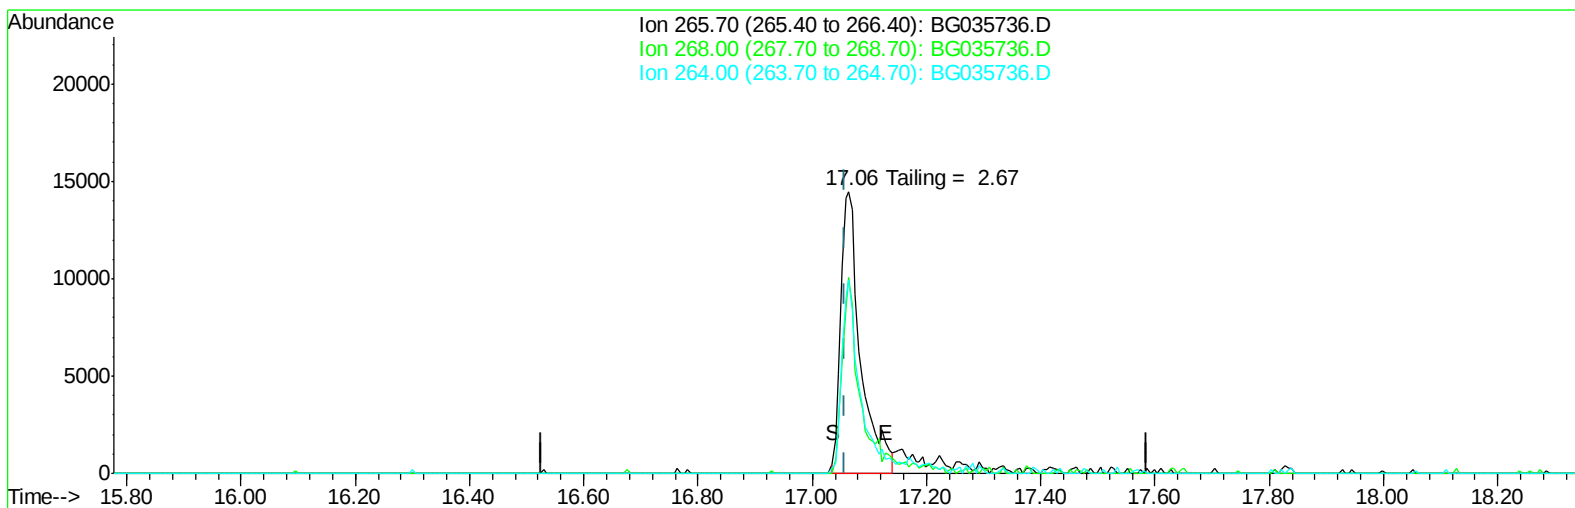

TIC: BG035736.D

(69) Pentachlorophenol (C)




17.064min (+0.006) 1280.86ng

response 35131

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.72
264.00	62.00	68.80
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071818\
Data File : BG035736.D
Acq On : 19 Jul 2018 3:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 19 05:01:27 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 17:45:13 2018
Response via : Initial Calibration

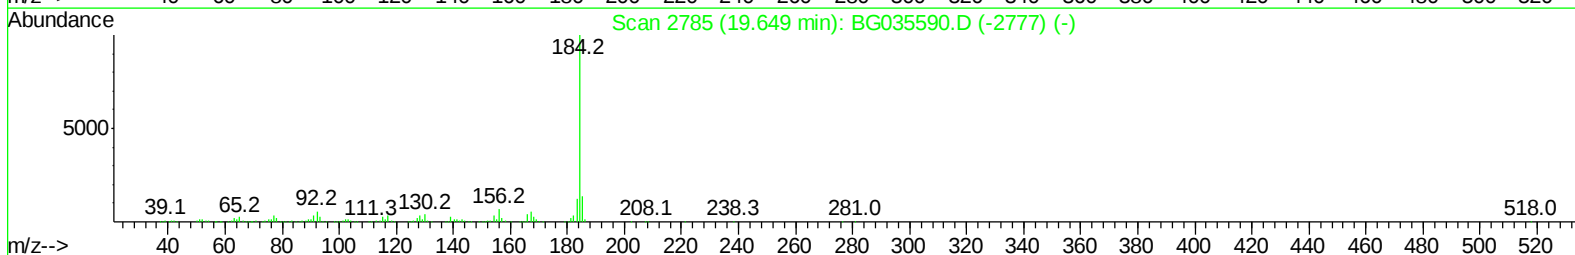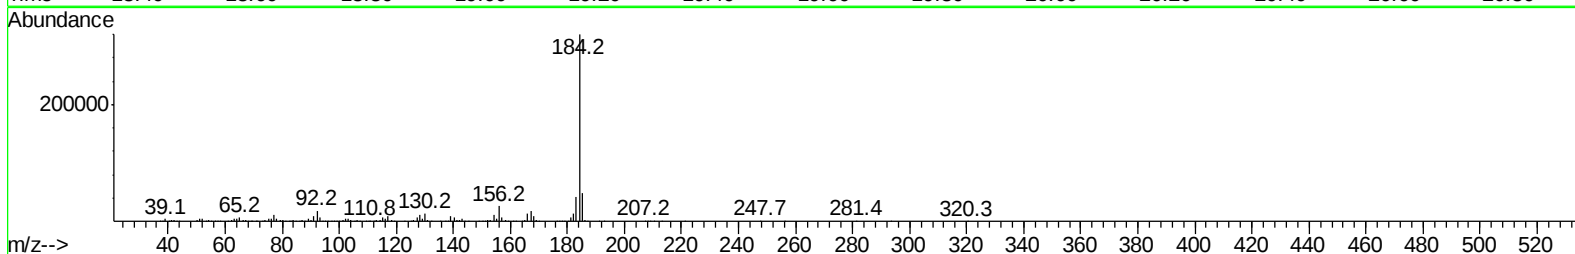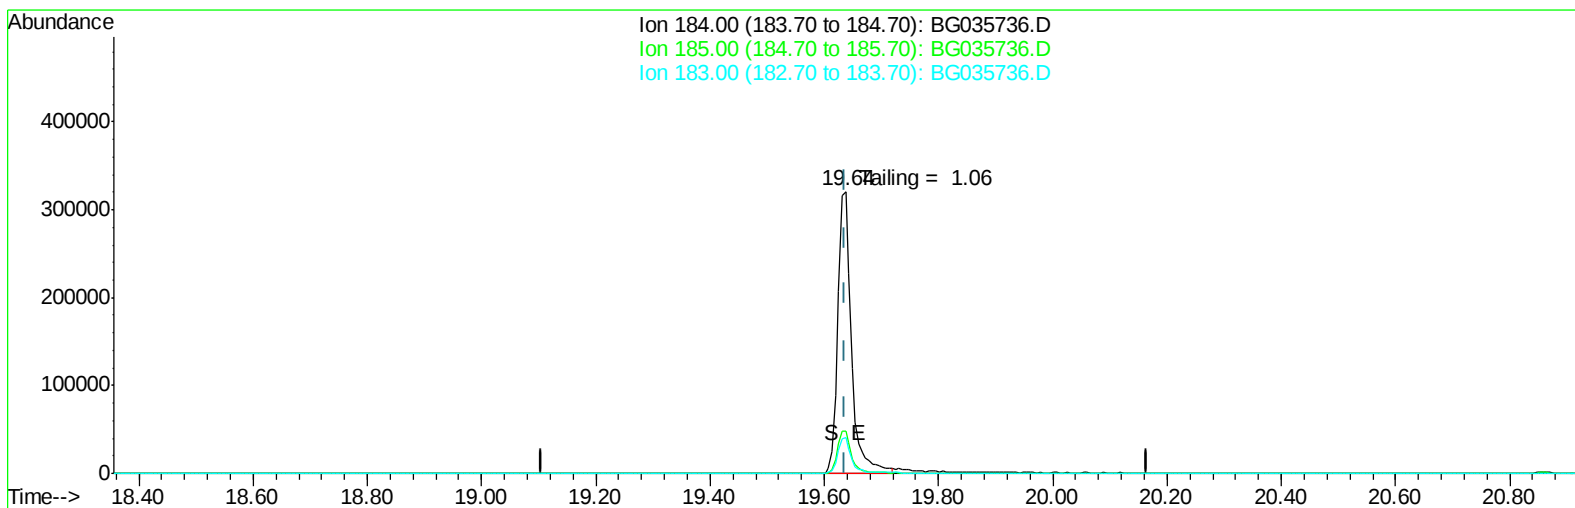

TIC: BG035736.D

(76) Benzidine

19.637min (+0.000) 4941.77ng

response 545536

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.87
183.00	13.30	12.81
0.00	0.00	0.00