

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071818\
 Data File : BG035726.D
 Acq On : 18 Jul 2018 20:51
 Operator : JU/SJ
 Sample : J4013-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-I-S

Quant Time: Jul 19 02:22:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 17:45:13 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	46313	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	170007	20.00	ng	0.00
38) Acenaphthene-d10	14.66	164	120993	20.00	ng	0.00
63) Phenanthrene-d10	17.40	188	335000	20.00	ng	0.00
75) Chrysene-d12	21.67	240	386765	20.00	ng	0.00
86) Perylene-d12	24.88	264	361235	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.63	112	357574	128.18	ng	0.00
7) Phenol-d6	7.21	99	457725	109.98	ng	0.00
23) Nitrobenzene-d5	9.20	82	360725	88.64	ng	0.00
41) 2,4,6-Tribromophenol	16.15	330	234045	146.76	ng	0.00
44) 2-Fluorobiphenyl	13.29	172	783438	86.75	ng	0.00
78) Terphenyl-d14	20.01	244	1673052	95.35	ng	0.00
Target Compounds						
31) Naphthalene	10.89	128	19806	2.236	ng	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071818\
Data File : BG035726.D
Acq On : 18 Jul 2018 20:51
Operator : JU/SJ
Sample : J4013-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-I-S

Quant Time: Jul 19 02:22:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 17:45:13 2018
Response via : Initial Calibration

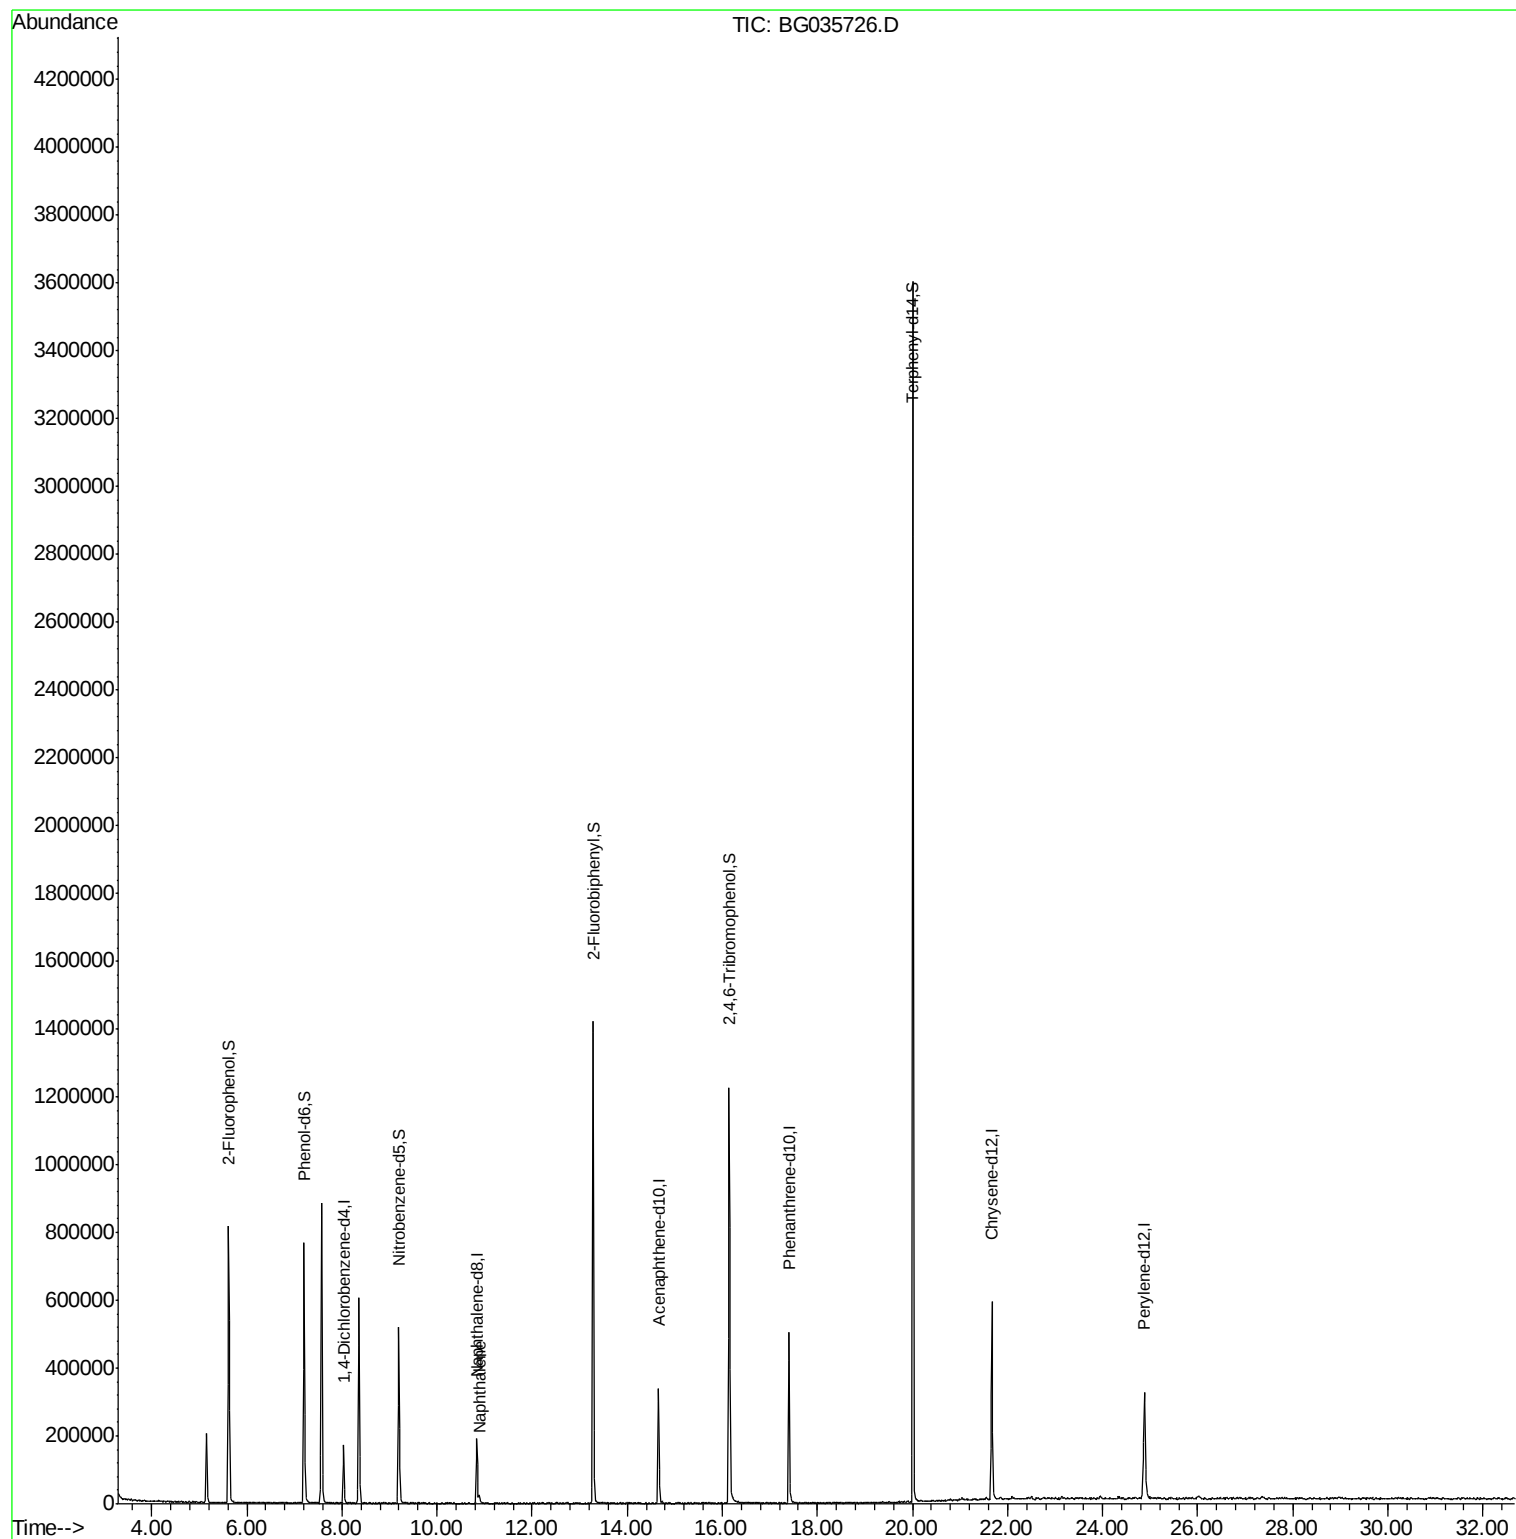

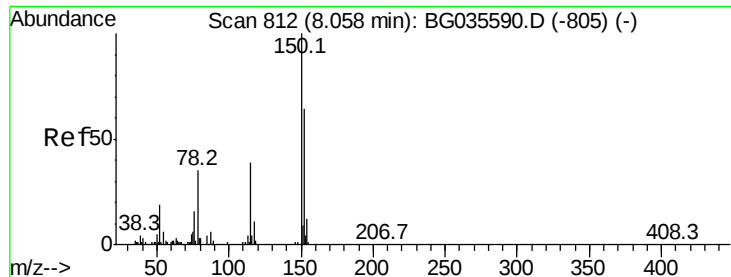


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 809
Delta R.T. -0.00 min
Lab File: BG035726.D
Acq: 18 Jul 2018 20:51

Instrument :
BNA_G
ClientSampleId :
TP-I-S

Tot Ion:152 Resp: 46313
Ion Ratio Lower Upper
152 100
150 152.2 126.6 189.8
115 62.3 53.0 79.4

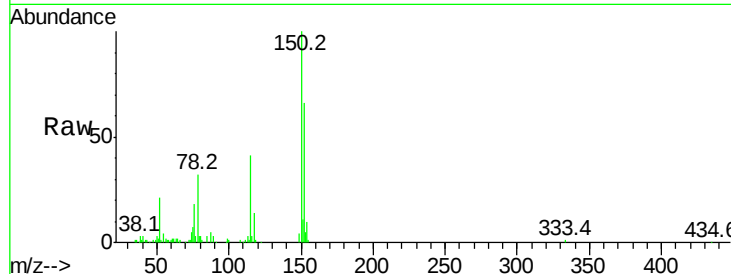


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

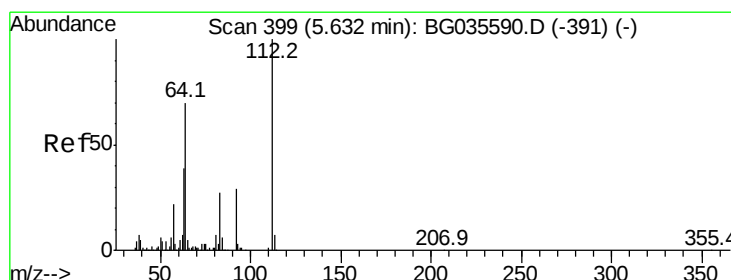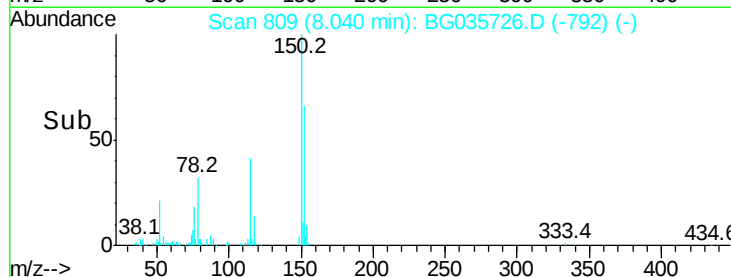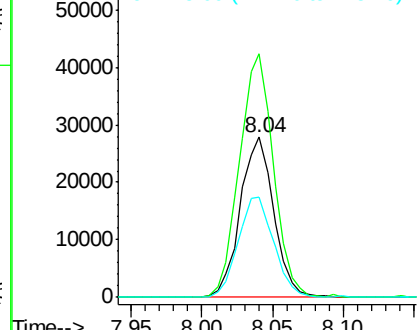



#5


2-Fluorophenol
Concen: 128.184 ng
RT: 5.63 min Scan# 398
Delta R.T. 0.01 min
Lab File: BG035726.D
Acq: 18 Jul 2018 20:51

Tgt Ion:112 Resp: 357574
Ion Ratio Lower Upper
112 100
64 63.4 56.3 84.5
63 34.7 30.1 45.1

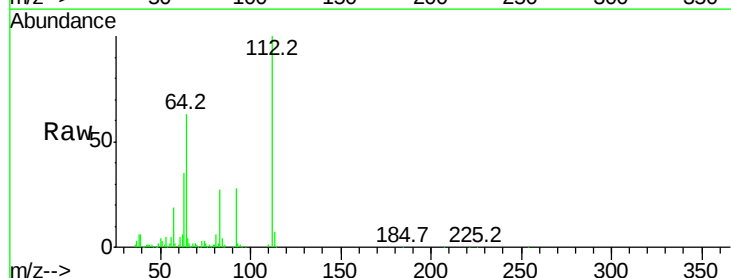

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

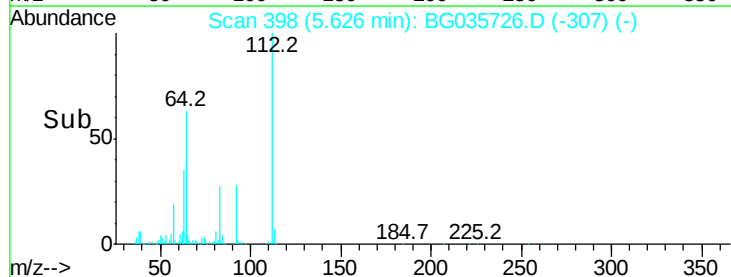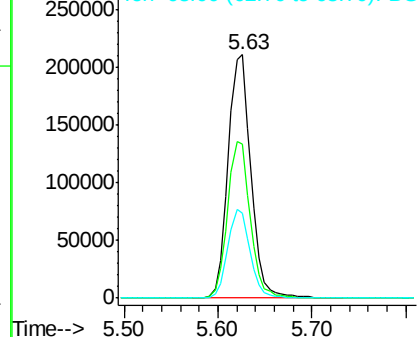

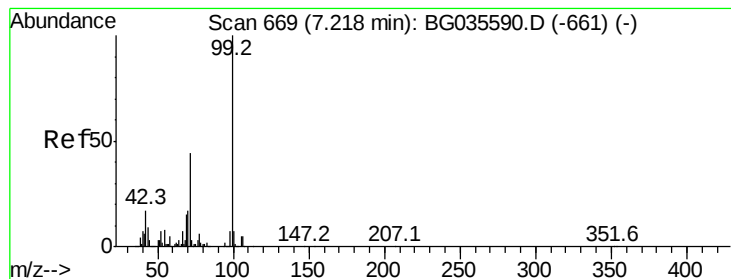

#7

Phenol-d6

Concen: 109.978 ng

RT: 7.21 min Scan# 667

Delta R.T. -0.00 min

Lab File: BG035726.D

Acq: 18 Jul 2018 20:51

Instrument :

BNA_G

ClientSampleId :

TP-I-S


Tot Ion: 99 Resp: 457725

Ion Ratio Lower Upper

99 100

42 16.5 14.1 21.1




71 42.7 26.1 39.1#

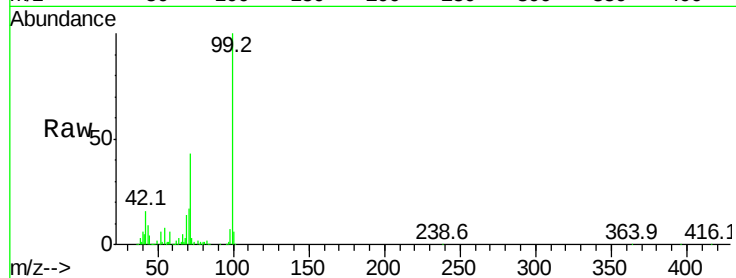

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

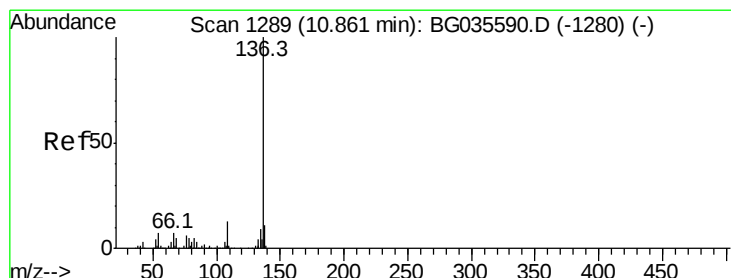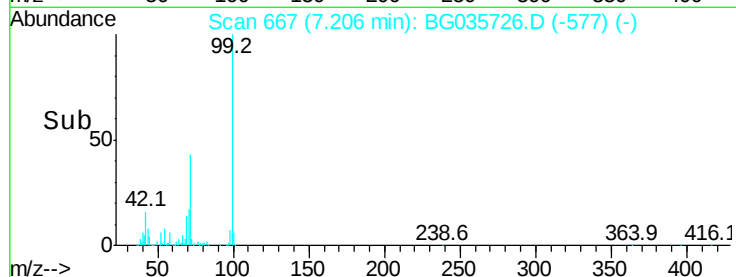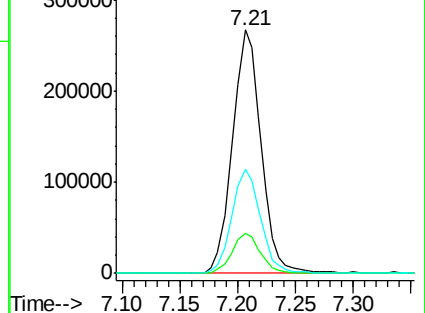

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.84 min Scan# 1286

Delta R.T. -0.00 min

Lab File: BG035726.D

Acq: 18 Jul 2018 20:51

Tgt Ion: 136 Resp: 170007


Ion Ratio Lower Upper

136 100

137 9.3 9.2 13.8

54 7.0 10.3 15.5#

68 4.3 4.5 6.7#


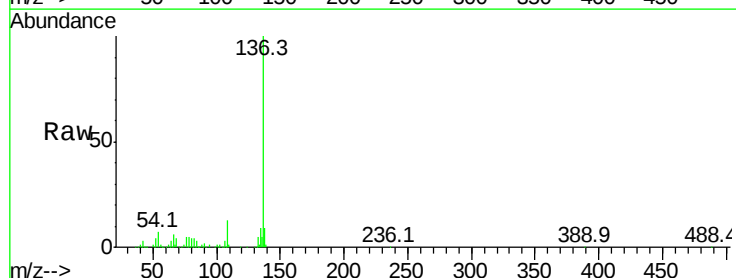


Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



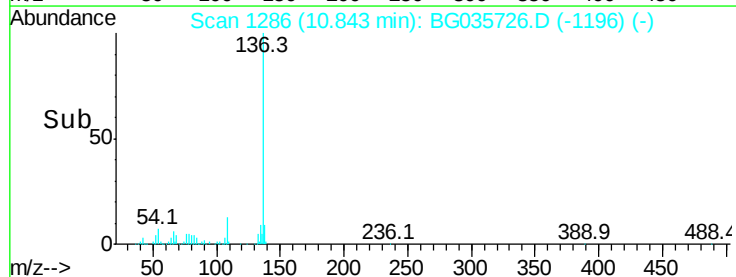
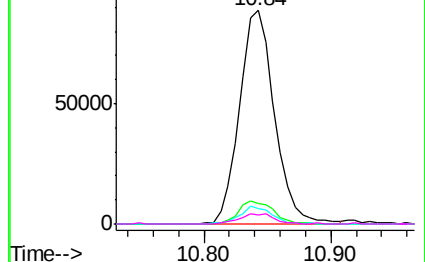




#23
 Nitrobenzene-d5
 Concen: 88.639 ng
 RT: 9.20 min Scan# 1006
 Delta R.T. -0.00 min
 Lab File: BG035726.D
 Acq: 18 Jul 2018 20:51




Instrument :
 BNA_G
 ClientSampleId :
 TP-I-S


Tot Ion	82	Resp	360725
Ion Ratio	Lower	Upper	
82	100		
128	33.5	29.7	44.5
54	44.4	43.1	64.7

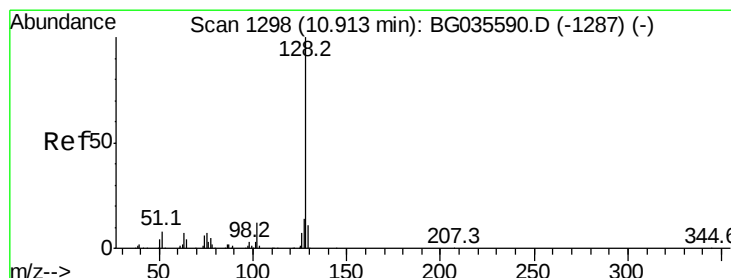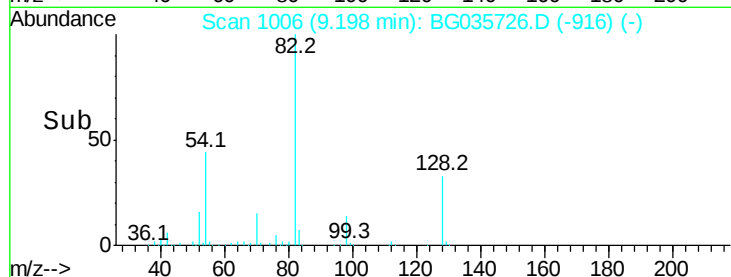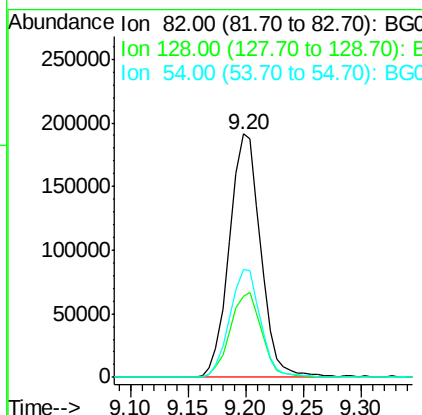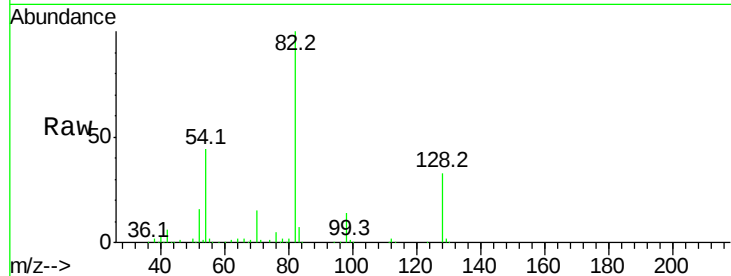

#31
 Naphthalene
 Concen: 2.236 ng
 RT: 10.89 min Scan# 1294
 Delta R.T. -0.00 min
 Lab File: BG035726.D
 Acq: 18 Jul 2018 20:51

Tgt Ion	128	Resp	19806
Ion Ratio	Lower	Upper	
128	100		
129	8.6	8.6	12.8
127	11.6	11.6	17.4

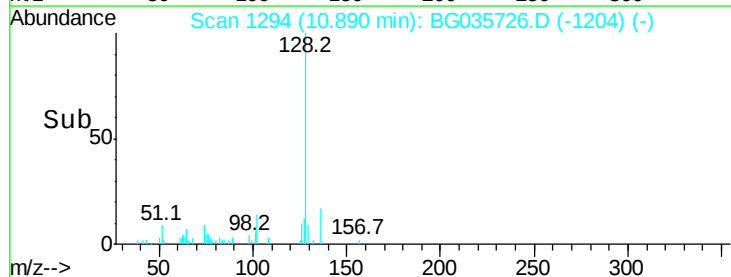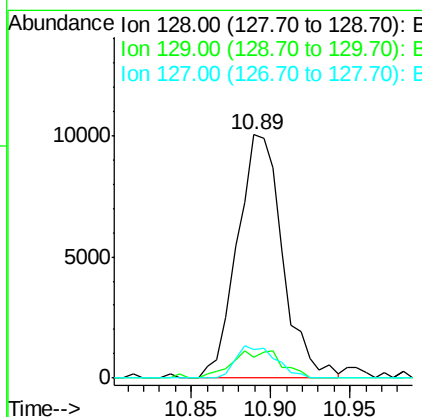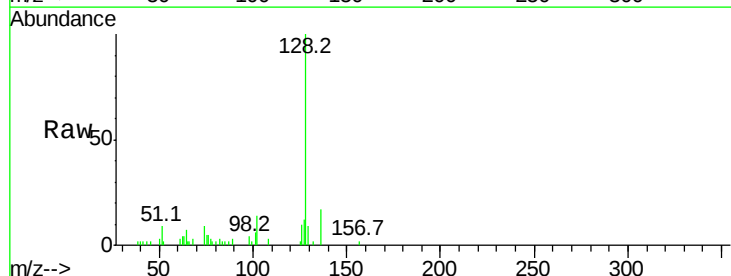

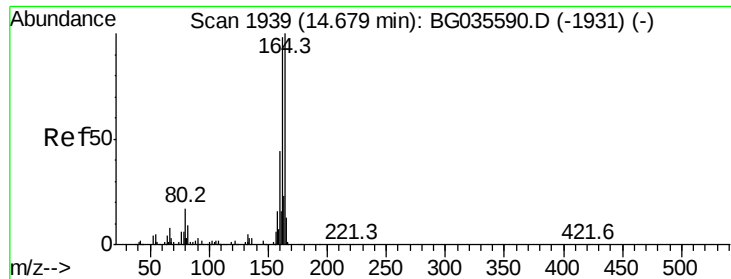

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.66 min Scan# 1936

Delta R.T. -0.00 min

Lab File: BG035726.D

Acq: 18 Jul 2018 20:51

Instrument :

BNA_G

ClientSampleId :

TP-I-S


Tot Ion:164 Resp: 120993

Ion Ratio Lower Upper

164 100

162 103.4 78.8 118.2




160 45.7 35.4 53.0

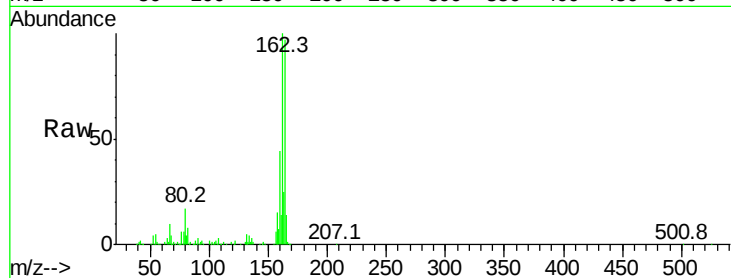

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

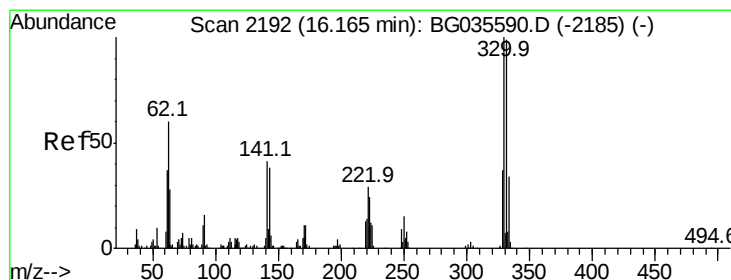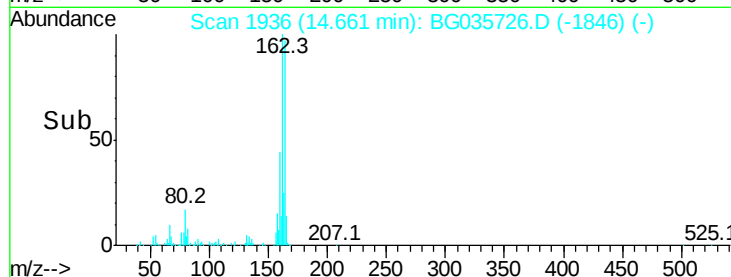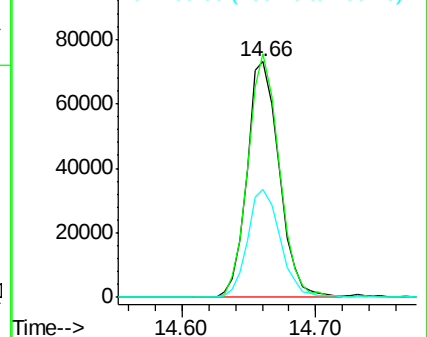

#41

2,4,6-Tribromophenol

Concen: 146.758 ng

RT: 16.15 min Scan# 2190

Delta R.T. -0.00 min

Lab File: BG035726.D

Acq: 18 Jul 2018 20:51


Tgt Ion:330 Resp: 234045

Ion Ratio Lower Upper

330 100

332 95.5 77.0 115.6



141 40.2 25.2 37.8#

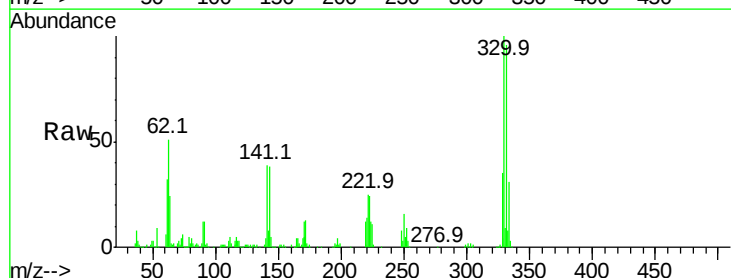


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



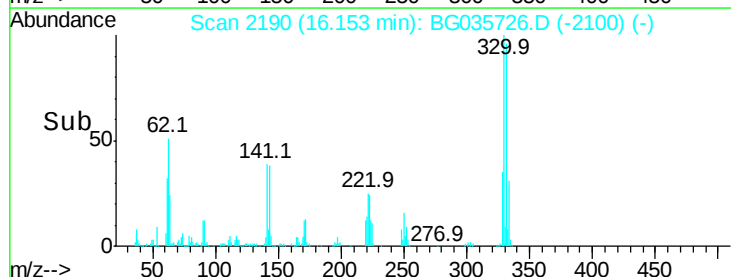
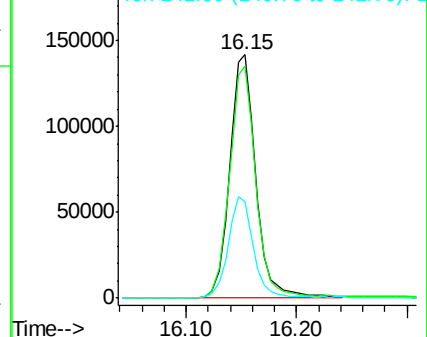


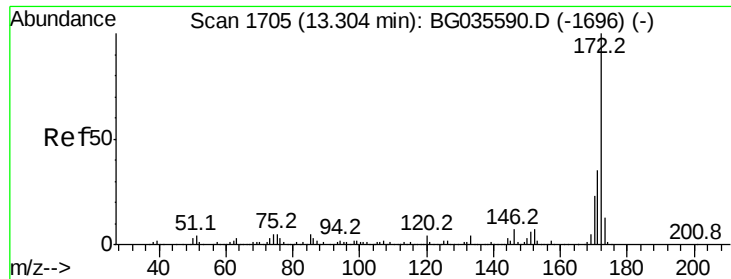

#44
2-Fluorobiphenyl
Concen: 86.749 ng
RT: 13.29 min Scan# 1702
Delta R.T. -0.00 min
Lab File: BG035726.D
Acq: 18 Jul 2018 20:51




Instrument :
BNA_G
ClientSampleId :
TP-I-S

Tot Ion:172 Resp: 783438
Ion Ratio Lower Upper
172 100
171 34.4 30.0 45.0
170 23.2 19.5 29.3

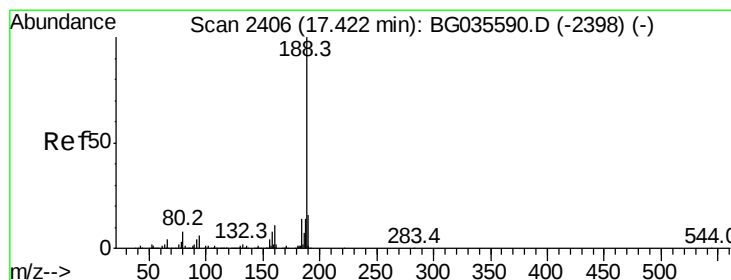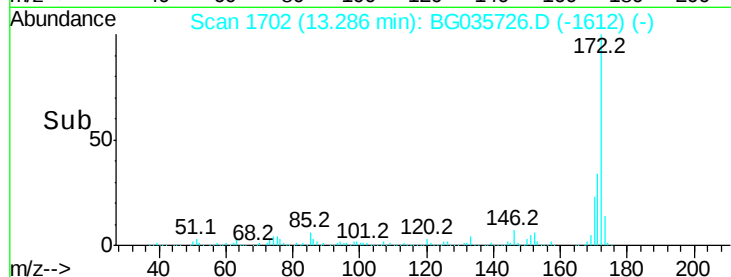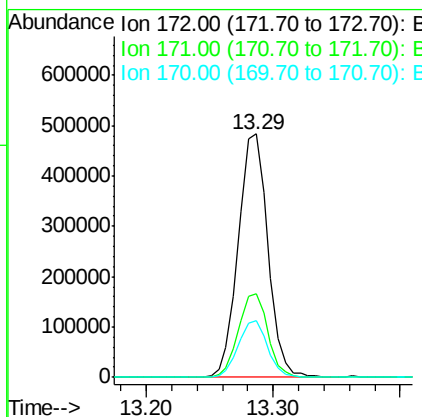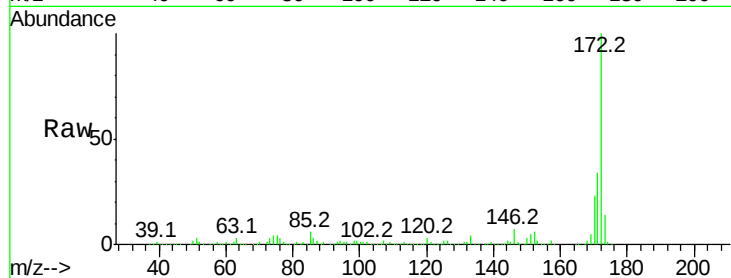

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.40 min Scan# 2403
Delta R.T. -0.00 min
Lab File: BG035726.D
Acq: 18 Jul 2018 20:51

Tgt Ion:188 Resp: 335000
Ion Ratio Lower Upper
188 100
94 6.4 6.9 10.3#
80 7.9 7.7 11.5

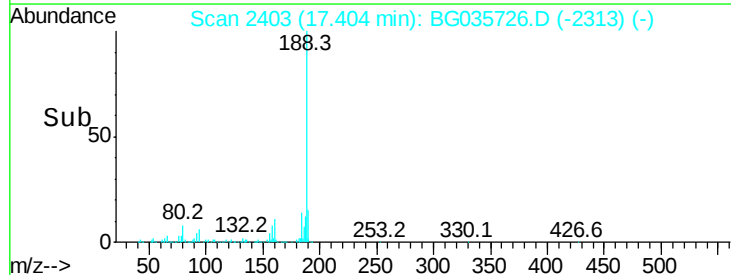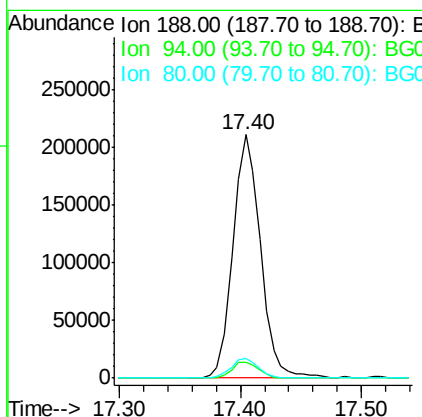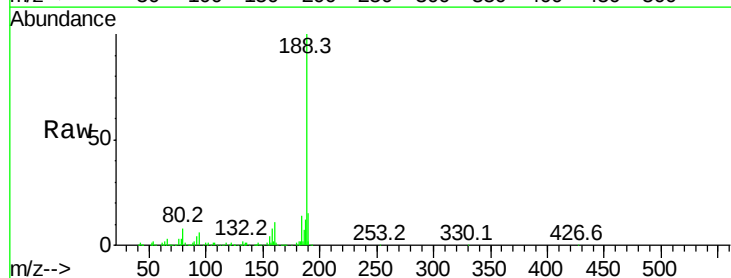



#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.67 min Scan# 3129

Delta R.T. -0.01 min

Lab File: BG035726.D

Acq: 18 Jul 2018 20:51

Instrument :

BNA_G

ClientSampleId :

TP-I-S


Tot Ion:240 Resp: 386765

Ion Ratio Lower Upper

240 100

120 6.5 6.8 10.2#




236 25.7 20.9 31.3

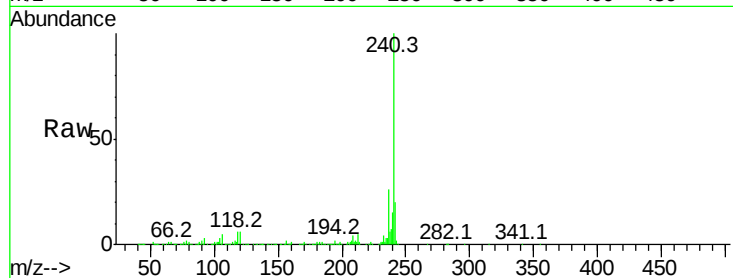

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

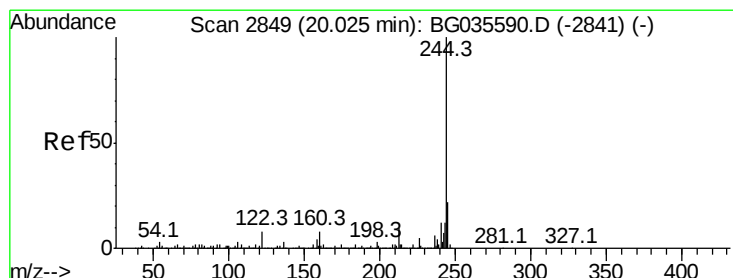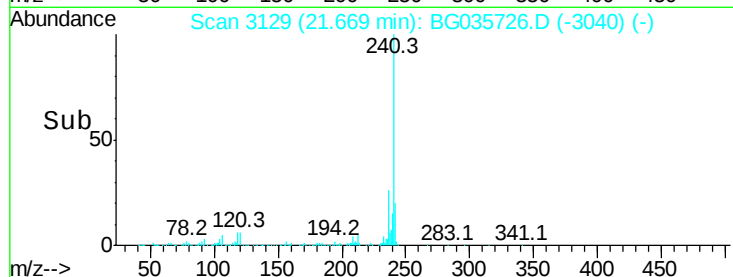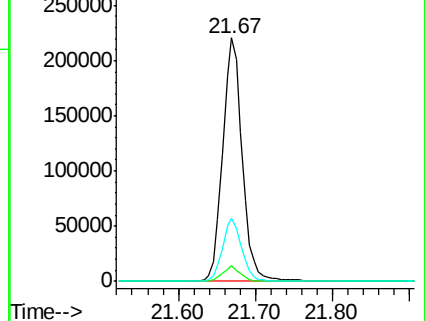

#78

Terphenyl-d14

Concen: 95.353 ng

RT: 20.01 min Scan# 2847

Delta R.T. -0.00 min

Lab File: BG035726.D

Acq: 18 Jul 2018 20:51


Tgt Ion:244 Resp: 1673052

Ion Ratio Lower Upper

244 100

212 9.7 5.8 8.8#



122 7.1 7.0 10.4

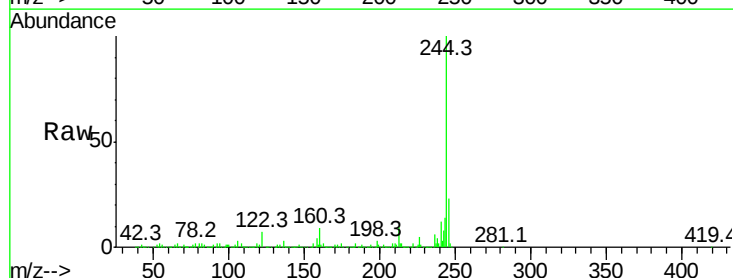


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

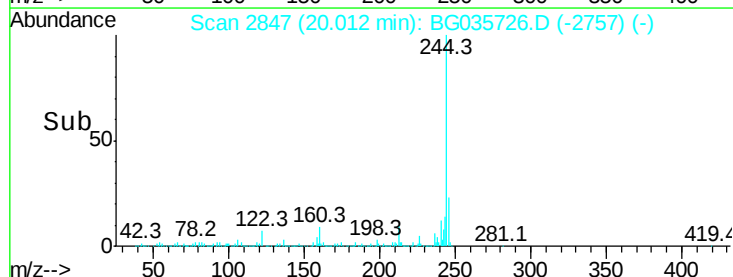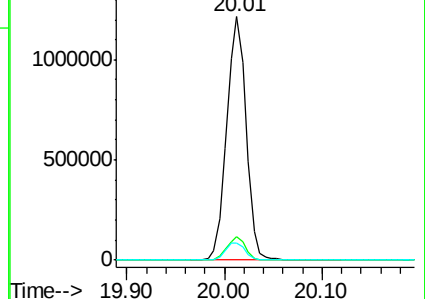

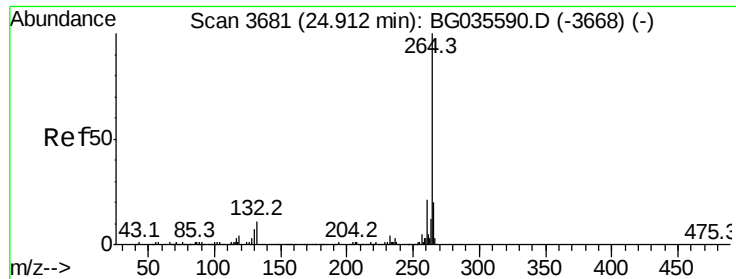

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 24.88 min Scan# 3676
 Delta R.T. -0.00 min
 Lab File: BG035726.D
 Acq: 18 Jul 2018 20:51

Instrument :
 BNA_G
 ClientSampleId :
 TP-I-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.1	17.4	26.0
265	21.4	17.7	26.5

