


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071818\
 Data File : BG035718.D
 Acq On : 18 Jul 2018 15:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

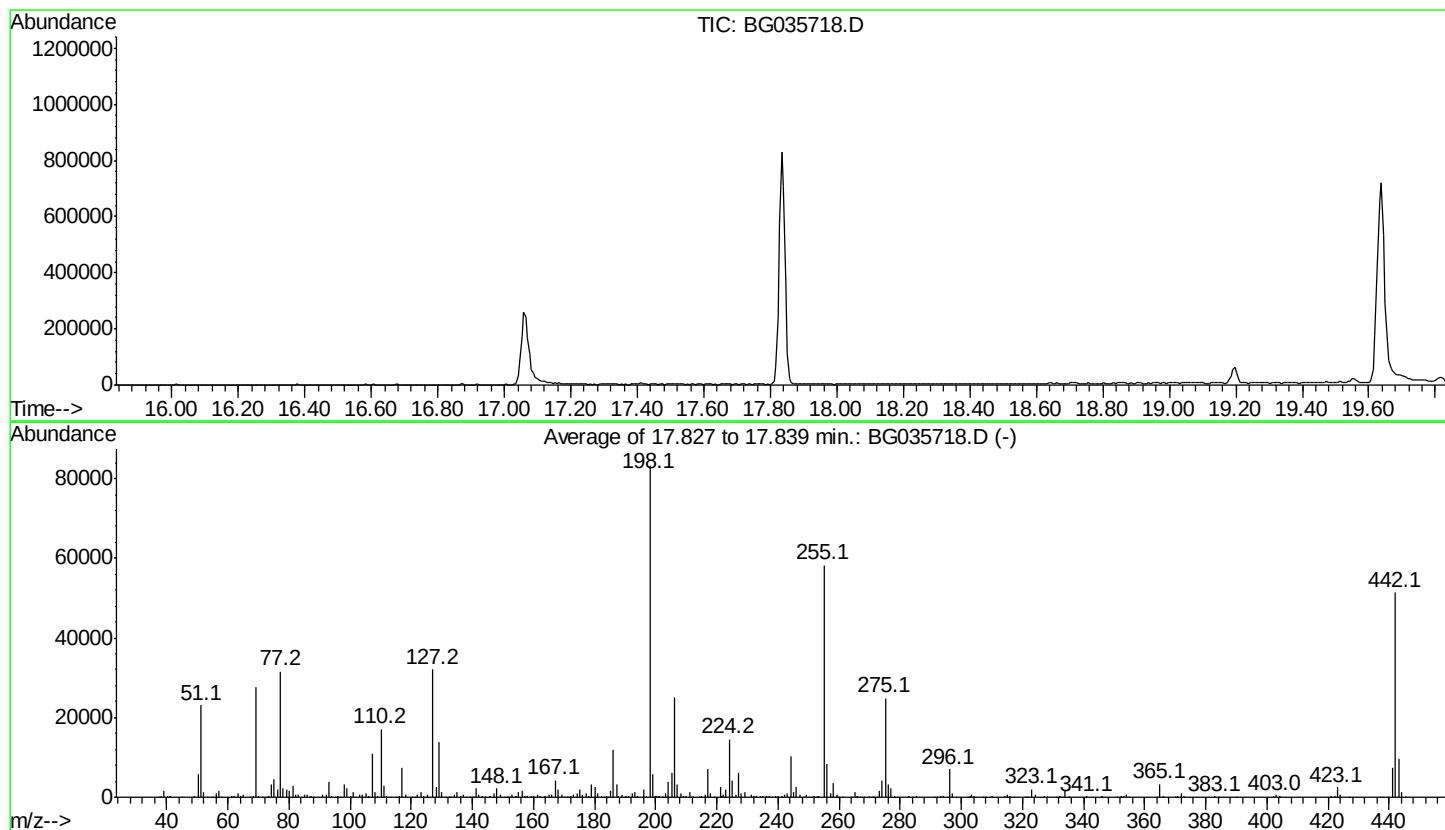

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.8	23117	PASS
68	69	0.00	2	1.4	376	PASS
69	198	0.00	100	33.1	27581	PASS
70	69	0.00	2	1.4	381	PASS
127	198	10	80	38.6	32117	PASS
197	198	0.00	2	0.4	337	PASS
198	198	100	100	100.0	83256	PASS
199	198	5	9	7.1	5875	PASS
275	198	10	60	29.9	24880	PASS
365	198	1	100	3.9	3234	PASS
441	198	0.01	100	8.9	7432	PASS
442	198	50	100	61.7	51394	PASS
443	442	15	24	18.8	9655	PASS