

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016334.D
 Acq On : 19 Jul 2023 21:02
 Operator : MA/JU
 Sample : 03472-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A46R1

Quant Time: Jul 19 22:43:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	74108	20.000	ng/ul	0.00
20) Naphthalene-d8	10.781	136	360227	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.604	164	251483	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.369	188	610510	20.000	ng/ul	0.00
79) Chrysene-d12	21.469	240	712689	20.000	ng/ul	0.00
88) Perylene-d12	23.951	264	809094	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	8183	3.907	ng/uL	0.00
4) Pyridine-d5	3.752	84	50317	9.634	ng/ul	0.03
7) Phenol-d5	7.175	99	135797	20.287	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.293	67	83798	18.514	ng/ul	0.02
11) 2-Chlorophenol-d4	7.499	132	109356	22.631	ng/ul	0.02
15) 4-Methylphenol-d8	8.669	113	33	0.006	ng/ul	-0.02
21) Nitrobenzene-d5	9.181	128	52077	20.955	ng/ul	0.05
24) 2-Nitrophenol-d4	9.916	143	52661	18.592	ng/ul	0.05
28) 2,4-Dichlorophenol-d3	10.528	165	95024	19.373	ng/ul	0.11
31) 4-Chloroaniline-d4	11.093	131	10878	1.384	ng/ul	0.15
46) Dimethylphthalate-d6	14.034	166	510184	26.595	ng/ul	0.02
49) Acenaphthylene-d8	14.304	160	534367	25.418	ng/ul	0.01
54) 4-Nitrophenol-d4	14.887	143	25	0.006	ng/ul	-0.04
60) Fluorene-d10	15.616	176	460358	28.674	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.828	200	46877	13.301	ng/ul	0.05
73) Anthracene-d10	17.481	188	543518	20.353	ng/ul	0.01
81) Pyrene-d10	19.704	212	1011585	27.354	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.786	264	756212	19.462	ng/ul	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.781	70	8997	1.887 ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016334.D
Acq On : 19 Jul 2023 21:02
Operator : MA/JU
Sample : 03472-20
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A46R1


Quant Time: Jul 19 22:43:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

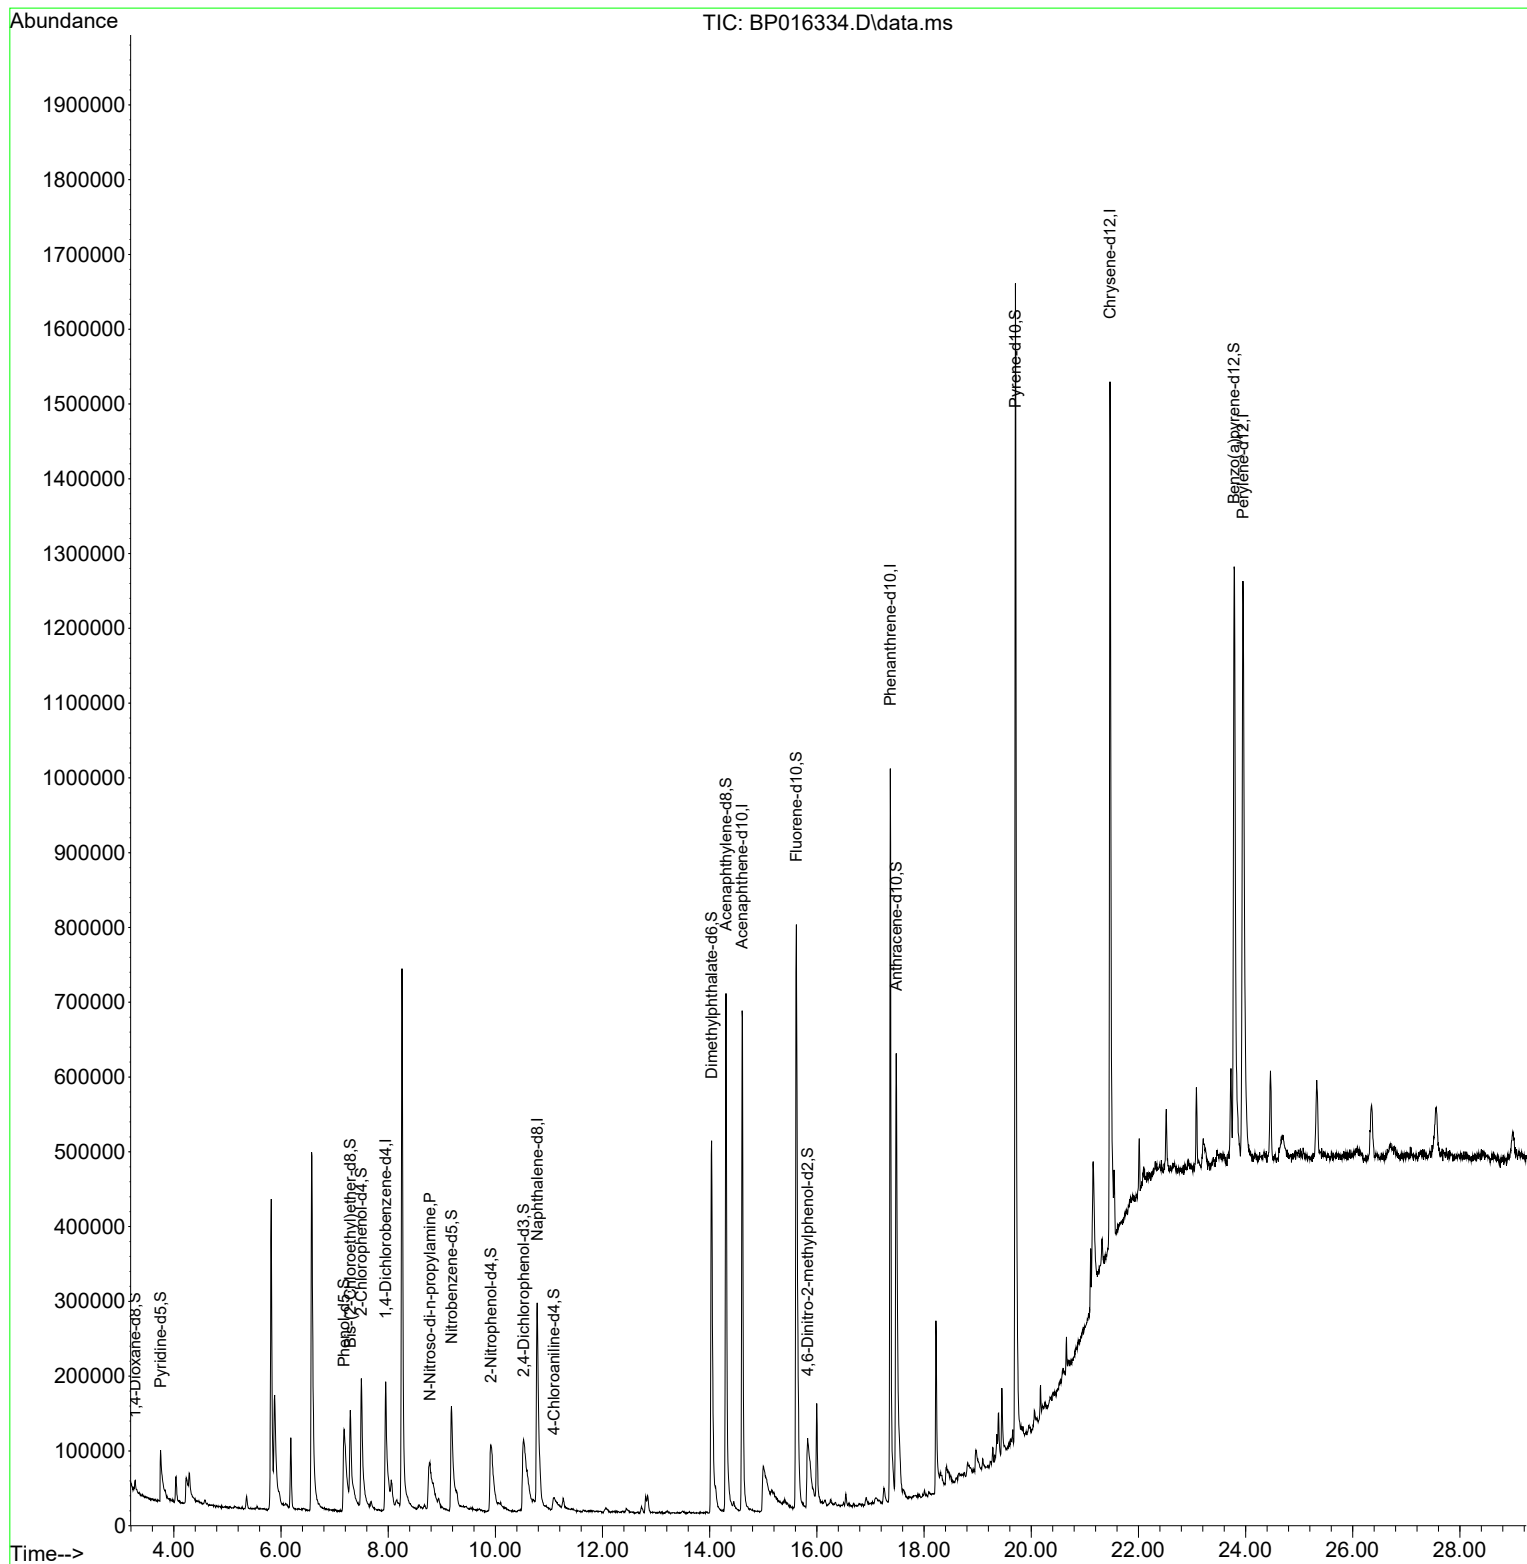

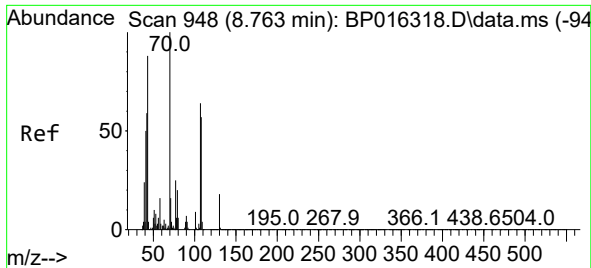

#17
N-Nitroso-di-n-propylamine
Concen: 1.887 ng/ul
RT: 8.781 min Scan# 91
Delta R.T. 0.018 min
Lab File: BP016334.D
Acq: 19 Jul 2023 21:02

Instrument :
BNA_G
ClientSampleId :
A46R1

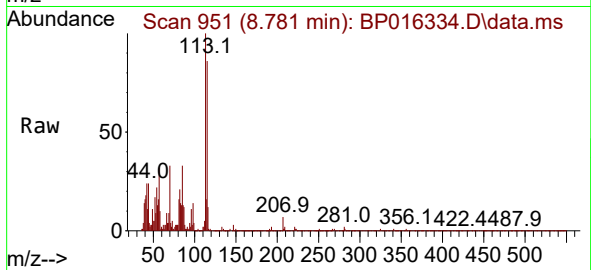

Tgt Ion:	70	Resp:	8997
Ion	Ratio	Lower	Upper
70	100		
42	71.7	50.8	76.2
101	0.8	7.0	10.6#
130	0.0	13.3	19.9#

