




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
 Data File : BG058302.D
 Acq On : 18 Jul 2023 15:39
 Operator : CG/JU
 Sample : PB154044BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK044

Manual IntegrationsAPPROVED

Quant Time: Jul 19 04:17:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :Sohil Jodhani 07/19/2023

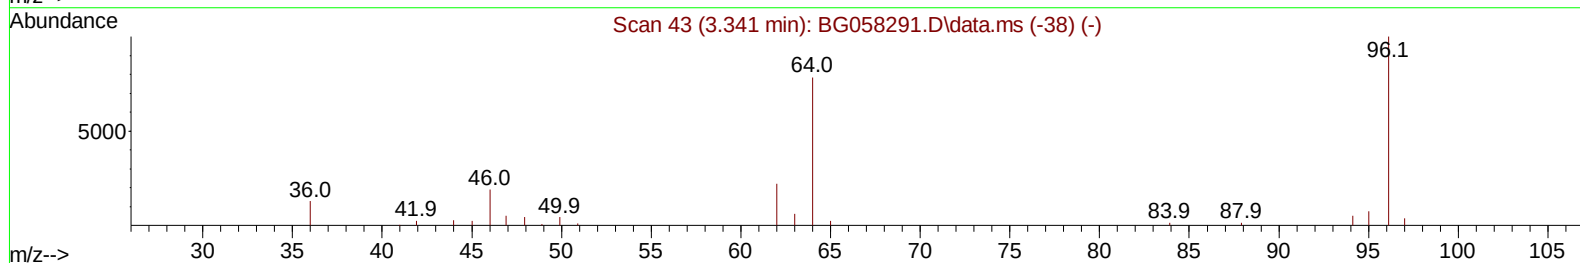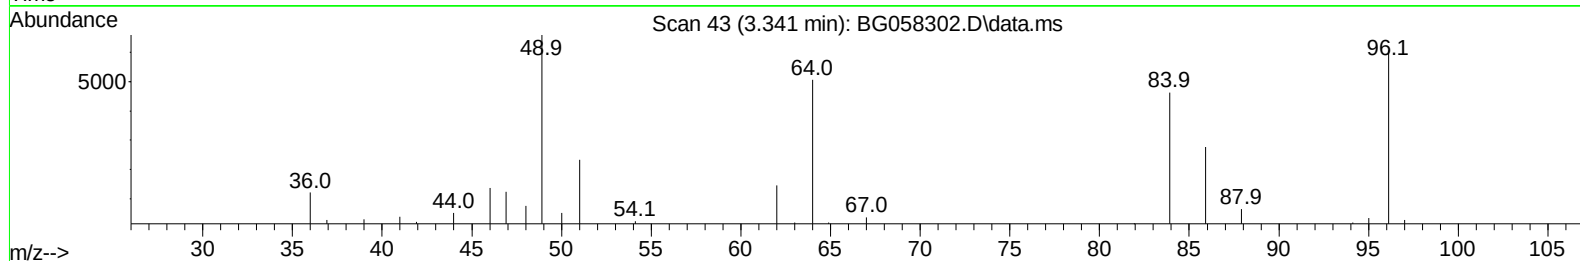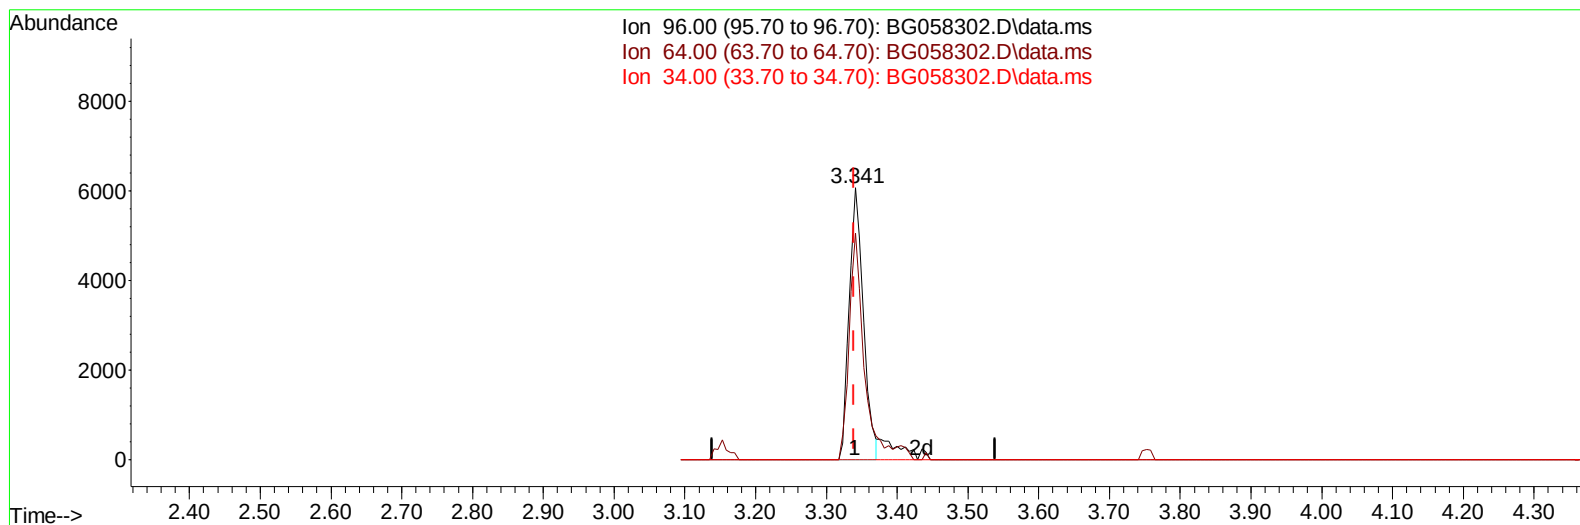

TIC: BG058302.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.341min (+ 0.002) 8.06 ng/uL

response 8494

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	91.80	83.46
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
 Data File : BG058302.D
 Acq On : 18 Jul 2023 15:39
 Operator : CG/JU
 Sample : PB154044BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK044

Manual IntegrationsAPPROVED

Quant Time: Jul 19 04:17:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :Sohil Jodhani 07/19/2023

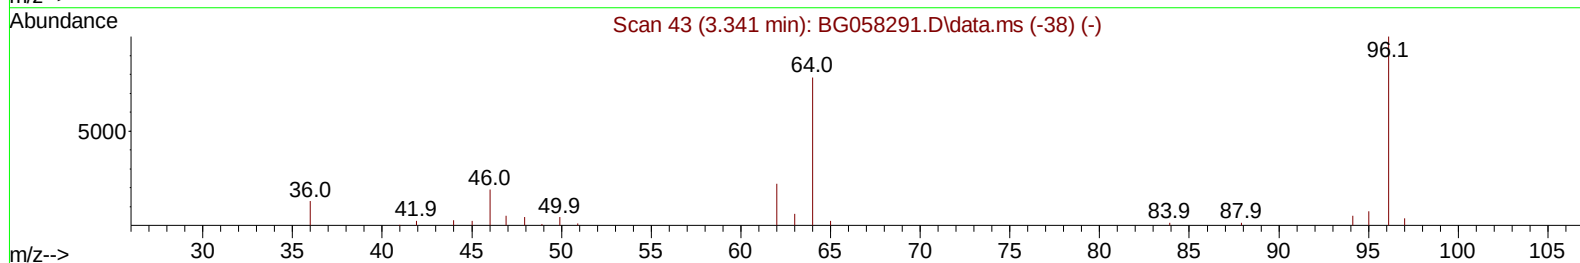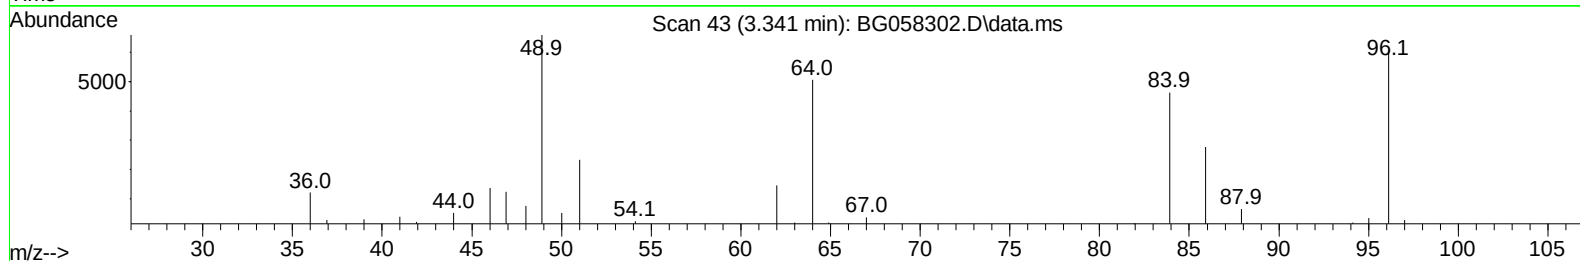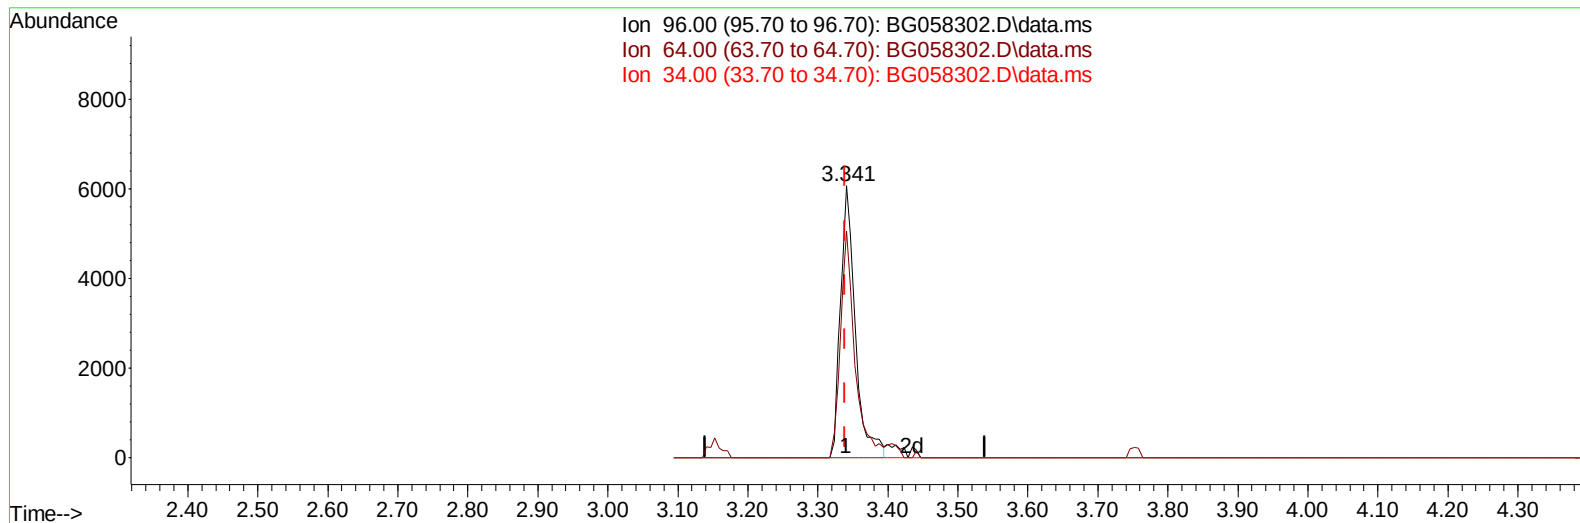

TIC: BG058302.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.341min (+ 0.002) 8.57 ng/uL m

response 9028

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	91.80	83.46
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
 Data File : BG058302.D
 Acq On : 18 Jul 2023 15:39
 Operator : CG/JU
 Sample : PB154044BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK044

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/19/2023
 Supervised By :Sohil Jodhani 07/19/2023

Quant Time: Jul 19 04:49:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.900	152		38790	20.000	ng/ul	0.00
20) Naphthalene-d8	10.697	136		187253	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164		141508	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.278	188		363660	20.000	ng/ul	0.00
79) Chrysene-d12	21.525	240		314024	20.000	ng/ul	0.00
88) Perylene-d12	24.663	264		376860	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.341	96		9028m	8.566	ng/uL	0.00
4) Pyridine-d5	3.752	84		128310	41.018	ng/ul	0.00
7) Phenol-d5	7.060	99		160932	43.735	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.225	67		98682	42.907	ng/ul	0.00
11) 2-Chlorophenol-d4	7.430	132		113266	43.973	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113		120083	42.783	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128		58369	41.586	ng/ul	0.00
24) 2-Nitrophenol-d4	9.780	143		66942	43.687	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.321	165		115724	39.397	ng/ul	0.00
31) 4-Chloroaniline-d4	10.838	131		162665	38.200	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166		421607	38.637	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160		458454	40.091	ng/ul	0.00
54) 4-Nitrophenol-d4	14.733	143		69161	41.968	ng/ul	0.00
60) Fluorene-d10	15.527	176		375660	41.582	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.644	200		71772	38.737	ng/ul	0.00
73) Anthracene-d10	17.377	188		637451	40.568	ng/ul	0.00
81) Pyrene-d10	19.669	212		763466	41.163	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.451	264		780476	42.848	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
Data File : BG058302.D
Acq On : 18 Jul 2023 15:39
Operator : CG/JU
Sample : PB154044BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK044

Manual IntegrationsAPPROVED

Quant Time: Jul 19 04:49:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 18 02:19:39 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2023
Supervised By :Sohil Jodhani 07/19/2023

