

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
 Data File : BG058306.D
 Acq On : 18 Jul 2023 18:27
 Operator : CG/JU
 Sample : 03444-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A46P5

Quant Time: Jul 19 04:57:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	36063	20.000	ng/ul	0.00
20) Naphthalene-d8	10.697	136	160395	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.533	164	118894	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.277	188	294323	20.000	ng/ul	0.00
79) Chrysene-d12	21.525	240	257668	20.000	ng/ul	0.00
88) Perylene-d12	24.663	264	307656	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.341	96	4982	5.085	ng/uL	0.00
4) Pyridine-d5	3.752	84	76198	26.201	ng/ul	0.00
7) Phenol-d5	7.060	99	102939	30.090	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.224	67	65854	30.798	ng/ul	0.00
11) 2-Chlorophenol-d4	7.430	132	72734	30.373	ng/ul	0.00
15) 4-Methylphenol-d8	8.599	113	77047	29.526	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	37714	31.369	ng/ul	0.00
24) 2-Nitrophenol-d4	9.780	143	41652	31.734	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.321	165	75754	30.108	ng/ul	0.00
31) 4-Chloroaniline-d4	10.838	131	106717	29.258	ng/ul	0.00
46) Dimethylphthalate-d6	13.940	166	268868	29.326	ng/ul	0.00
49) Acenaphthylene-d8	14.228	160	306376	31.888	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	34502	24.918	ng/ul	0.00
60) Fluorene-d10	15.526	176	247635	32.624	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.644	200	37585	25.065	ng/ul	0.00
73) Anthracene-d10	17.377	188	405203	31.862	ng/ul	0.00
81) Pyrene-d10	19.669	212	483881	31.795	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.445	264	480006	32.280	ng/ul	0.00


Target Compounds					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.414	149	13249	1.339	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
Data File : BG058306.D
Acq On : 18 Jul 2023 18:27
Operator : CG/JU
Sample : 03444-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A46P5


Quant Time: Jul 19 04:57:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 18 02:19:39 2023
Response via : Initial Calibration

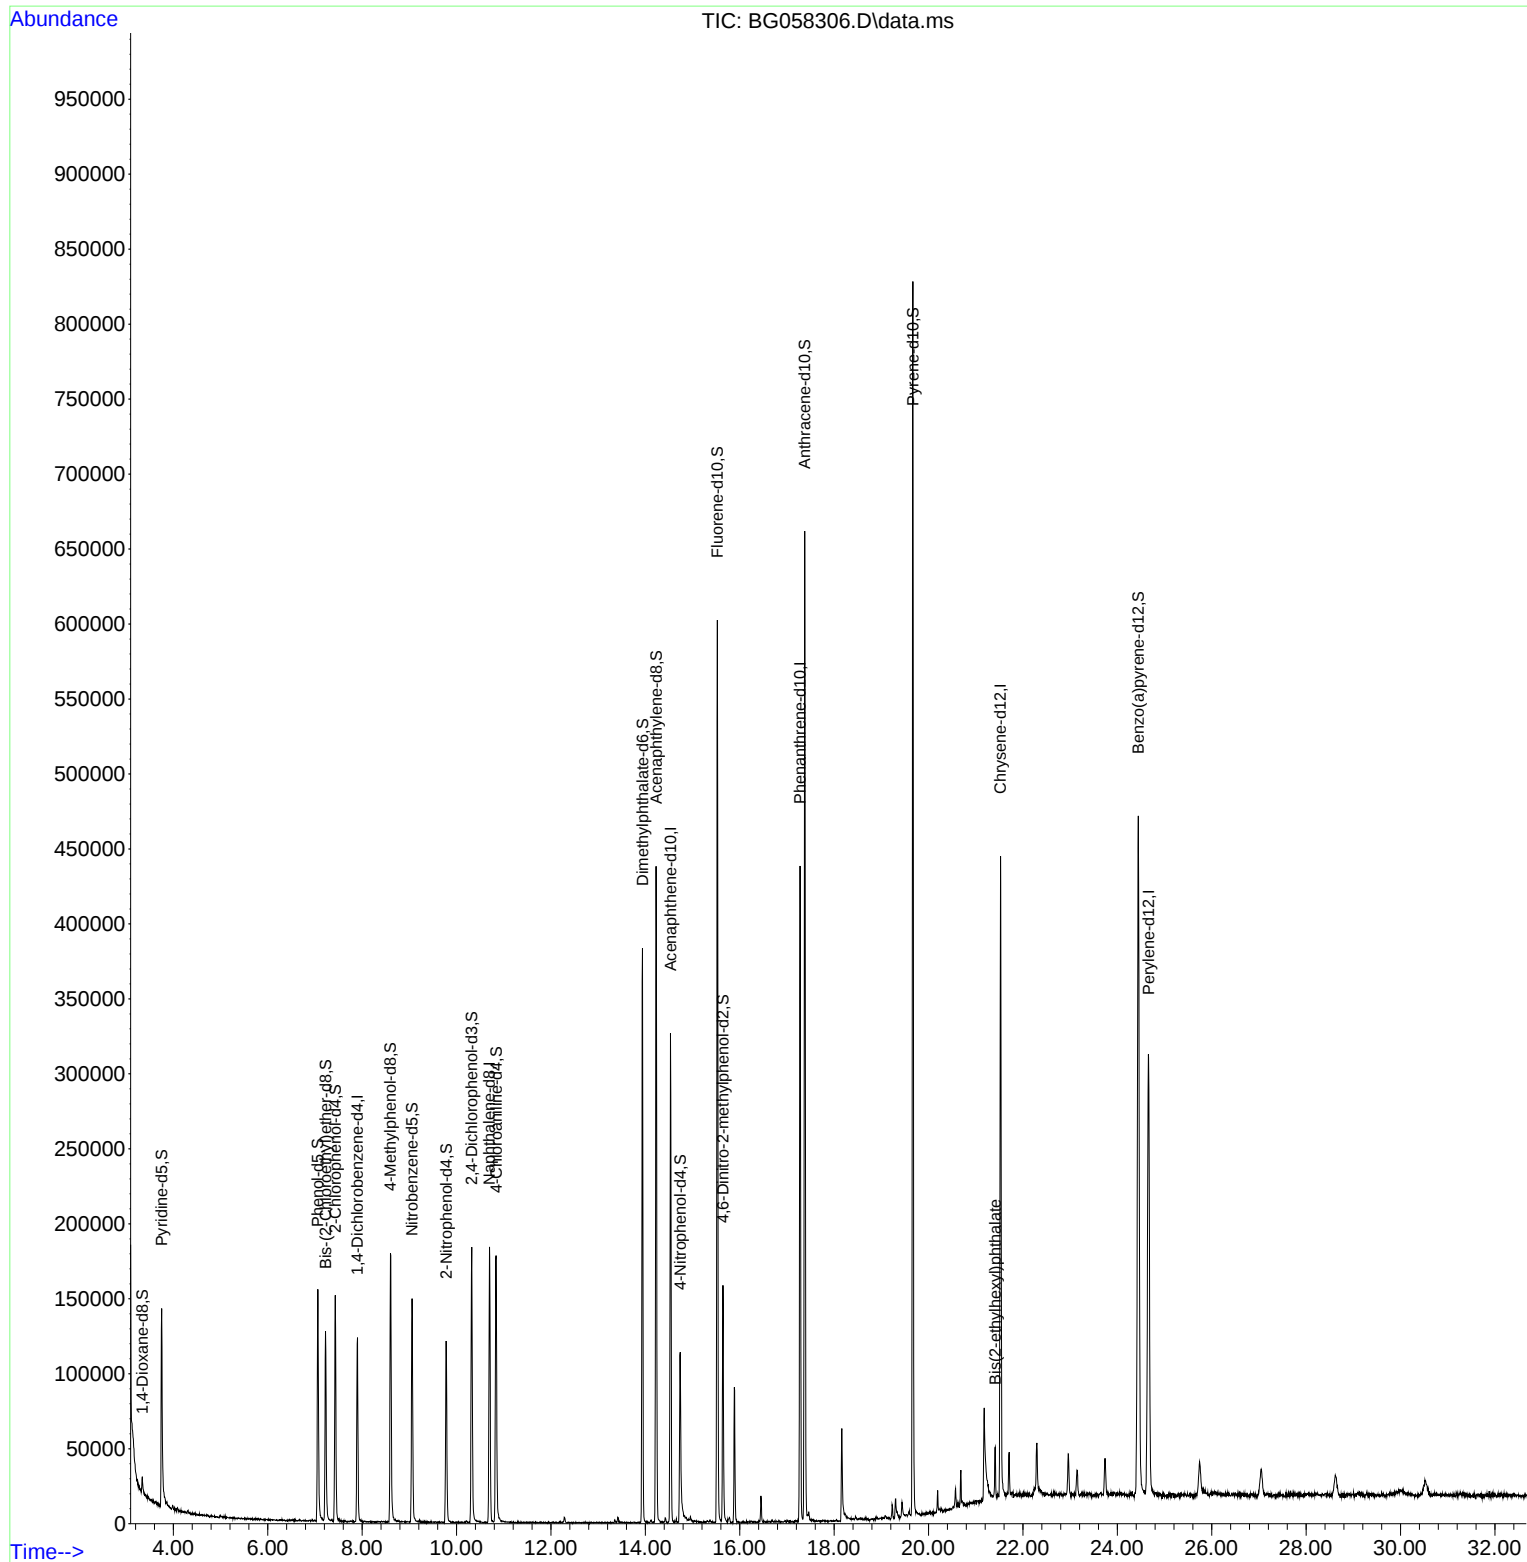

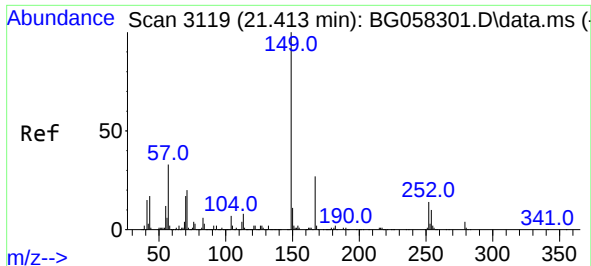

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.339 ng/ul
 RT: 21.414 min Scan# 3119
 Delta R.T. 0.001 min
 Lab File: BG058306.D
 Acq: 18 Jul 2023 18:27

Instrument :
 BNA_G
 ClientSampleId :
 A46P5

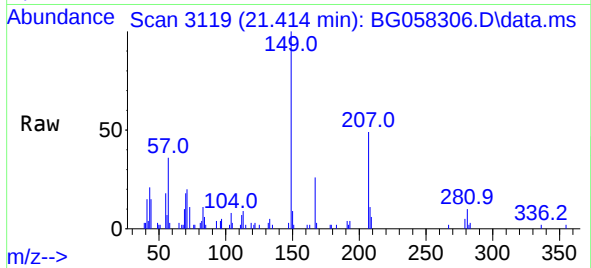

Tgt Ion:149 Resp: 13249
 Ion Ratio Lower Upper
 149 100
 167 26.2 21.6 32.4
 279 4.9 3.0 4.4#

