

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
 Data File : BG058370.D
 Acq On : 20 Jul 2023 22:28
 Operator : CG/JU
 Sample : 03472-33
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A46T0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/21/2023
 Supervised By :mohammad ahmed 07/21/2023

Quant Time: Jul 21 00:07:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	42529	20.000	ng/u1	0.00
20) Naphthalene-d8	10.695	136	205163	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.532	164	150286	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.276	188	334515	20.000	ng/u1	0.00
79) Chrysene-d12	21.524	240	271932	20.000	ng/u1	0.00
88) Perylene-d12	24.661	264	324863	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	1622	1.404	ng/uL	0.00
4) Pyridine-d5	3.745	84	22340	6.514	ng/u1	0.00
7) Phenol-d5	7.058	99	33100	8.204	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.223	67	22878	9.073	ng/u1	0.00
11) 2-Chlorophenol-d4	7.423	132	23938	8.476	ng/u1	0.00
15) 4-Methylphenol-d8	8.615	113	1435	0.466	ng/u1	0.01
21) Nitrobenzene-d5	9.056	128	14030	9.123	ng/u1	0.00
24) 2-Nitrophenol-d4	9.779	143	16586	9.879	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.319	165	24023	7.464	ng/u1	0.00
31) 4-Chloroaniline-d4	10.836	131	209	0.045	ng/u1	0.00
46) Dimethylphthalate-d6	13.933	166	111893	9.655	ng/u1	0.00
49) Acenaphthylene-d8	14.226	160	118069	9.722	ng/u1	0.00
54) 4-Nitrophenol-d4	14.738	143	11012	6.292	ng/u1	0.00
60) Fluorene-d10	15.525	176	106155	11.064	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.648	200	8755	5.137	ng/u1	0.00
73) Anthracene-d10	17.376	188	97206	6.725	ng/u1	0.00
81) Pyrene-d10	19.661	212	140780	8.765	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.438	264	57680	3.674	ng/u1	-0.01
Target Compounds					Qvalue	
16) Acetophenone	8.715	105	16301	3.110	ng/u1	99
72) Phenanthrene	17.317	178	116550	7.332	ng/u1	98
74) Anthracene	17.405	178	17873	1.120	ng/u1	98
80) Fluoranthene	19.332	202	196982	10.706	ng/u1	98
82) Pyrene	19.696	202	116173	6.231	ng/u1	98
85) Benzo(a)anthracene	21.506	228	77757	4.254	ng/u1	99
86) Bis(2-ethylhexyl)phtha...	21.406	149	24829	2.378	ng/u1	98
87) Chrysene	21.571	228	75006	4.326	ng/u1	98
90) Benzo(b)fluoranthene	23.668	252	94513	5.028	ng/u1#	97
91) Benzo(k)fluoranthene	23.727	252	39027m	2.082	ng/u1	
93) Benzo(a)pyrene	24.508	252	17686	1.058	ng/u1#	96
94) Indeno(1,2,3-cd)pyrene	28.222	276	28624	1.300	ng/u1#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
Data File : BG058370.D
Acq On : 20 Jul 2023 22:28
Operator : CG/JU
Sample : 03472-33
Misc :
ALS Vial : 41 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
A46T0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/21/2023
Supervised By :mohammad ahmed 07/21/2023


Quant Time: Jul 21 00:07:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 18 02:19:39 2023
Response via : Initial Calibration

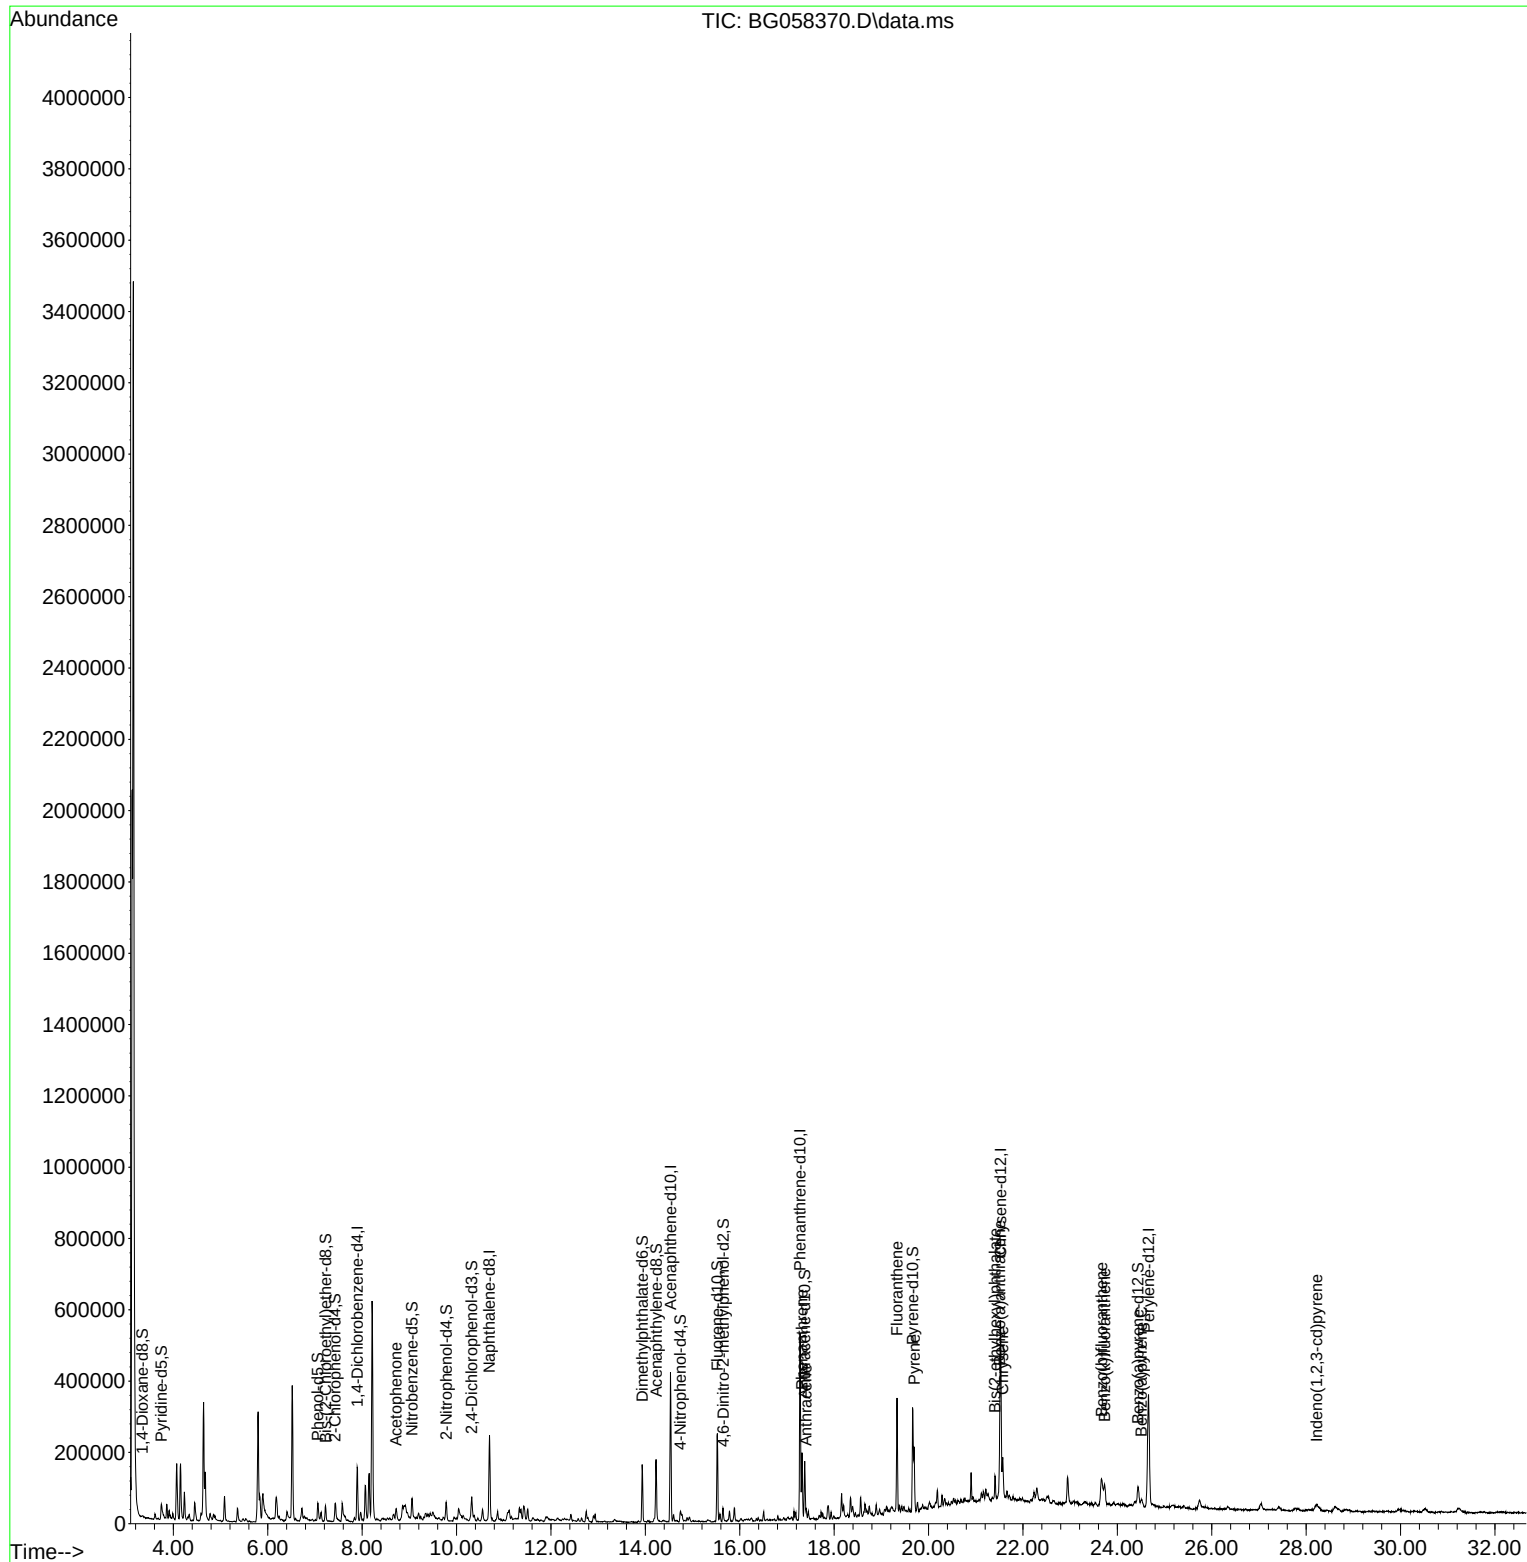

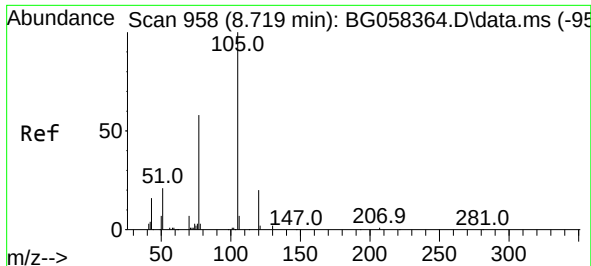

#16
Acetophenone
Concen: 3.110 ng/ul
RT: 8.715 min Scan# 91
Delta R.T. -0.006 min
Lab File: BG058370.D
Acq: 20 Jul 2023 22:28




Instrument :
BNA_G
ClientSampleId :
A46T0

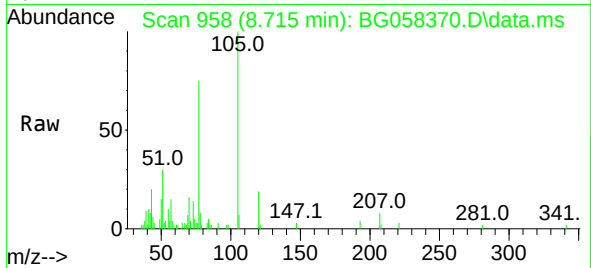

Tgt Ion:105 Resp: 1630
Ion Ratio Lower Upper
105 100
77 75.4 60.7 91.1
51 30.3 23.5 35.3




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/21/2023
Supervised By :mohammad ahmed 07/21/2023

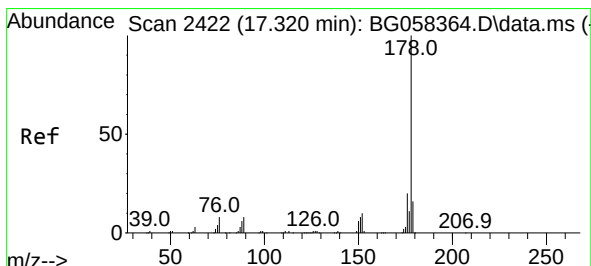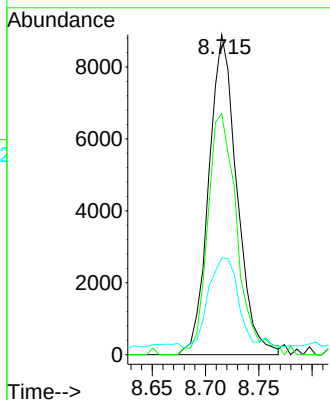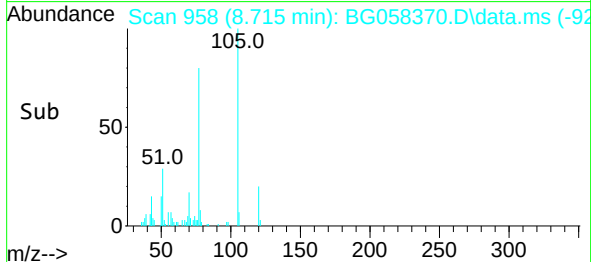

#72
Phenanthrene
Concen: 7.332 ng/ul
RT: 17.317 min Scan# 2422
Delta R.T. -0.006 min
Lab File: BG058370.D
Acq: 20 Jul 2023 22:28


Tgt Ion:178 Resp: 116550
Ion Ratio Lower Upper
178 100
179 16.1 11.9 17.9
176 19.5 15.8 23.8

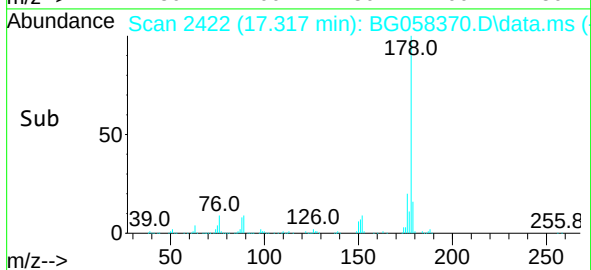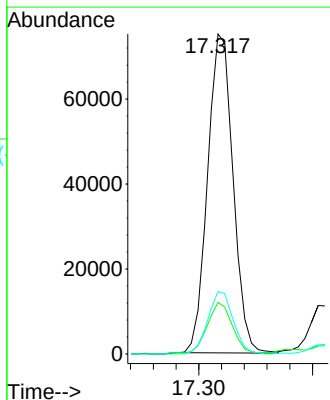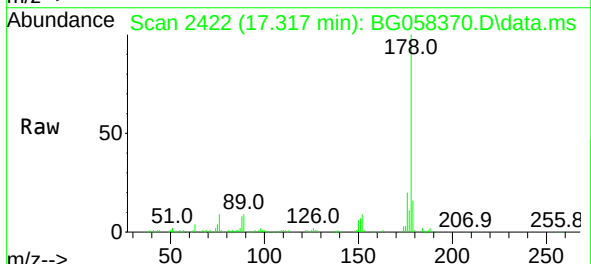

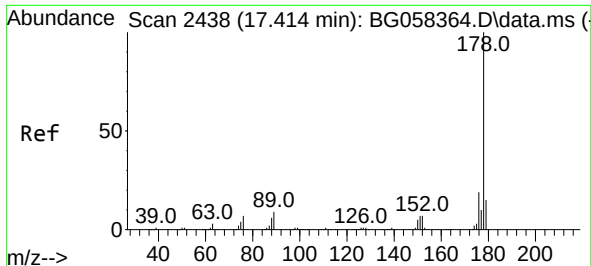

#74
 Anthracene
 Concen: 1.120 ng/ul
 RT: 17.405 min Scan# 2438
 Delta R.T. -0.012 min
 Lab File: BG058370.D
 Acq: 20 Jul 2023 22:28




Instrument :
 BNA_G
 ClientSampleId :
 A46T0

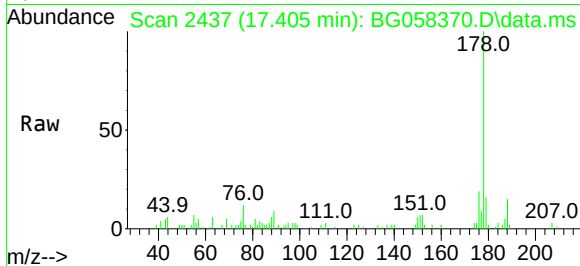


Tgt Ion:178 Resp: 1787
 Ion Ratio Lower Upper
 178 100
 179 16.5 13.4 20.2
 176 19.0 16.2 24.2

Manual Integrations
 APPROVED



Reviewed By :Yogesh Patel 07/21/2023
 Supervised By :mohammad ahmed 07/21/2023

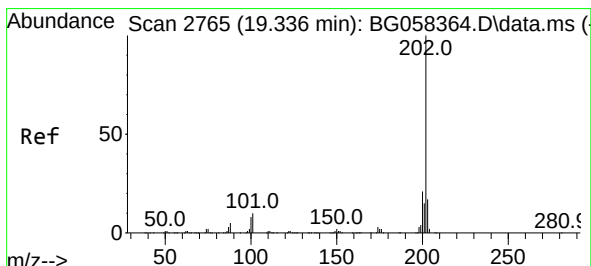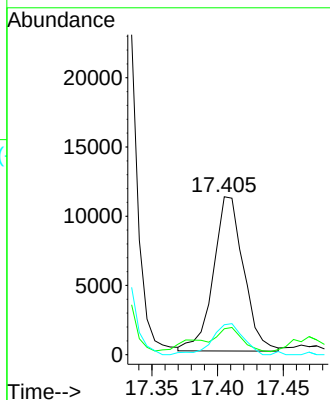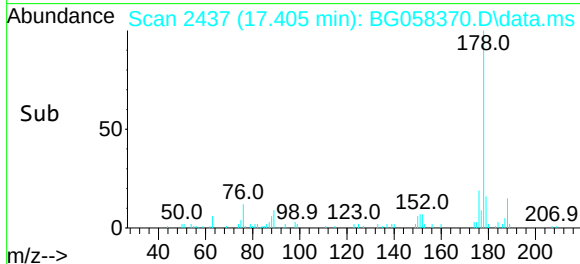


#80
 Fluoranthene
 Concen: 10.706 ng/ul
 RT: 19.332 min Scan# 2765
 Delta R.T. -0.000 min
 Lab File: BG058370.D
 Acq: 20 Jul 2023 22:28

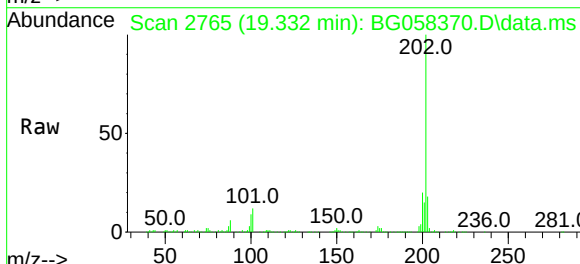

Tgt Ion:202 Resp: 196982
 Ion Ratio Lower Upper
 202 100
 101 11.6 8.6 12.8
 100 8.5 7.2 10.8

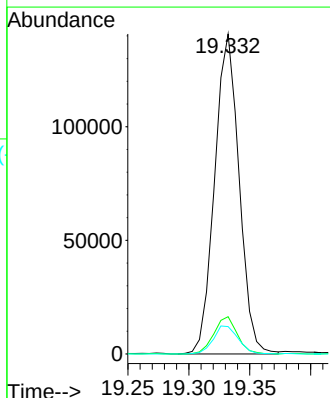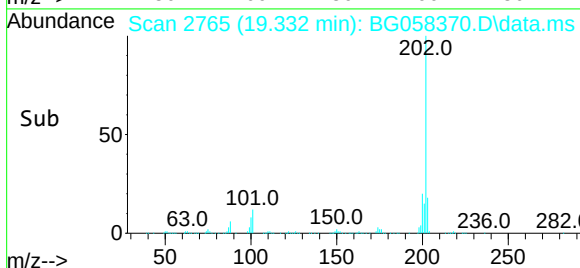

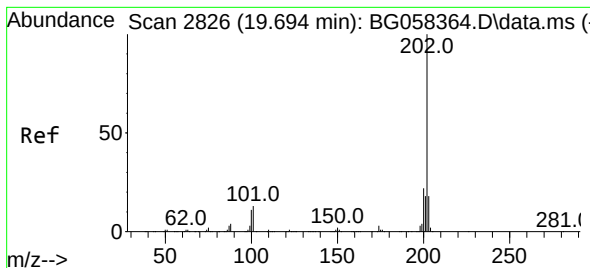

#82

Pyrene

Concen: 6.231 ng/ul

RT: 19.696 min Scan# 2826

Delta R.T. -0.000 min

Lab File: BG058370.D

Acq: 20 Jul 2023 22:28

Instrument :

BNA_G

ClientSampleId :

A46T0





Tgt Ion:202	Resp: 11617
Ion Ratio	Lower Upper
202 100	
101 11.8	10.2 15.2
100 10.2	8.9 13.3

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/21/2023

Supervised By :mohammad ahmed 07/21/2023

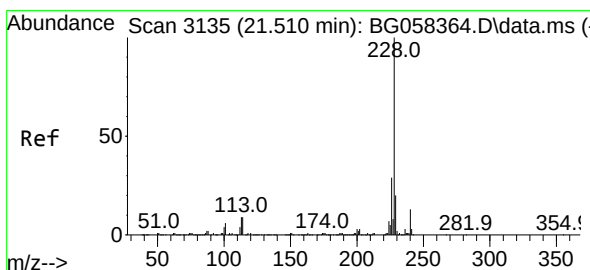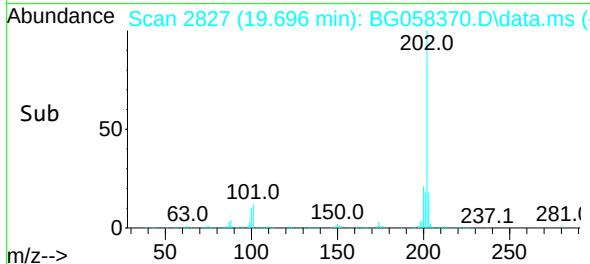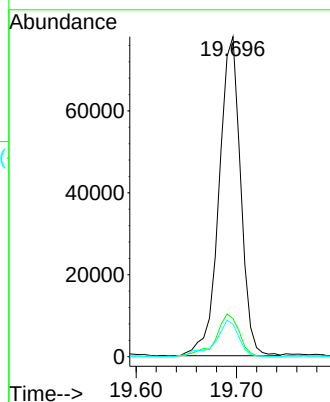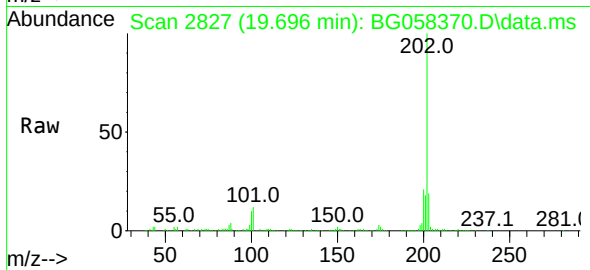

#85

Benzo(a)anthracene

Concen: 4.254 ng/ul




RT: 21.506 min Scan# 3135


Delta R.T. -0.006 min

Lab File: BG058370.D

Acq: 20 Jul 2023 22:28


Tgt Ion:228	Resp: 77757
Ion Ratio	Lower Upper
228 100	
229 19.9	15.7 23.5
226 28.1	21.8 32.8

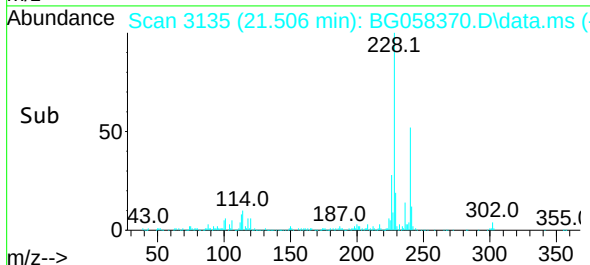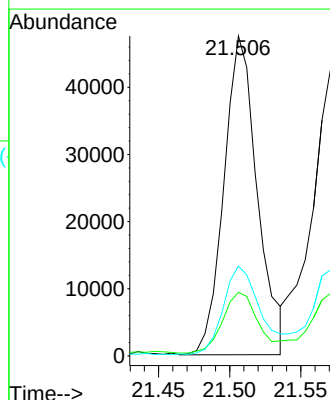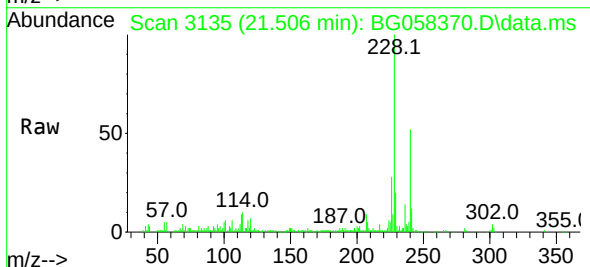

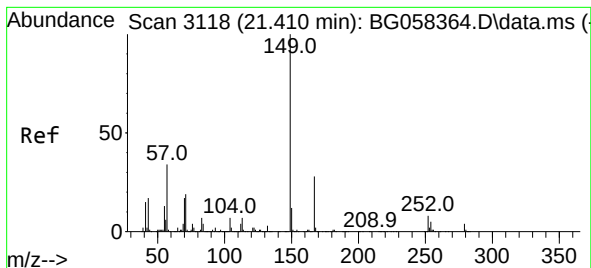

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.378 ng/ul
 RT: 21.406 min Scan# 3118
 Delta R.T. -0.006 min
 Lab File: BG058370.D
 Acq: 20 Jul 2023 22:28




Instrument :
 BNA_G
 ClientSampleId :
 A46T0

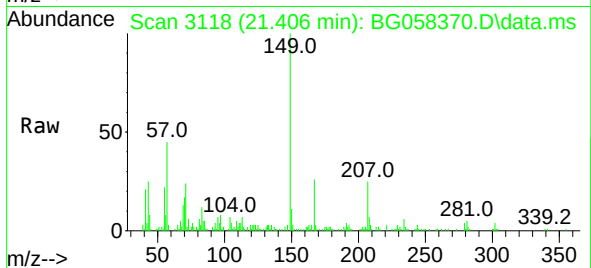

Tgt Ion:149 Resp: 24829
 Ion Ratio Lower Upper
 149 100
 167 25.8 21.6 32.4
 279 3.7 3.0 4.4




Manual Integrations
 APPROVED


Reviewed By :Yogesh Patel 07/21/2023
 Supervised By :mohammad ahmed 07/21/2023

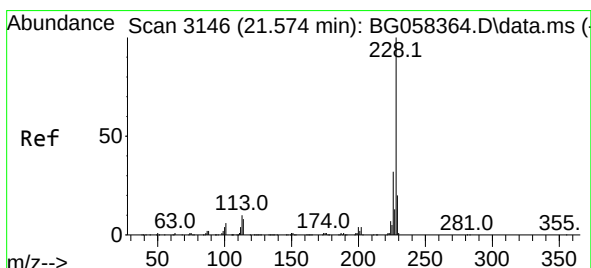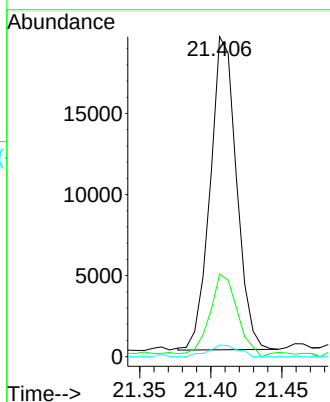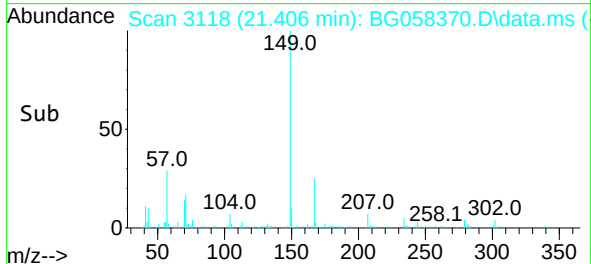

#87
 Chrysene
 Concen: 4.326 ng/ul
 RT: 21.571 min Scan# 3146
 Delta R.T. -0.006 min
 Lab File: BG058370.D
 Acq: 20 Jul 2023 22:28


Tgt Ion:228 Resp: 75006
 Ion Ratio Lower Upper
 228 100
 226 30.1 24.0 36.0
 229 21.8 15.8 23.8

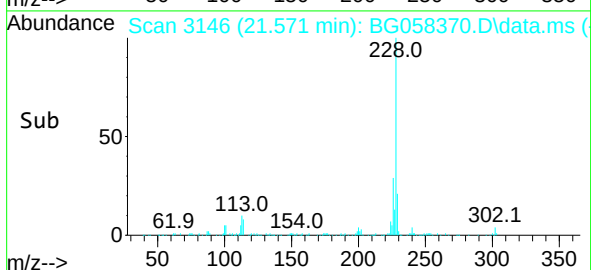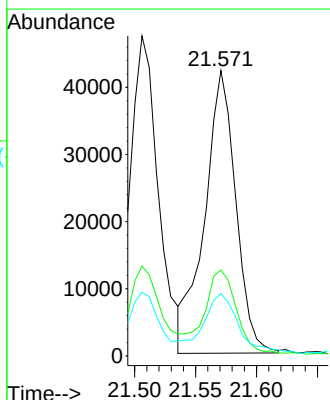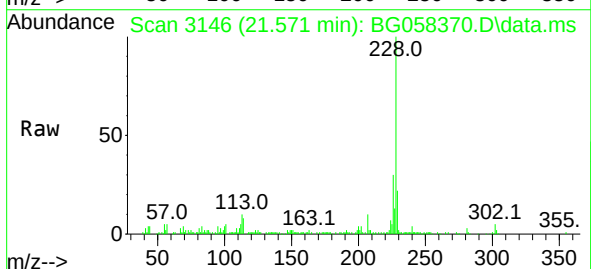

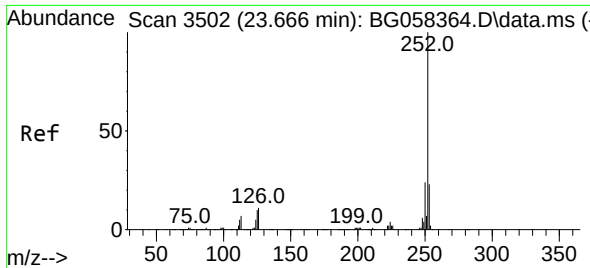

#90
Benzo(b)fluoranthene
Concen: 5.028 ng/ul
RT: 23.668 min Scan# 3503
Delta R.T. -0.000 min
Lab File: BG058370.D
Acq: 20 Jul 2023 22:28




Instrument :
BNA_G
ClientSampleId :
A46T0

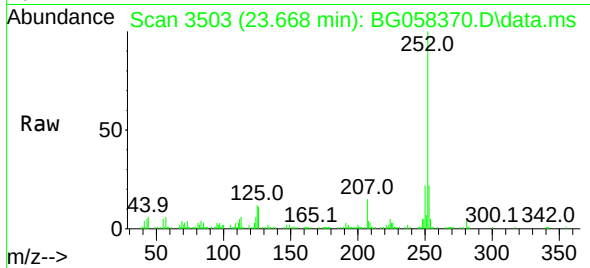


Tgt Ion:252 Resp: 9451
Ion Ratio Lower Upper
252 100
253 22.0 17.9 26.9
125 11.6 6.7 10.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/21/2023
Supervised By :mohammad ahmed 07/21/2023

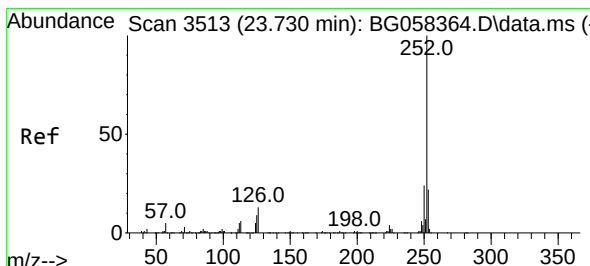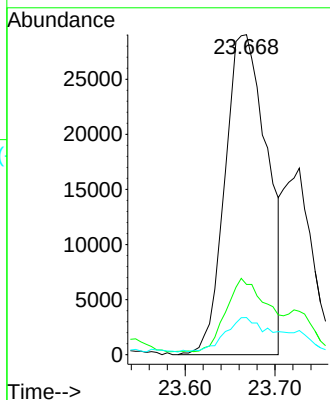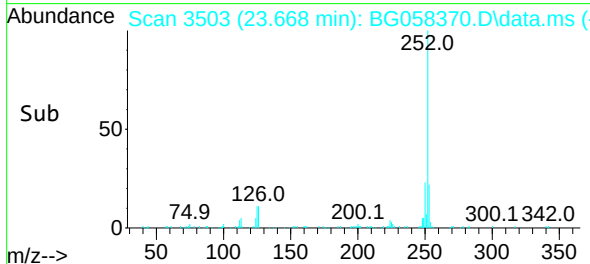


#91
Benzo(k)fluoranthene
Concen: 2.082 ng/ul m
RT: 23.727 min Scan# 3513
Delta R.T. -0.006 min
Lab File: BG058370.D
Acq: 20 Jul 2023 22:28

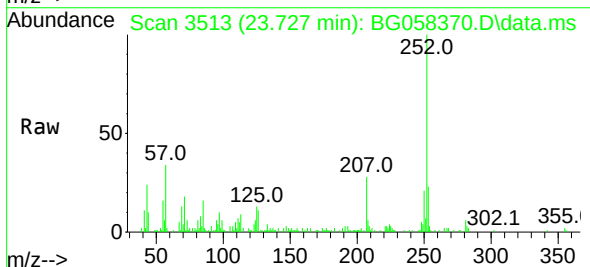

Tgt Ion:252 Resp: 39027
Ion Ratio Lower Upper
252 100
253 23.3 18.3 27.5
125 13.0 7.4 11.0

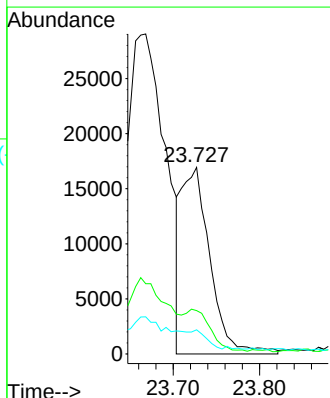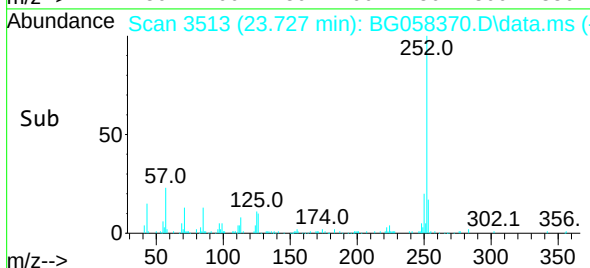

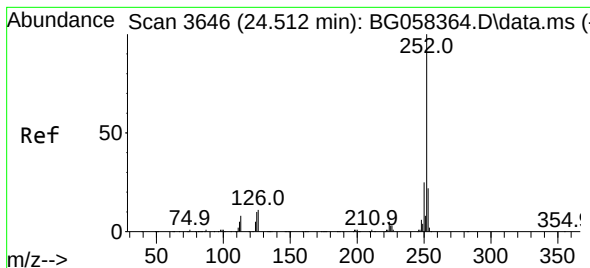

#93

Benzo(a)pyrene

Concen: 1.058 ng/ul

RT: 24.508 min Scan# 3646

Delta R.T. -0.012 min

Lab File: BG058370.D

Acq: 20 Jul 2023 22:28

Instrument :

BNA_G

ClientSampleId :

A46T0





Tgt Ion:	252	Resp:	17680
Ion Ratio	Lower	Upper	
252	100		
253	21.9	17.4	26.0
125	14.7	7.7	11.5

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/21/2023

Supervised By :mohammad ahmed 07/21/2023

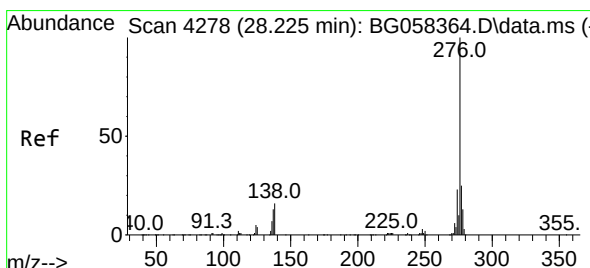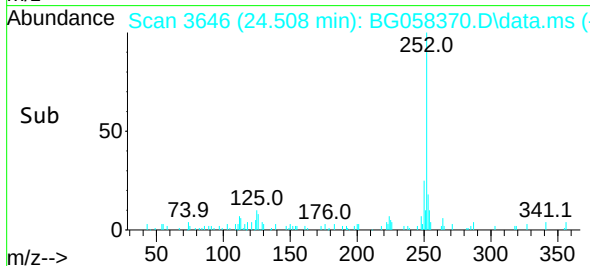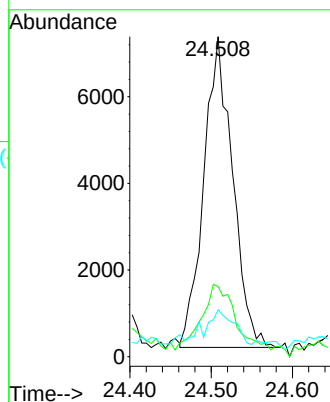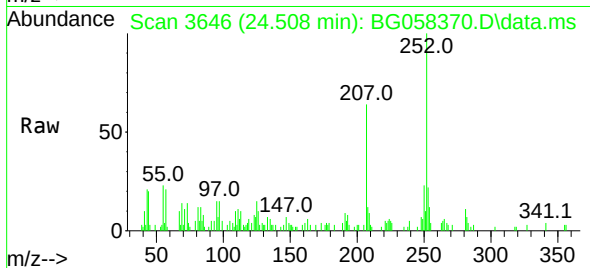

#94

Indeno(1,2,3-cd)pyrene

Concen: 1.300 ng/ul

RT: 28.222 min Scan# 4278

Delta R.T. -0.006 min

Lab File: BG058370.D

Acq: 20 Jul 2023 22:28

Tgt Ion:	276	Resp:	28624
Ion Ratio	Lower	Upper	
276	100		
138	20.7	13.8	20.6
277	28.0	19.2	28.8

