

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
 Data File : BG058347.D
 Acq On : 20 Jul 2023 5:10
 Operator : CG/JU
 Sample : PB154087BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK087

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.341	39	43	53	rVB	16421	27166	1.49%	0.155%
2	3.746	107	112	125	rBV	209286	363273	19.97%	2.071%
3	4.081	164	169	176	rVB4	3742	7567	0.42%	0.043%
4	4.781	286	288	295	rVB4	1287	1883	0.10%	0.011%
5	7.060	669	676	694	rBV	230857	407976	22.43%	2.325%
6	7.225	697	704	712	rBV	178333	305366	16.79%	1.741%
7	7.424	730	738	754	rVB	222658	390871	21.49%	2.228%
8	7.895	812	818	830	rBV	151955	262020	14.41%	1.494%
9	8.600	930	938	952	rBV	293022	524557	28.84%	2.990%
10	9.058	1008	1016	1029	rBV	227485	411560	22.63%	2.346%
11	9.775	1130	1138	1151	rBV	182723	337920	18.58%	1.926%
12	10.315	1221	1230	1241	rBV	282777	531203	29.21%	3.028%
13	10.697	1286	1295	1305	rBV	243132	434213	23.87%	2.475%
14	10.832	1310	1318	1331	rBV	289565	545699	30.00%	3.111%
15	12.284	1560	1565	1572	rBV2	3650	6306	0.35%	0.036%
16	13.417	1754	1758	1764	rVB2	4445	6770	0.37%	0.039%
17	13.935	1840	1846	1856	rBV	586768	870507	47.86%	4.962%
18	14.228	1889	1896	1910	rBV	674572	1068708	58.76%	6.092%
19	14.534	1941	1948	1957	rBV	435169	672843	36.99%	3.835%
20	14.734	1976	1982	2004	rBV	180314	394817	21.71%	2.250%
21	15.527	2109	2117	2128	rBV	897627	1376983	75.71%	7.849%
22	15.644	2131	2137	2147	rBV	237283	359824	19.78%	2.051%
23	15.756	2152	2156	2163	rVV3	3925	7381	0.41%	0.042%
24	17.278	2408	2415	2425	rBV	575798	871220	47.90%	4.966%
25	17.378	2425	2432	2444	rVV	982136	1522523	83.71%	8.678%
26	19.234	2741	2748	2752	rBV2	12144	18257	1.00%	0.104%
27	19.305	2755	2760	2764	rVB	9486	14281	0.79%	0.081%
28	19.575	2804	2806	2810	rBV4	1760	2392	0.13%	0.014%
29	19.669	2815	2822	2833	rBV	1184669	1766774	97.14%	10.071%
30	20.509	2961	2965	2969	rBV8	2944	4854	0.27%	0.028%
31	20.586	2976	2978	2980	rBV3	2636	2608	0.14%	0.015%
32	20.621	2981	2984	2988	rVB4	6827	8317	0.46%	0.047%
33	20.656	2988	2990	2991	rBV2	2076	2015	0.11%	0.011%
34	20.685	2991	2995	2998	rVV5	2138	3950	0.22%	0.023%
35	21.173	3076	3078	3083	rVB4	6422	7473	0.41%	0.043%
36	21.214	3083	3085	3087	rVB2	2676	1913	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
 Data File : BG058347.D
 Acq On : 20 Jul 2023 5:10
 Operator : CG/JU
 Sample : PB154087BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK087

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

37	21.526	3131	3138	3150	rBV2	531211	872974	48.00%	4.976%
38	21.608	3150	3152	3154	rBV3	2563	1915	0.11%	0.011%
39	21.702	3164	3168	3172	rVB2	12433	14111	0.78%	0.080%
40	22.154	3243	3245	3246	rBV2	3237	3016	0.17%	0.017%
41	22.289	3265	3268	3278	rVB4	21742	47070	2.59%	0.268%
42	22.959	3375	3382	3389	rVB5	18691	39639	2.18%	0.226%
43	23.130	3409	3411	3414	rBV4	3094	3483	0.19%	0.020%
44	23.459	3465	3467	3470	rBV4	2912	2353	0.13%	0.013%
45	23.735	3509	3514	3520	rVB2	17809	35858	1.97%	0.204%
46	24.446	3624	3635	3649	rBV2	666843	1818864	100.00%	10.368%
47	24.657	3661	3671	3686	rVB	359878	1017218	55.93%	5.798%
48	25.427	3800	3802	3805	rBV4	2791	2892	0.16%	0.016%
49	25.738	3847	3855	3864	rBV3	21967	67830	3.73%	0.387%
50	27.043	4070	4077	4088	rVB4	19247	64714	3.56%	0.369%
51	27.366	4128	4132	4134	rBV4	3103	4346	0.24%	0.025%
52	32.336	4975	4978	4981	rBV5	3075	5437	0.30%	0.031%




Sum of corrected areas: 17543710

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
Data File : BG058347.D
Acq On : 20 Jul 2023 5:10
Operator : CG/JU
Sample : PB154087BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK087

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

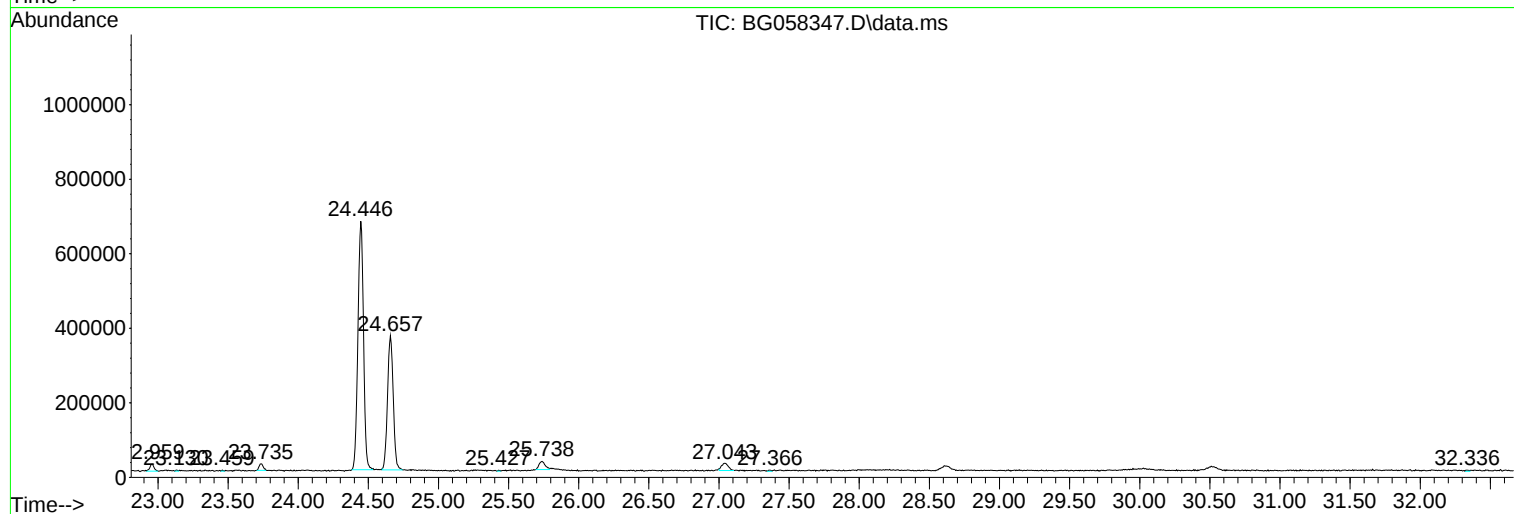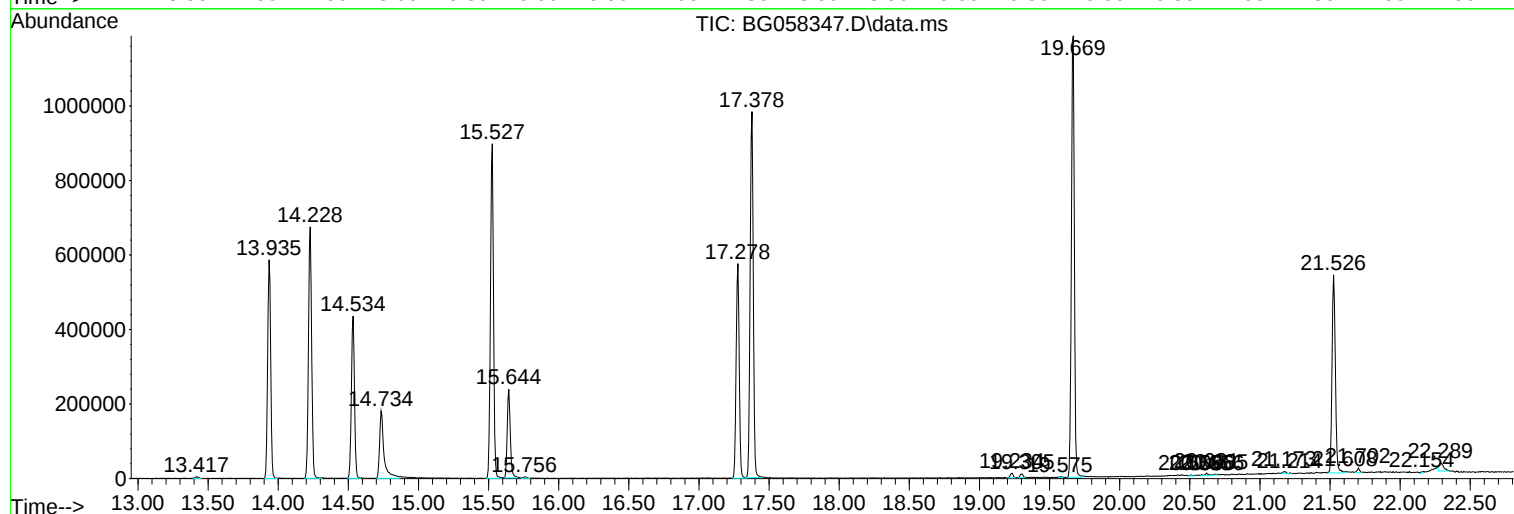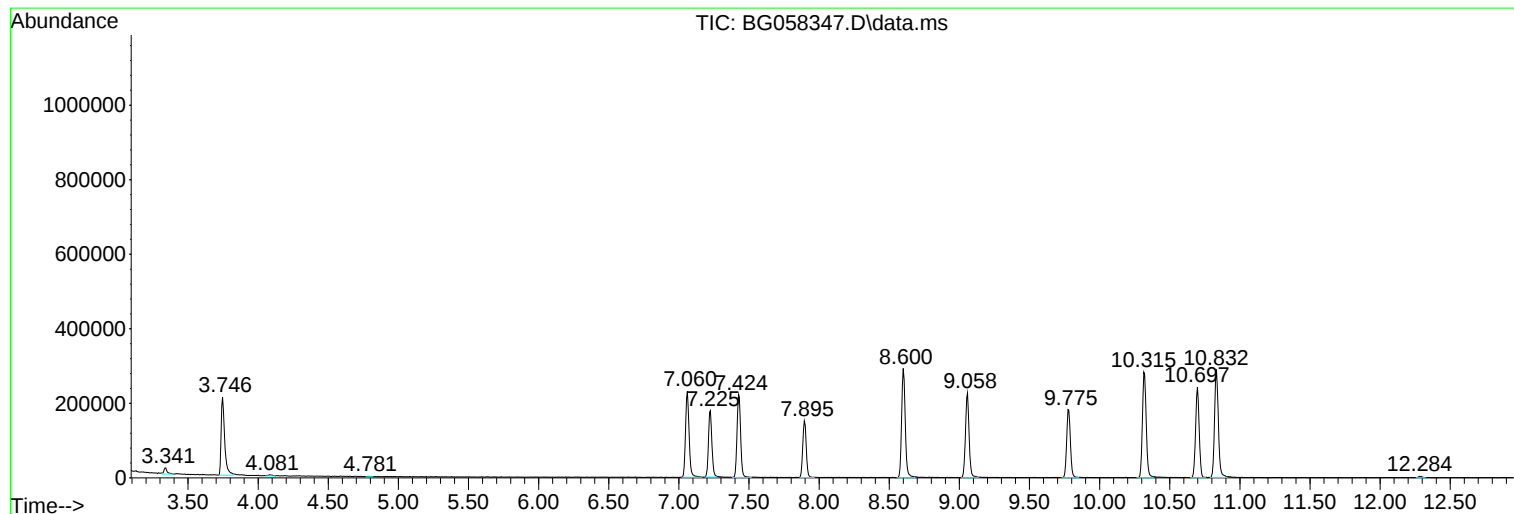

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
Data File : BG058347.D
Acq On : 20 Jul 2023 5:10
Operator : CG/JU
Sample : PB154087BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK087

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071823\
Data File : BG058347.D
Acq On : 20 Jul 2023 5:10
Operator : CG/JU
Sample : PB154087BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK087

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc