
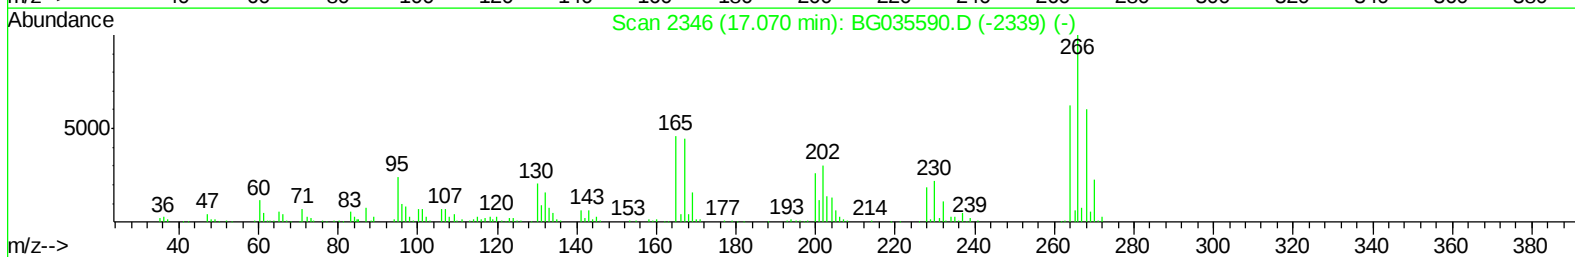
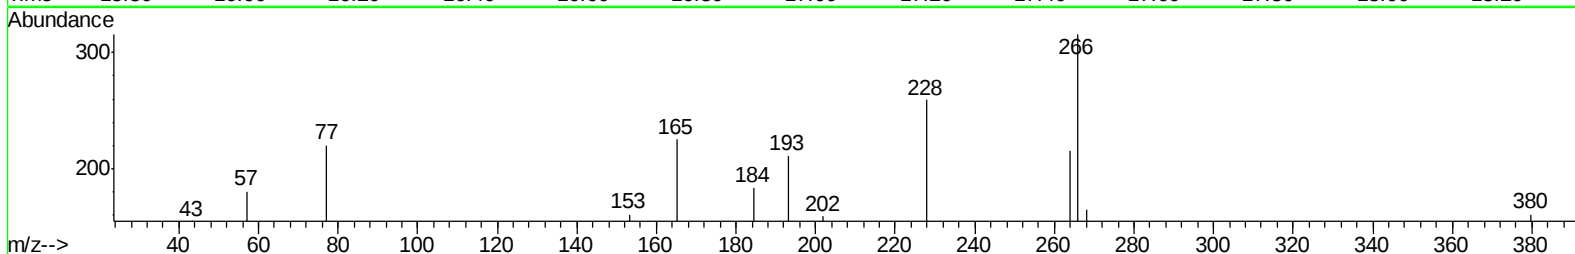


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071918\
Data File : BG035754.D
Acq On : 19 Jul 2018 18:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 04:15:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 18 17:45:13 2018
Response via : Initial Calibration

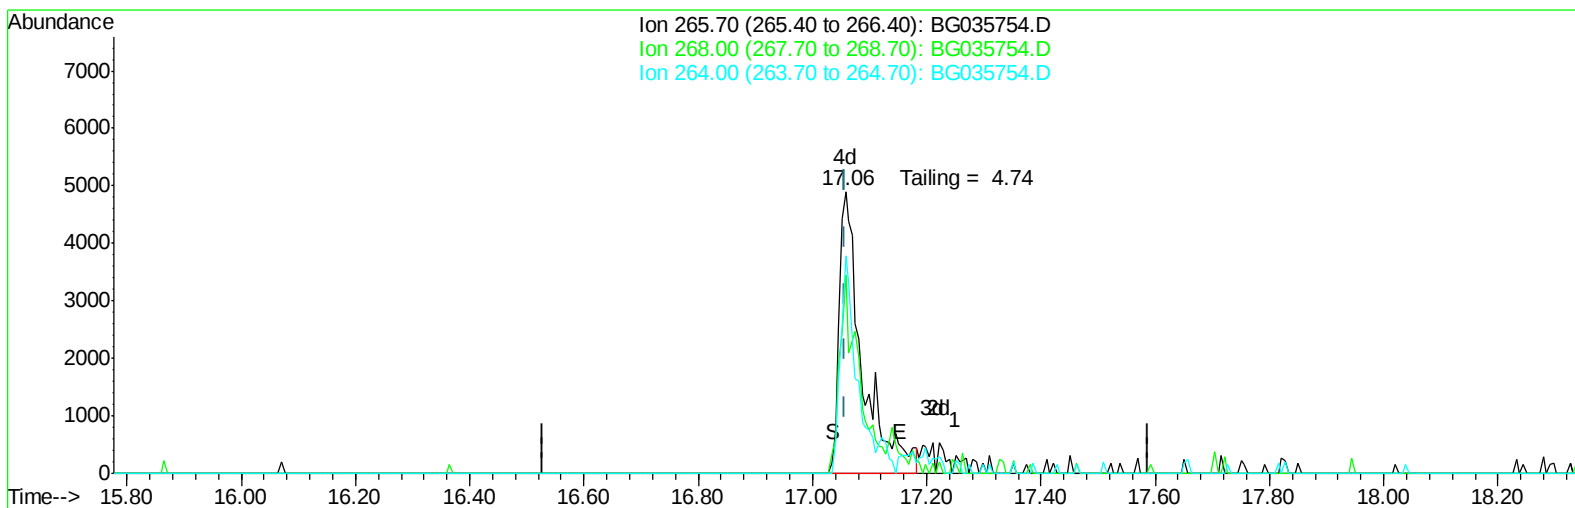

TIC: BG035754.D

(69) Pentachlorophenol (C)




17.251min (+0.194) 95.20ng

response 354

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	51.90
264.00	62.00	68.04
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG071918\
 Data File : BG035754.D
 Acq On : 19 Jul 2018 18:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 04:15:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 18 17:45:13 2018
 Response via : Initial Calibration

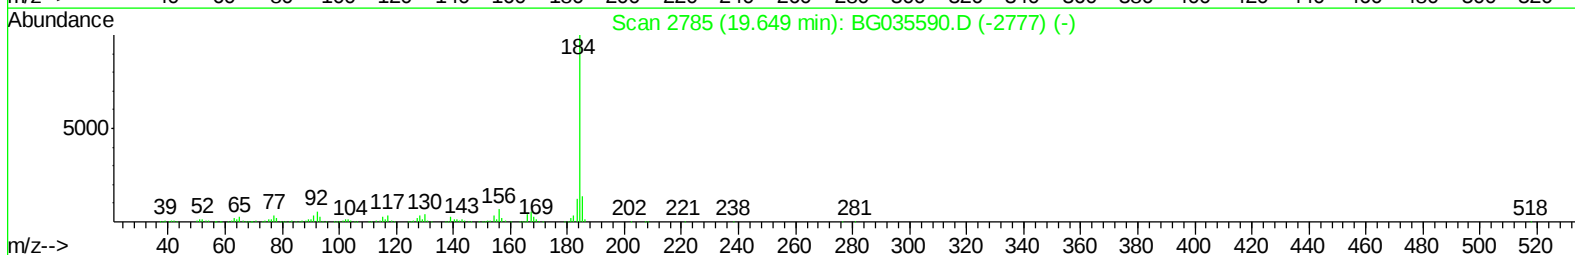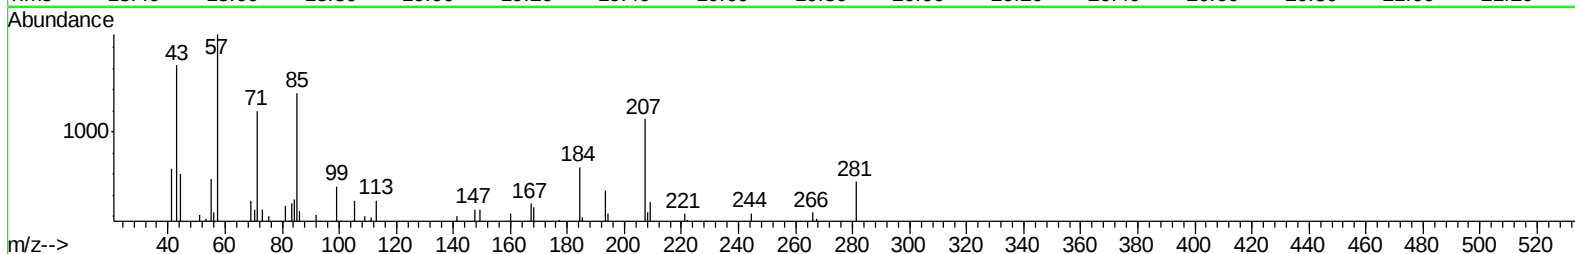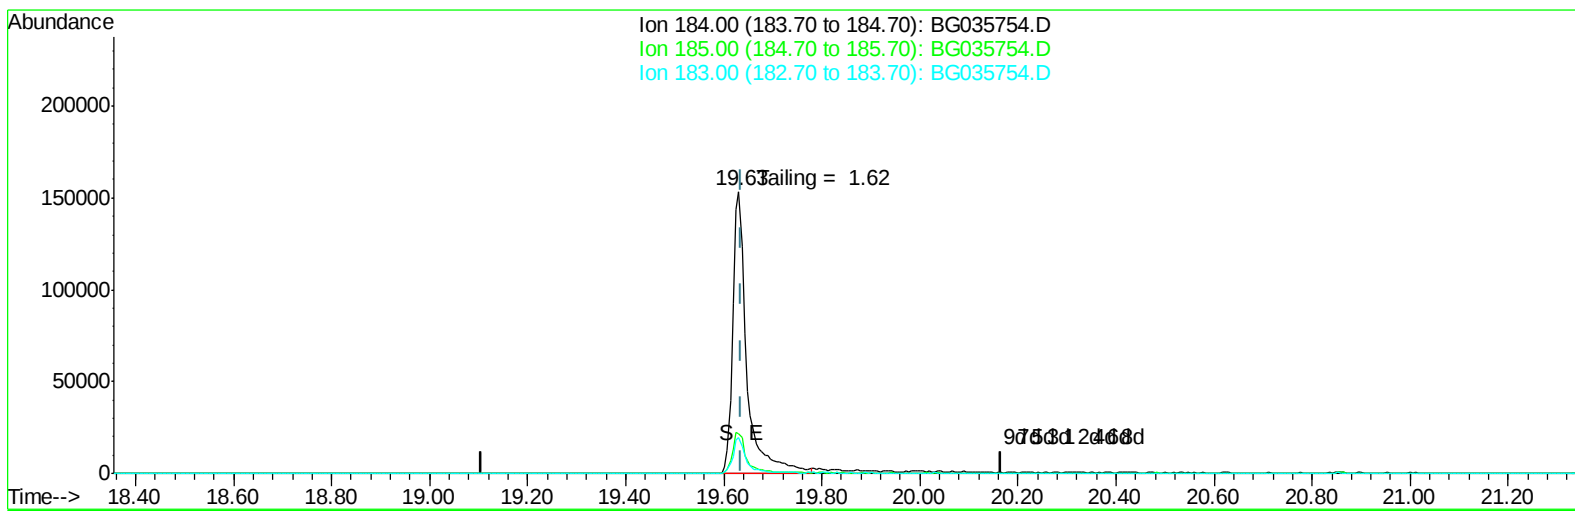

TIC: BG035754.D

(76) Benzidine

20.306min (+0.670) 240.11ng

response 808

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	28.27#
183.00	13.30	0.00#
0.00	0.00	0.00