
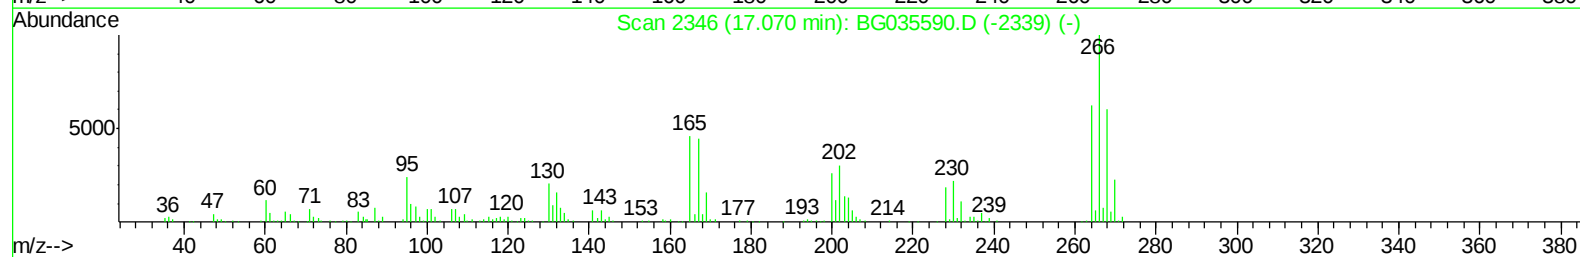
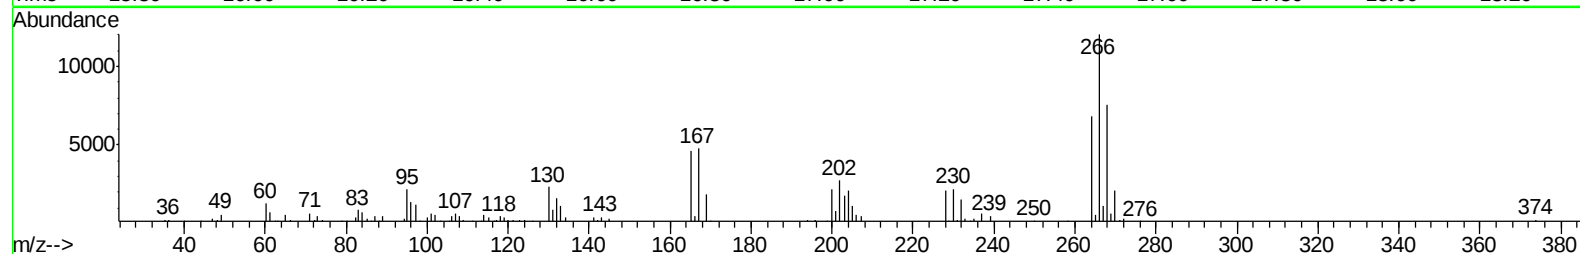


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071918\
Data File : BG035773.D
Acq On : 20 Jul 2018 7:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 08:22:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 15:28:54 2018
Response via : Initial Calibration

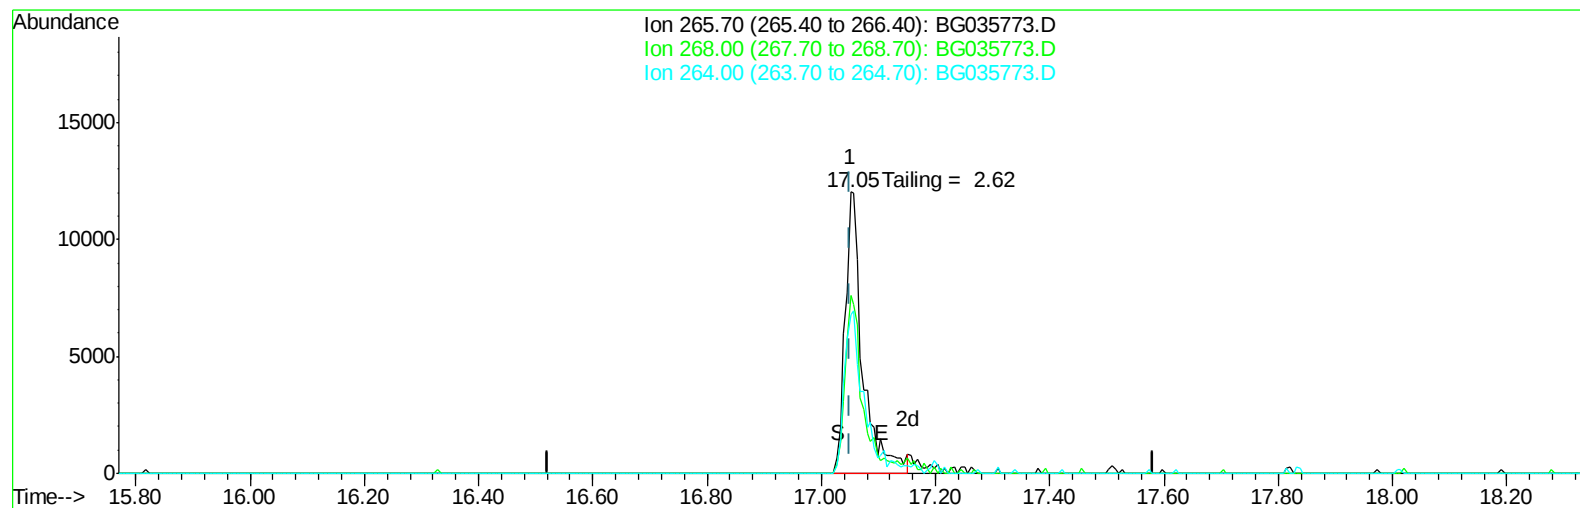

TIC: BG035773.D

(69) Pentachlorophenol (C)




17.051min (-0.000) 7233.09ng

response 25634

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.98
264.00	62.00	56.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG071918\
Data File : BG035773.D
Acq On : 20 Jul 2018 7:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 08:22:56 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 15:28:54 2018
Response via : Initial Calibration

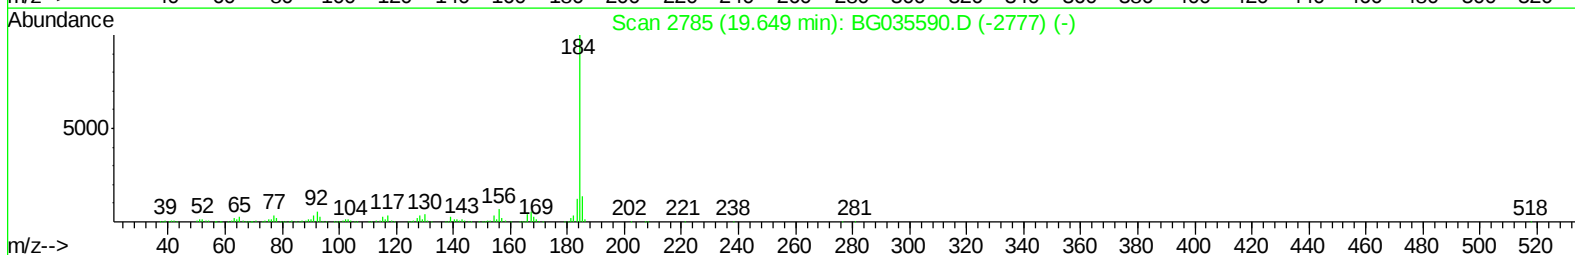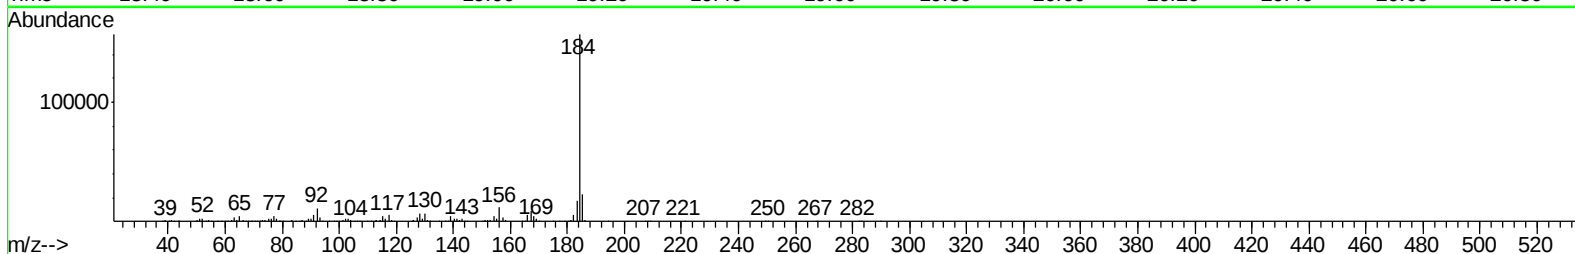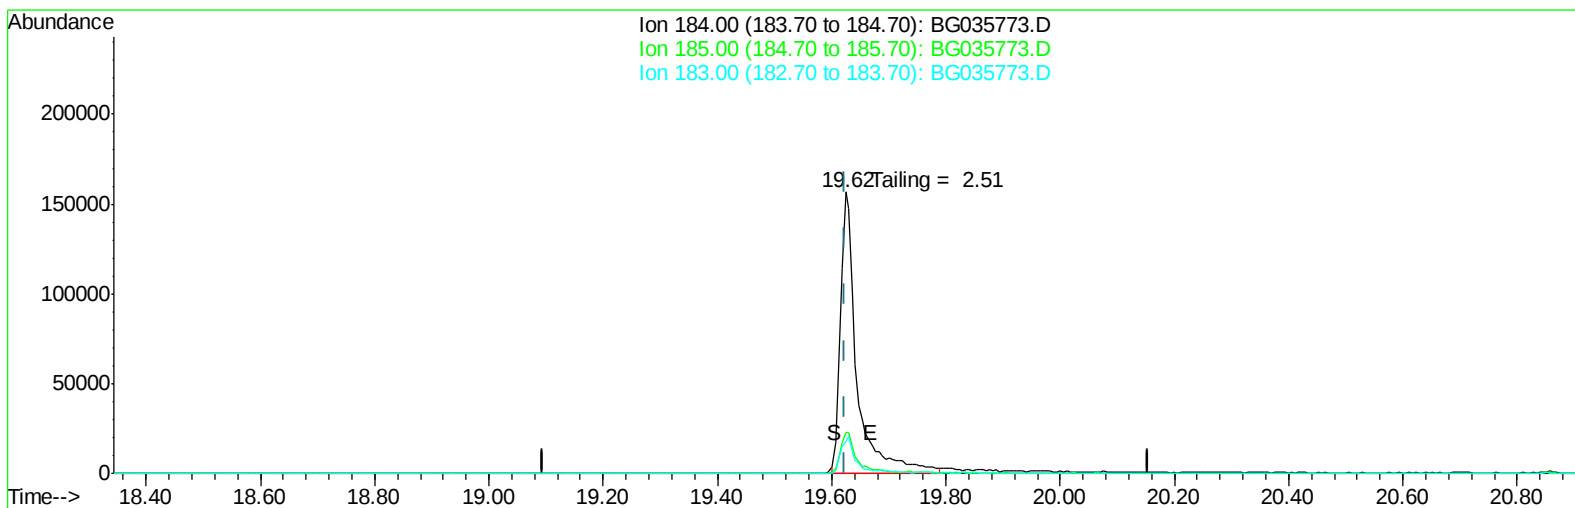

TIC: BG035773.D

(76) Benzidine

19.624min (-0.000) 172641.91ng

response 317716

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.57
183.00	13.30	11.19
0.00	0.00	0.00