


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071918\
Data File : BG035754.D
Acq On : 19 Jul 2018 18:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 31 12:30:06 2018

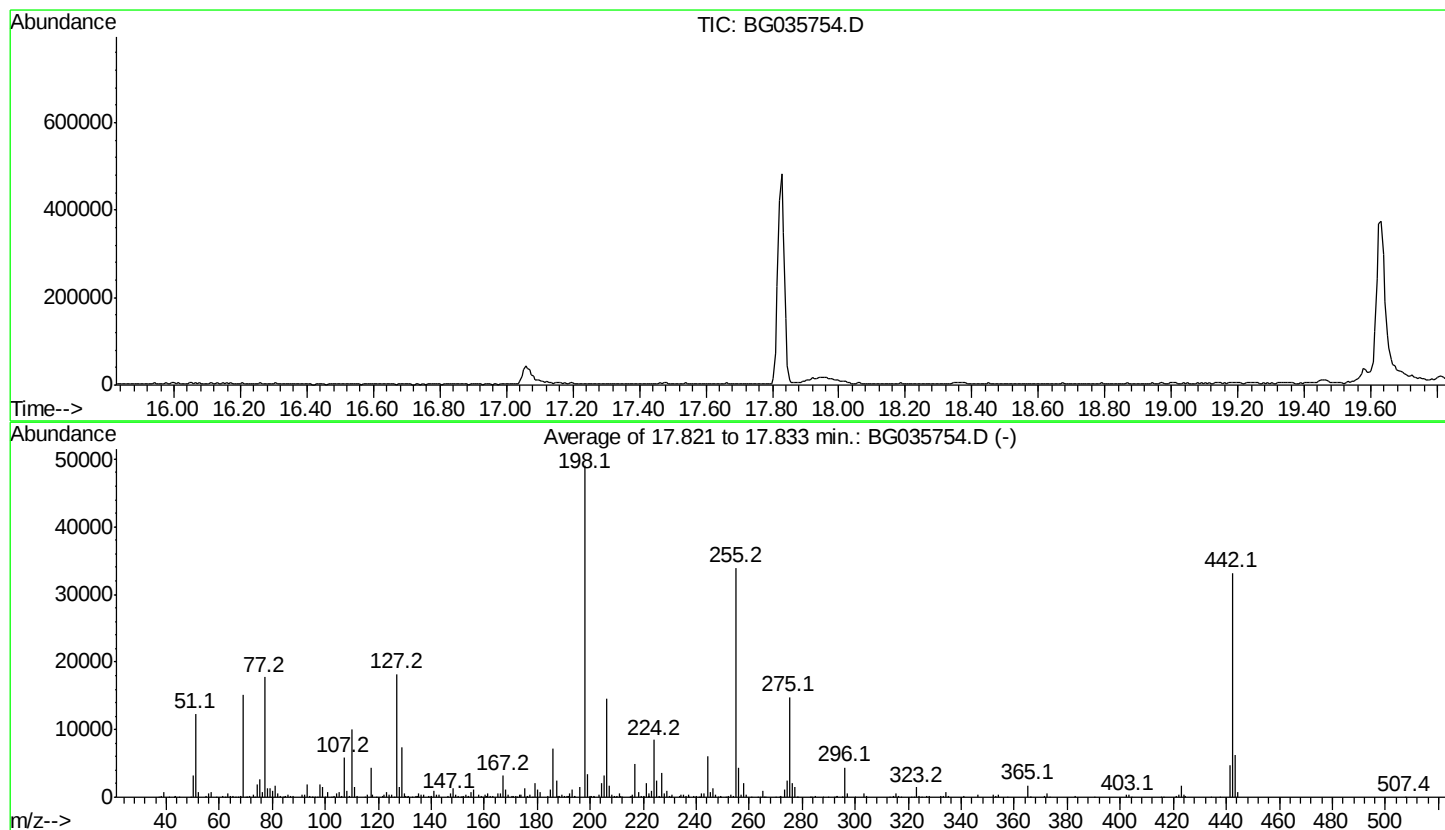

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	12318	PASS
68	69	0.00	2	0.8	128	PASS
69	198	0.00	100	30.8	15126	PASS
70	69	0.00	2	0.5	71	PASS
127	198	10	80	37.1	18187	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49034	PASS
199	198	5	9	7.0	3430	PASS
275	198	10	60	30.2	14799	PASS
365	198	1	100	3.7	1801	PASS
441	198	0.01	100	9.6	4710	PASS
442	198	50	100	67.6	33165	PASS
443	442	15	24	19.1	6346	PASS