


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071918\
 Data File : BG035773.D
 Acq On : 20 Jul 2018 7:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

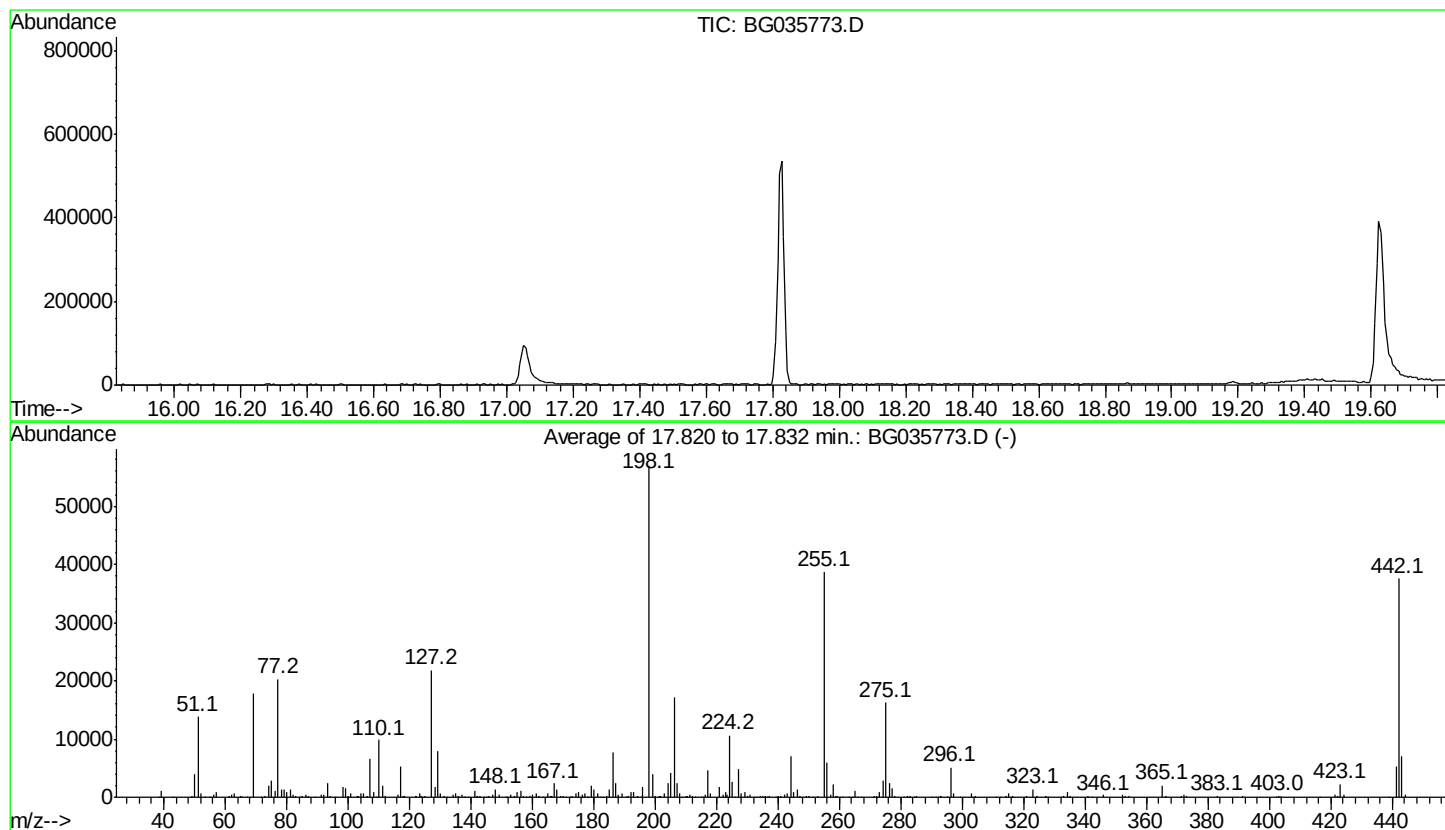

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	13774	PASS
68	69	0.00	2	0.5	91	PASS
69	198	0.00	100	31.5	17925	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.4	21848	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	56968	PASS
199	198	5	9	7.1	4035	PASS
275	198	10	60	28.5	16246	PASS
365	198	1	100	3.6	2028	PASS
441	198	0.01	100	9.3	5325	PASS
442	198	50	100	65.9	37533	PASS
443	442	15	24	19.0	7138	PASS