
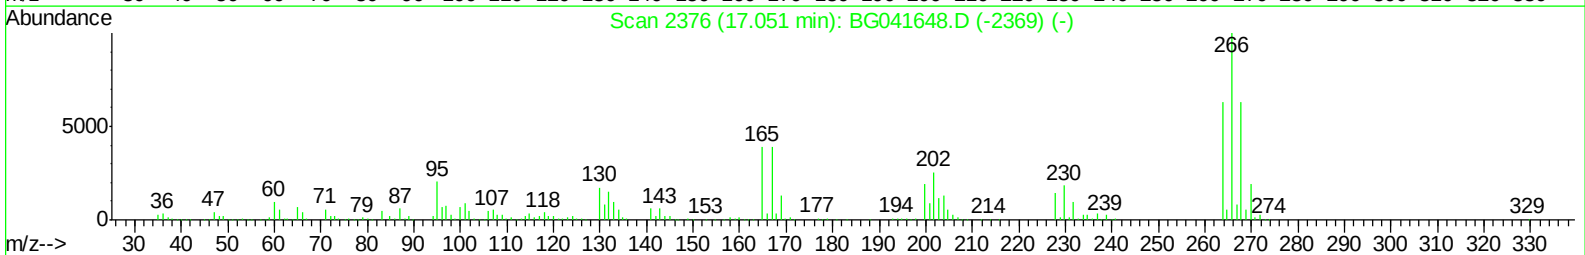
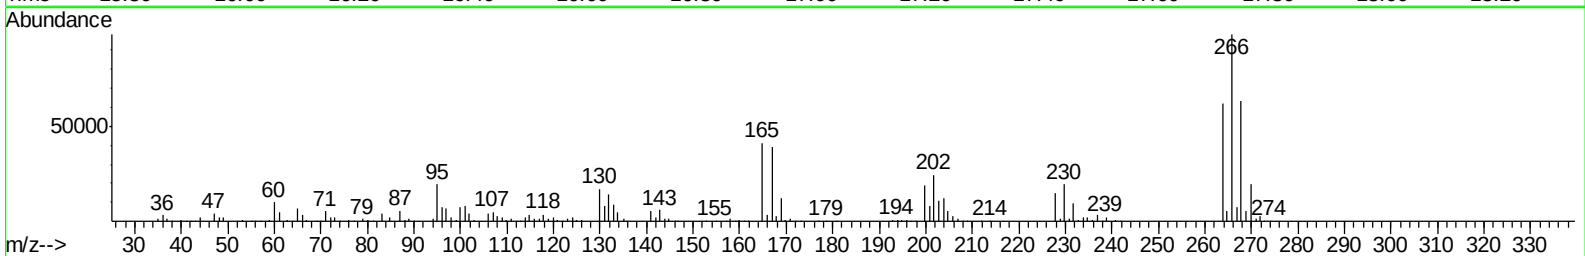


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071919\
Data File : BG041724.D
Acq On : 19 Jul 2019 7:56
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 06:37:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 16:16:21 2019
Response via : Initial Calibration

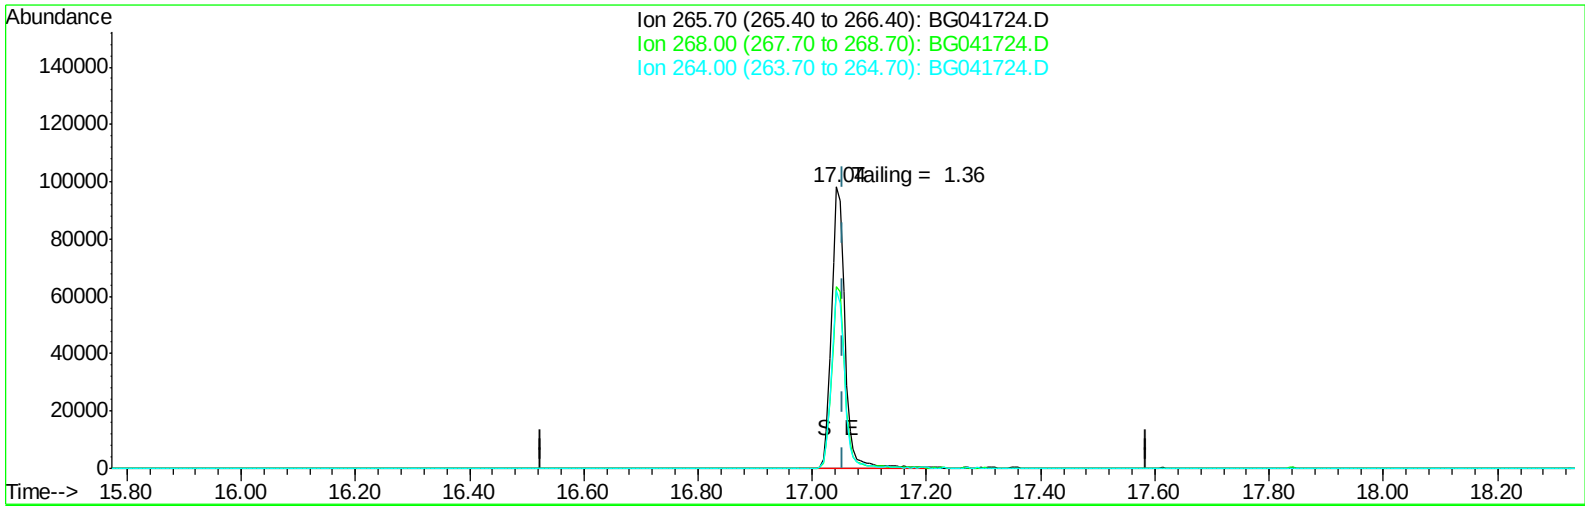

TIC: BG041724.D

(70) Pentachlorophenol (C)




17.043min (-0.013) 28972.51ng

response 157149

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	64.56
264.00	64.30	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG071919\
 Data File : BG041724.D
 Acq On : 19 Jul 2019 7:56
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 06:37:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 15 16:16:21 2019
 Response via : Initial Calibration

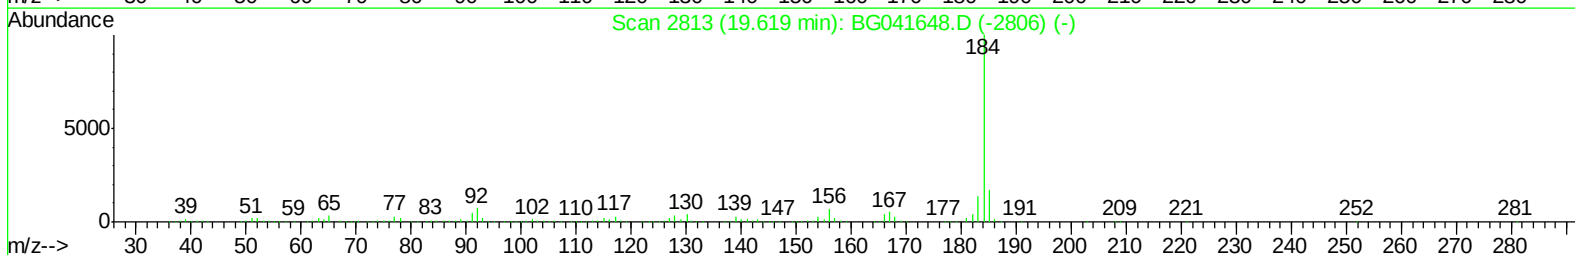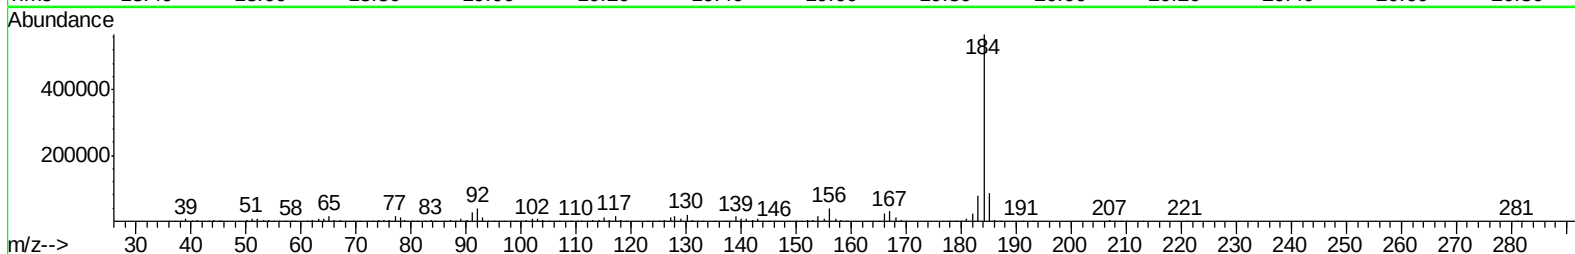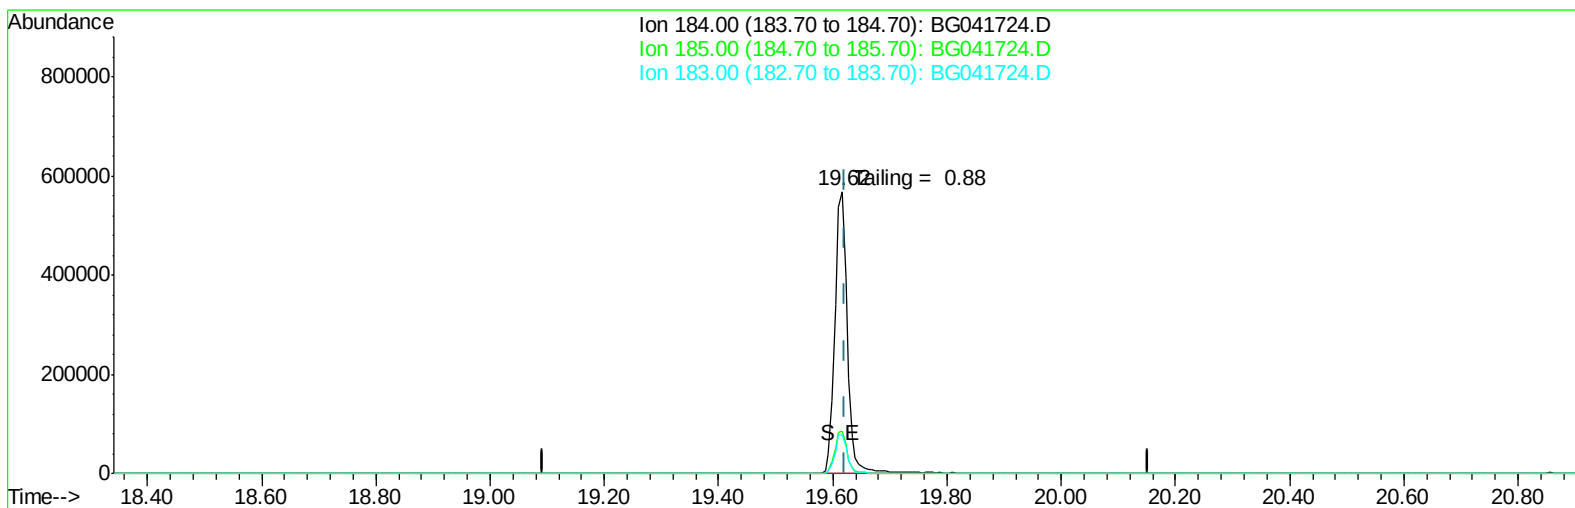

TIC: BG041724.D

(77) Benzidine

19.616min (-0.007) 0.00ng

response 854786

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.97
183.00	14.70	13.56
0.00	0.00	0.00