


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG071919\
 Data File : BG041724.D
 Acq On : 19 Jul 2019 7:56
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 15 16:16:21 2019

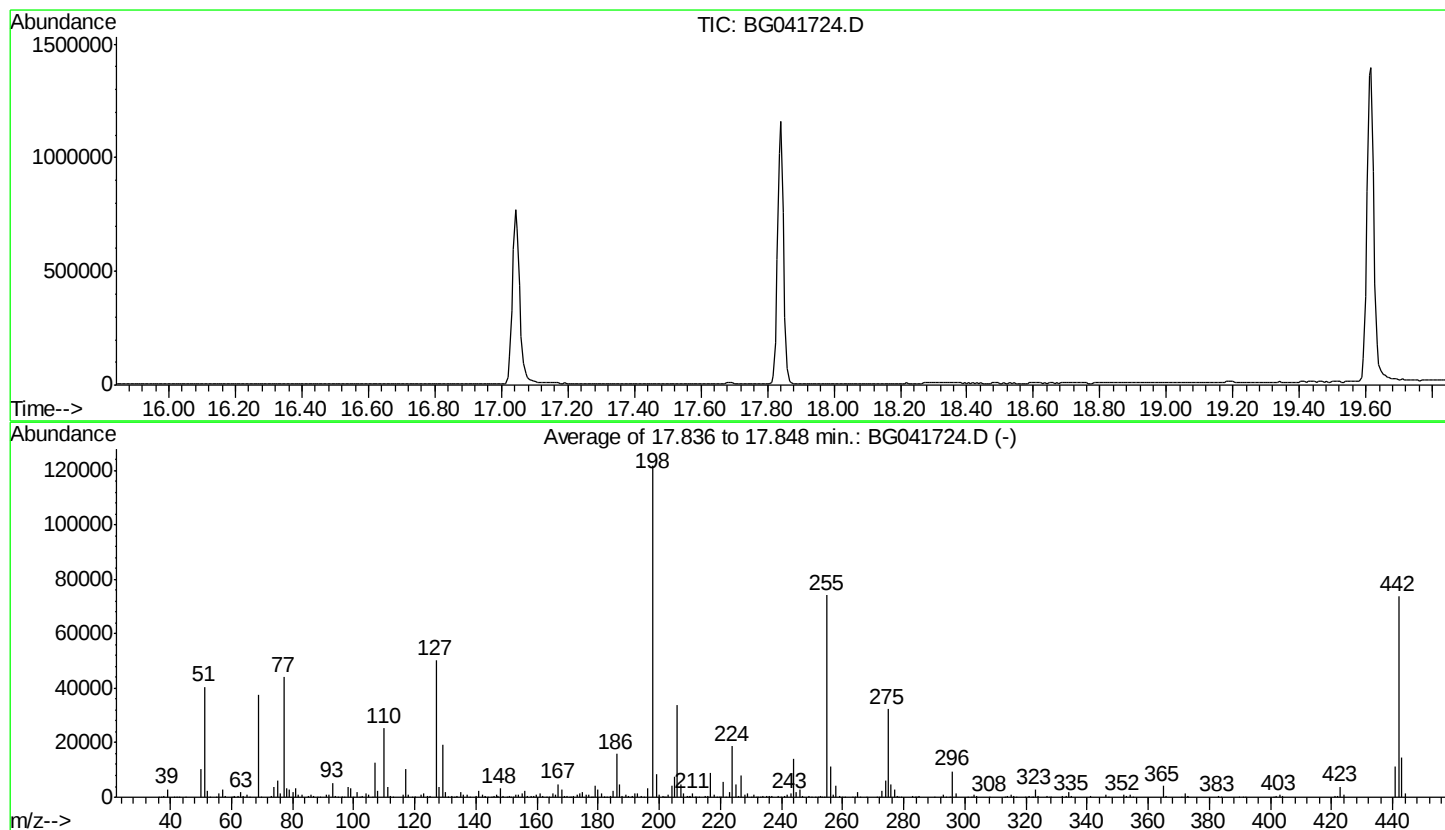

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	40592	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.9	37643	PASS
70	69	0.00	2	0.7	250	PASS
127	198	10	80	41.2	50210	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121730	PASS
199	198	5	9	7.2	8710	PASS
275	198	10	60	26.6	32394	PASS
365	198	1	100	3.5	4220	PASS
441	198	0.01	100	9.5	11513	PASS
442	198	50	100	60.5	73645	PASS
443	442	15	24	20.0	14750	PASS