
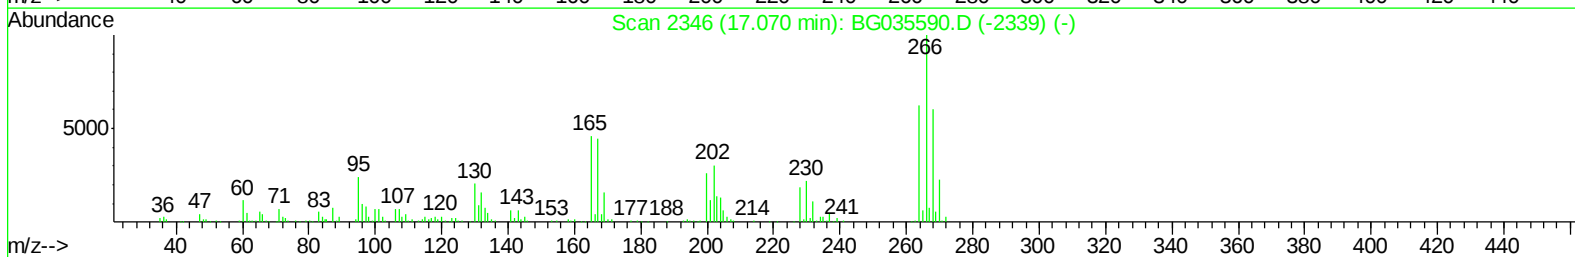
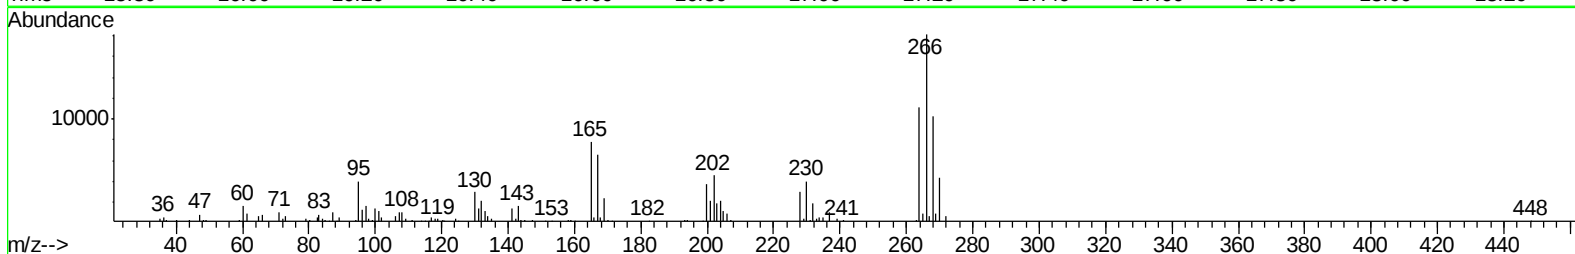


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072018\
Data File : BG035801.D
Acq On : 21 Jul 2018 2:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 02:31:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 15:28:54 2018
Response via : Initial Calibration

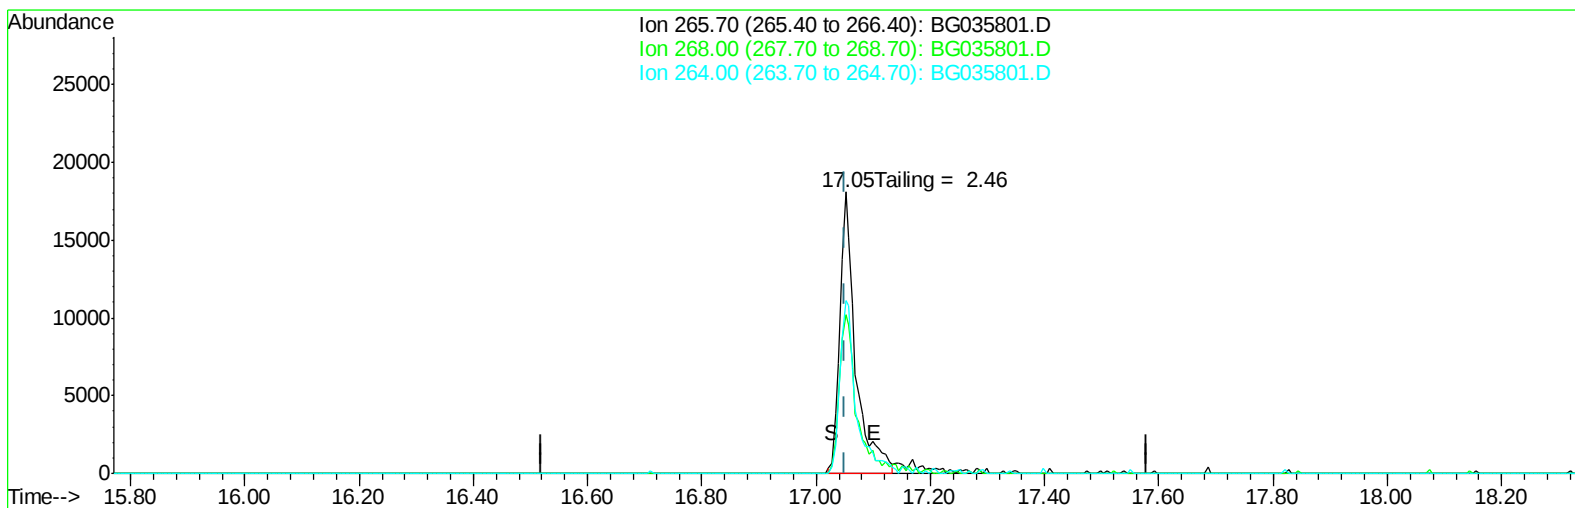

TIC: BG035801.D

(69) Pentachlorophenol (C)




17.051min (-0.000) 12480.08ng

response 34784

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	56.32
264.00	62.00	61.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072018\
Data File : BG035801.D
Acq On : 21 Jul 2018 2:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 02:31:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 15:28:54 2018
Response via : Initial Calibration

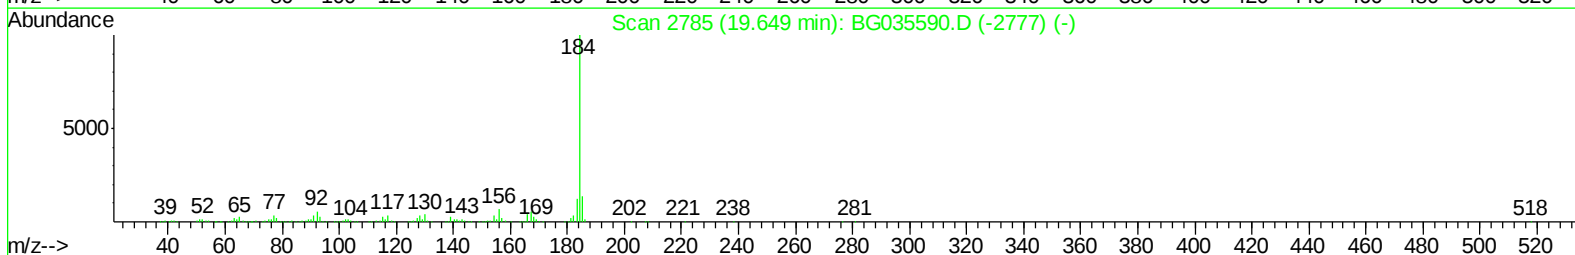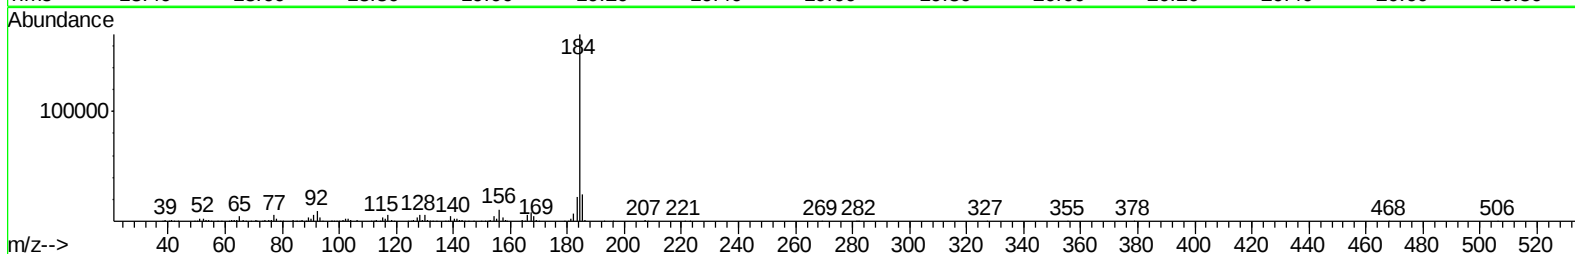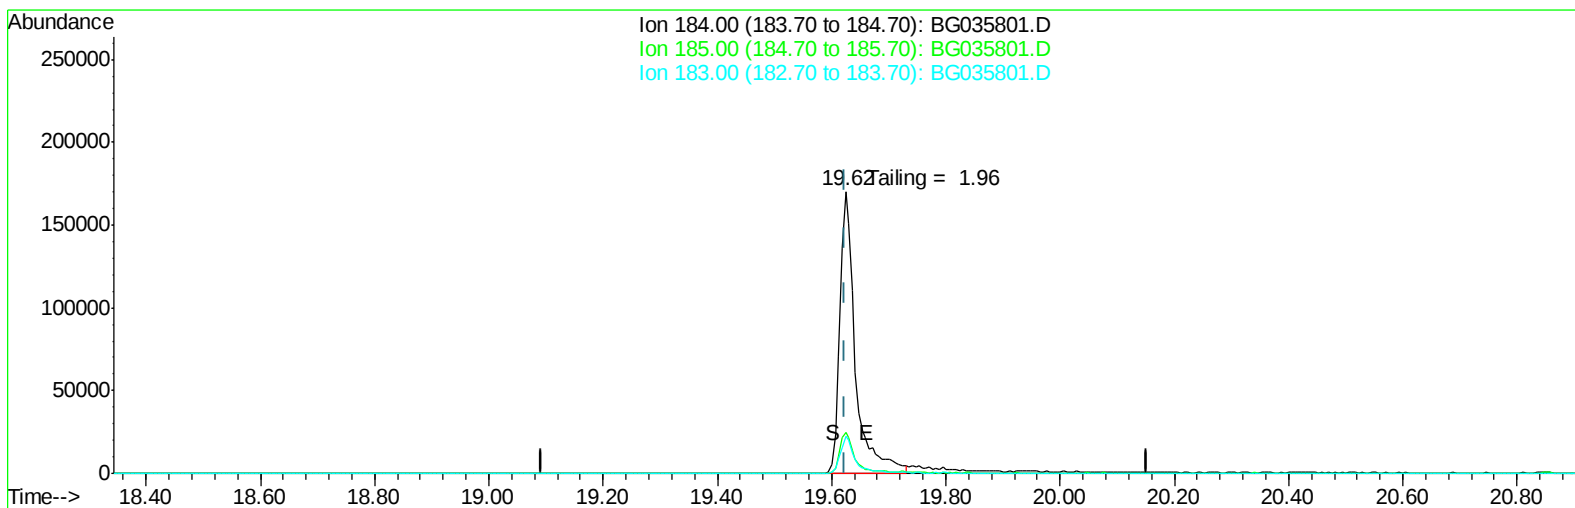

TIC: BG035801.D

(76) Benzidine

19.624min (-0.000) 217578.32ng

response 331771

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.37
183.00	13.30	13.35
0.00	0.00	0.00