


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072018\
 Data File : BG035782.D
 Acq On : 20 Jul 2018 13:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

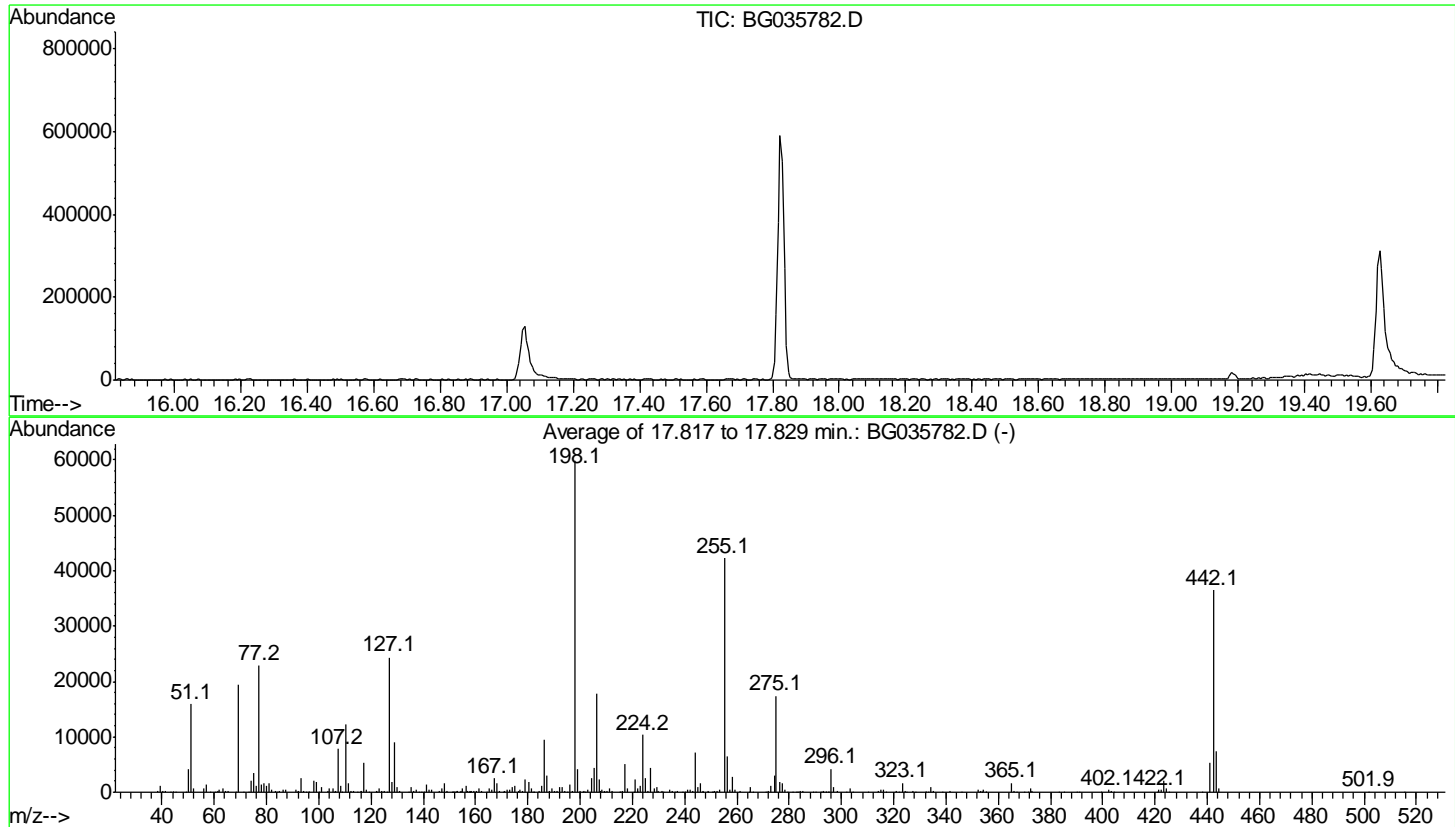

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	15898	PASS
68	69	0.00	2	0.6	113	PASS
69	198	0.00	100	32.6	19541	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.6	24333	PASS
197	198	0.00	2	0.5	271	PASS
198	198	100	100	100.0	59888	PASS
199	198	5	9	7.0	4169	PASS
275	198	10	60	29.0	17390	PASS
365	198	1	100	2.8	1680	PASS
441	198	0.01	100	9.1	5424	PASS
442	198	50	100	61.0	36509	PASS
443	442	15	24	20.0	7292	PASS