

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
 Data File : BG058385.D
 Acq On : 21 Jul 2023 13:11
 Operator : CG/JU
 Sample : 03504-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A46W9

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

Quant Time: Jul 21 22:34:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	46574	20.000	ng/u1	0.00
20) Naphthalene-d8	10.695	136	206106	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.532	164	140839	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.276	188	302970	20.000	ng/u1	0.00
79) Chrysene-d12	21.530	240	243314	20.000	ng/u1	0.00
88) Perylene-d12	24.661	264	306921	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.339	96	1289	1.019	ng/uL	0.00
4) Pyridine-d5	3.745	84	31497	8.386	ng/u1	0.00
7) Phenol-d5	7.064	99	24006	5.433	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.217	67	15461	5.599	ng/u1	0.00
11) 2-Chlorophenol-d4	7.429	132	17697	5.722	ng/u1	0.00
15) 4-Methylphenol-d8	8.604	113	7209	2.139	ng/u1	0.00
21) Nitrobenzene-d5	9.056	128	8856	5.732	ng/u1	0.00
24) 2-Nitrophenol-d4	9.779	143	9369	5.555	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.325	165	16889	5.224	ng/u1	0.00
31) 4-Chloroaniline-d4	10.807	131	360	0.077	ng/u1	-0.03
46) Dimethylphthalate-d6	13.933	166	57623	5.306	ng/u1	0.00
49) Acenaphthylene-d8	14.227	160	63235	5.556	ng/u1	0.00
54) 4-Nitrophenol-d4	14.755	143	3635	2.216	ng/u1	0.02
60) Fluorene-d10	15.519	176	50930	5.664	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.648	200	2677	1.734	ng/u1	0.00
73) Anthracene-d10	17.376	188	71415	5.455	ng/u1	0.00
81) Pyrene-d10	19.667	212	74828	5.207	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.444	264	48407	3.263	ng/u1	0.00
Target Compounds					Qvalue	
6) Benzaldehyde	7.035	77	2441	1.368	ng/u1	97
8) Phenol	7.094	94	6622	1.443	ng/u1	94
16) Acetophenone	8.715	105	26198	4.565	ng/u1	95
30) Naphthalene	10.748	128	134332	12.194	ng/u1	99
36) 2-Methylnaphthalene	12.352	142	58071	7.868	ng/u1	98
37) 1-Methylnaphthalene	12.576	142	40444	5.346	ng/u1	93
43) 1,1'-Biphenyl	13.363	154	20944	2.199	ng/u1	97
52) Acenaphthene	14.597	153	203809	23.894	ng/u1	99
56) Dibenzofuran	14.932	168	223833	18.429	ng/u1	99
61) Fluorene	15.578	166	254224	25.524	ng/u1	97
72) Phenanthrene	17.323	178	1785388m	124.003	ng/u1	
74) Anthracene	17.411	178	559578	38.714	ng/u1	99
77) Carbazole	17.681	167	175607	14.015	ng/u1	97
80) Fluoranthene	19.338	202	1543989	93.783	ng/u1	98
82) Pyrene	19.697	202	1032562	61.899	ng/u1	98
85) Benzo(a)anthracene	21.512	228	689614	42.167	ng/u1	97
86) Bis(2-ethylhexyl)phtha...	21.412	149	21618	2.314	ng/u1	100
87) Chrysene	21.577	228	639041m	41.195	ng/u1	
90) Benzo(b)fluoranthene	23.674	252	646742	36.419	ng/u1#	97
91) Benzo(k)fluoranthene	23.727	252	275804m	15.572	ng/u1	
93) Benzo(a)pyrene	24.514	252	248116	15.709	ng/u1	97
94) Indeno(1,2,3-cd)pyrene	28.228	276	204137	9.809	ng/u1	98
95) Dibenzo(a,h)anthracene	28.263	278	82029	4.807	ng/u1#	93

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
 Data File : BG058385.D
 Acq On : 21 Jul 2023 13:11
 Operator : CG/JU
 Sample : 03504-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A46W9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

Quant Time: Jul 21 22:34:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
Data File : BG058385.D
Acq On : 21 Jul 2023 13:11
Operator : CG/JU
Sample : 03504-11
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
A46W9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023


Quant Time: Jul 21 22:34:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 18 02:19:39 2023
Response via : Initial Calibration

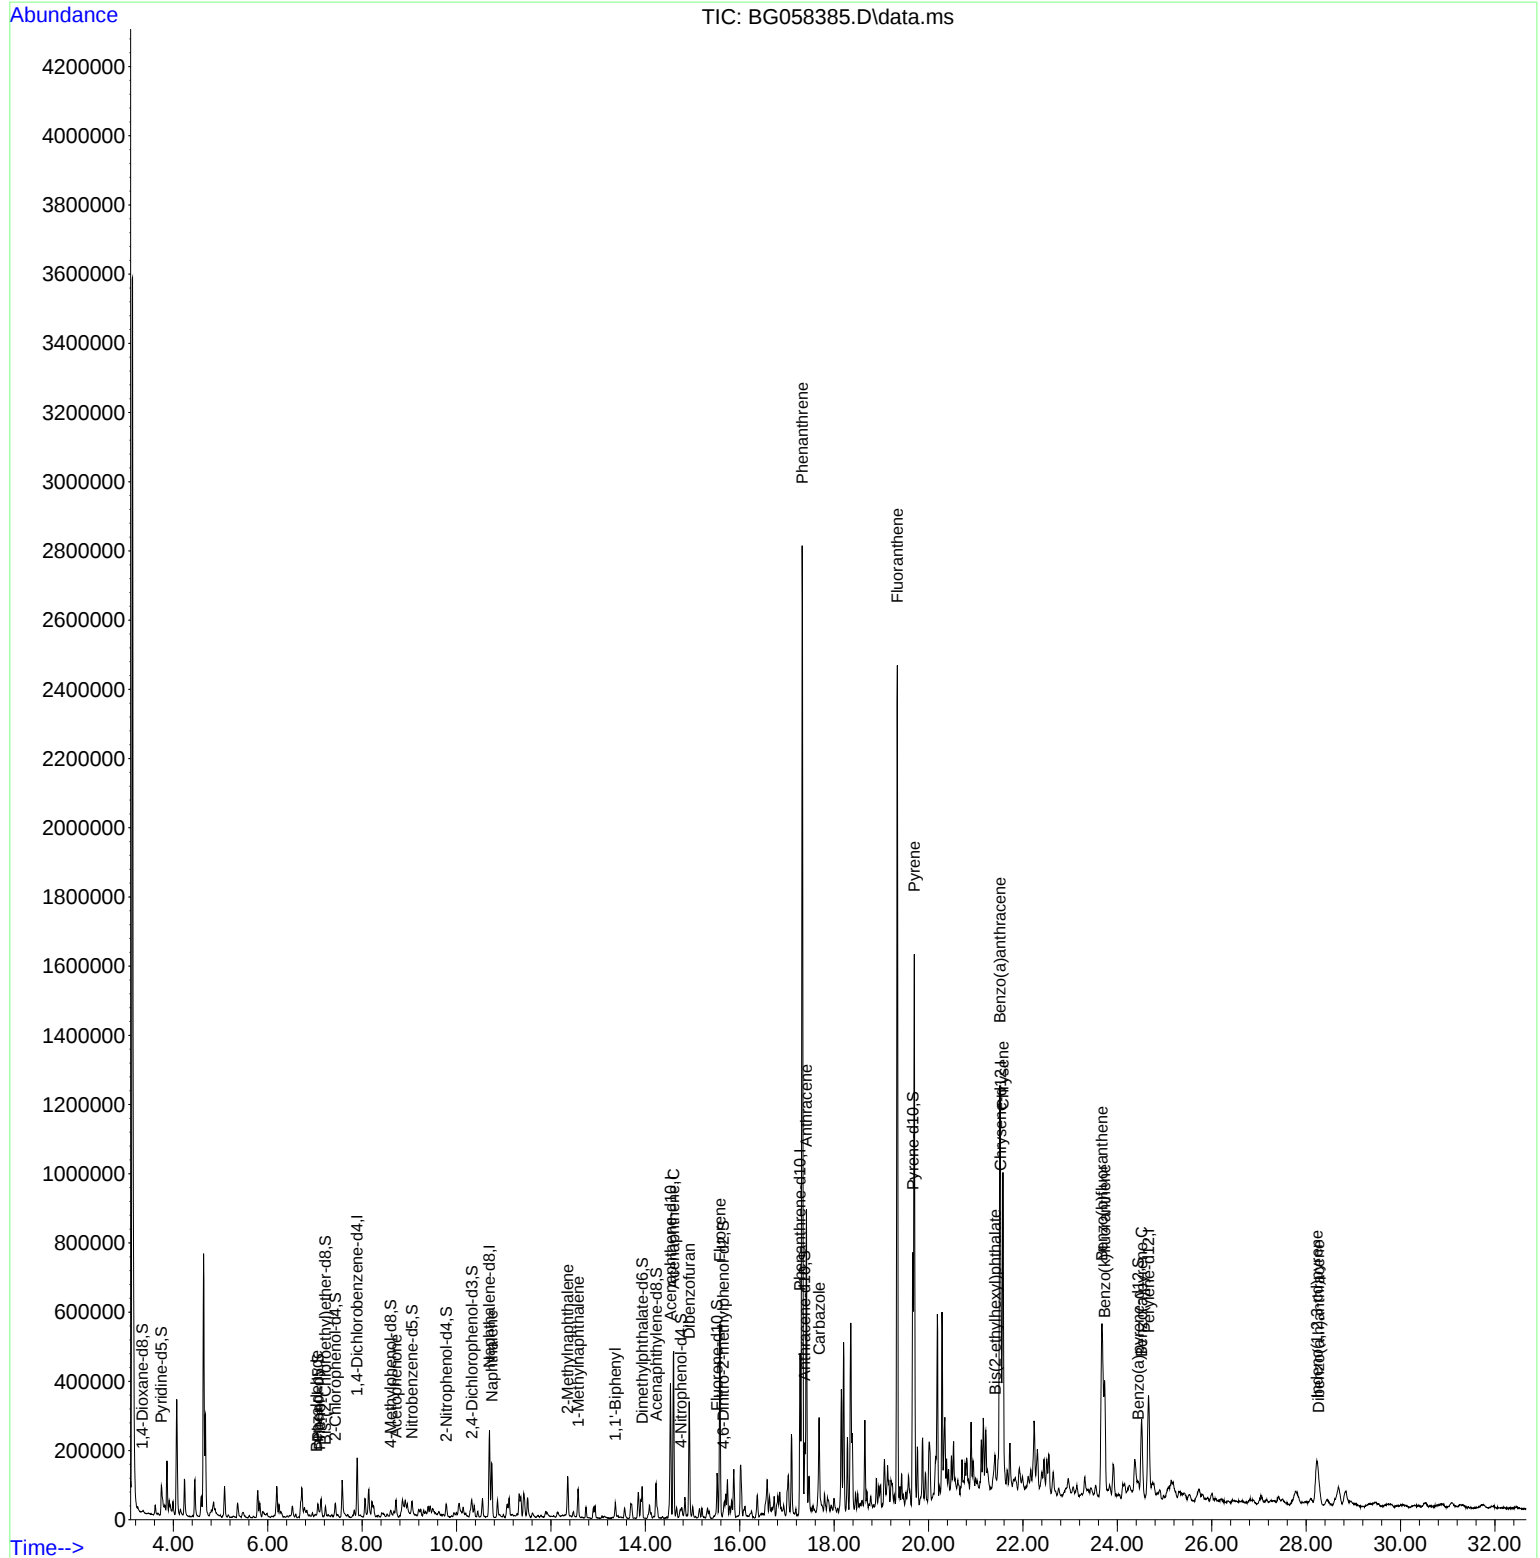



#6
Benzaldehyde
Concen: 1.368 ng/ul
RT: 7.035 min Scan# 611
Delta R.T. -0.000 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Instrument :
BNA_G
ClientSampleId :
A46W9



Tgt Ion: 77 Resp: 244
Ion Ratio Lower Upper
77 100
105 102.6 78.2 117.4
106 89.7 71.6 107.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023

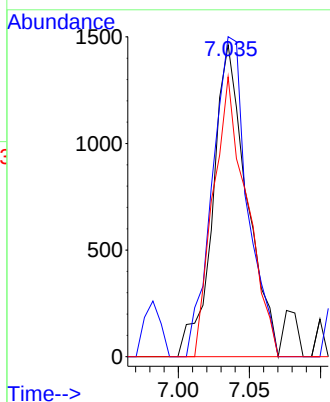

#8
Phenol
Concen: 1.443 ng/ul
RT: 7.094 min Scan# 682
Delta R.T. 0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11


Tgt Ion: 94 Resp: 6622
Ion Ratio Lower Upper
94 100
65 24.2 23.8 35.8
66 40.7 31.2 46.8

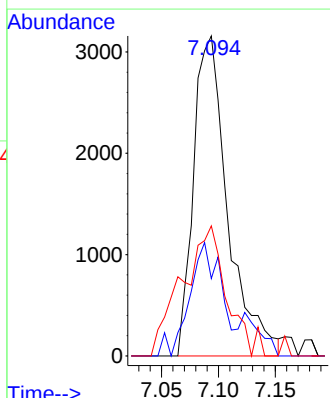



#16
Acetophenone
Concen: 4.565 ng/ul
RT: 8.715 min Scan# 91
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Instrument :
BNA_G
ClientSampleId :
A46W9




Tgt Ion:105 Resp: 26198
Ion Ratio Lower Upper
105 100
77 80.2 60.7 91.1
51 27.5 23.5 35.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023

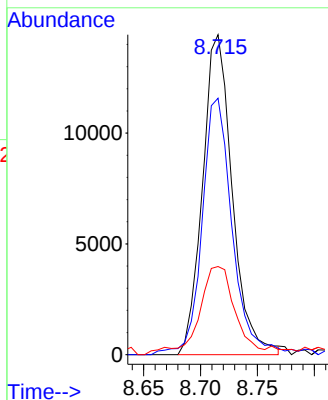


#30
Naphthalene
Concen: 12.194 ng/ul
RT: 10.748 min Scan# 1304
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11



Tgt Ion:128 Resp: 134332
Ion Ratio Lower Upper
128 100
129 10.9 8.8 13.2
127 13.0 10.8 16.2

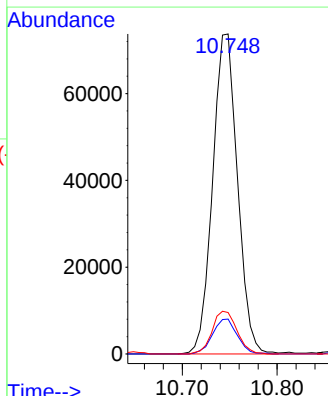







#36
2-Methylnaphthalene
Concen: 7.868 ng/ul
RT: 12.352 min Scan# 11
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11

Instrument :
BNA_G
ClientSampleId :
A46W9

Tgt Ion:142 Resp: 5807
Ion Ratio Lower Upper
142 100
141 92.8 72.6 108.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023



#37
1-Methylnaphthalene
Concen: 5.346 ng/ul
RT: 12.576 min Scan# 1615
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11


Tgt Ion:142 Resp: 40444
Ion Ratio Lower Upper
142 100
141 87.7 75.8 113.6
116 4.1 3.2 4.8

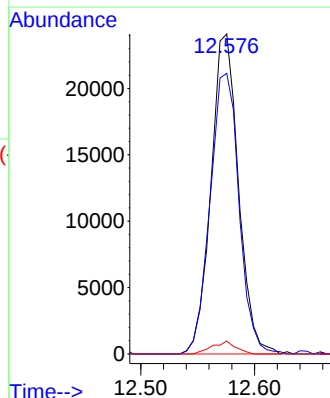



#43
1,1'-Biphenyl
Concen: 2.199 ng/ul
RT: 13.363 min Scan# 11
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Instrument :
BNA_G
ClientSampleId :
A46W9



Tgt Ion:154 Resp: 20944
Ion Ratio Lower Upper
154 100
153 38.1 31.8 47.6
76 15.8 11.7 17.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023



#52
Acenaphthene
Concen: 23.894 ng/ul
RT: 14.597 min Scan# 1959
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11

Tgt Ion:153 Resp: 203809
Ion Ratio Lower Upper
153 100
152 47.6 39.1 58.7
154 85.2 68.7 103.1

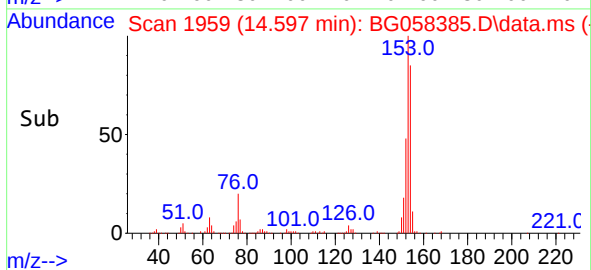







#56
Dibenzofuran
Concen: 18.429 ng/ul
RT: 14.932 min Scan# 2015
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11

Instrument :
BNA_G
ClientSampleId :
A46W9

Tgt Ion:168 Resp: 22383
Ion Ratio Lower Upper
168 100
139 35.4 27.8 41.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023

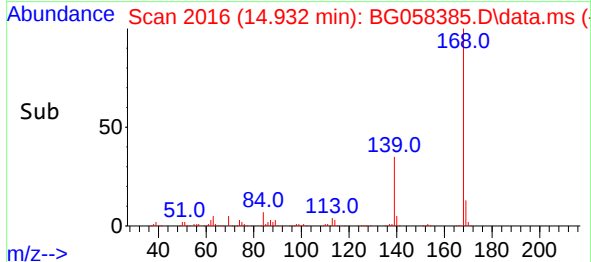

#61
Fluorene
Concen: 25.524 ng/ul
RT: 15.578 min Scan# 2126
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11


Tgt Ion:166 Resp: 254224
Ion Ratio Lower Upper
166 100
165 97.3 80.2 120.2
167 13.0 10.5 15.7

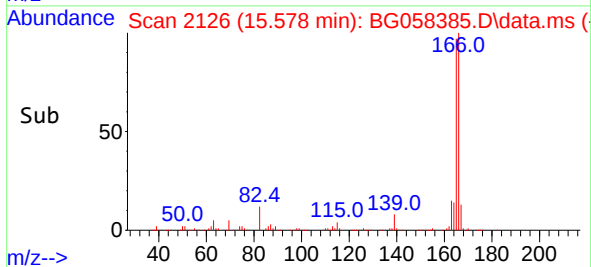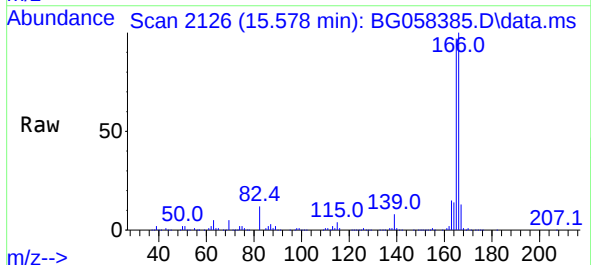



#72
Phenanthrene
Concen: 124.003 ng/ul m
RT: 17.323 min Scan# 2422
Delta R.T. -0.000 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Instrument :
BNA_G
ClientSampleId :
A46W9




Tgt Ion:178 Resp: 1785388
Ion Ratio Lower Upper
178 100
179 18.1 11.9 17.9
176 22.3 15.8 23.8

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023

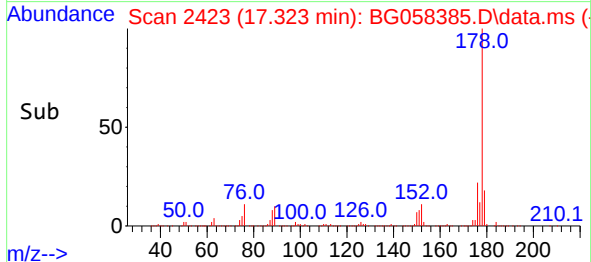


#74
Anthracene
Concen: 38.714 ng/ul
RT: 17.411 min Scan# 2438
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Tgt Ion:178 Resp: 559578
Ion Ratio Lower Upper
178 100
179 16.5 13.4 20.2
176 19.3 16.2 24.2

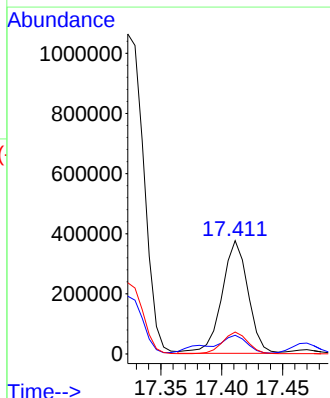



#77
 Carbazole
 Concen: 14.015 ng/ul
 RT: 17.681 min Scan# 2483
 Delta R.T. -0.000 min
 Lab File: BG058385.D
 Acq: 21 Jul 2023 13:11




Instrument :
 BNA_G
 ClientSampleId :
 A46W9




Tgt Ion:167 Resp: 175607
 Ion Ratio Lower Upper
 167 100
 166 20.9 17.8 26.8
 139 12.4 9.4 14.0

Manual Integrations
 APPROVED



Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

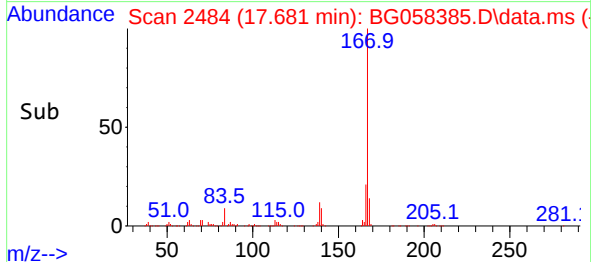


#80
 Fluoranthene
 Concen: 93.783 ng/ul
 RT: 19.338 min Scan# 2766
 Delta R.T. 0.006 min
 Lab File: BG058385.D
 Acq: 21 Jul 2023 13:11




Tgt Ion:202 Resp: 1543989
 Ion Ratio Lower Upper
 202 100
 101 11.9 8.6 12.8
 100 9.5 7.2 10.8

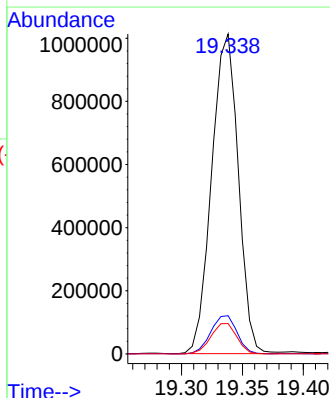



#82
Pyrene
Concen: 61.899 ng/ul
RT: 19.697 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Instrument :
BNA_G
ClientSampleId :
A46W9




Tgt Ion:202 Resp: 103256
Ion Ratio Lower Upper
202 100
101 13.6 10.2 15.2
100 11.7 8.9 13.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023

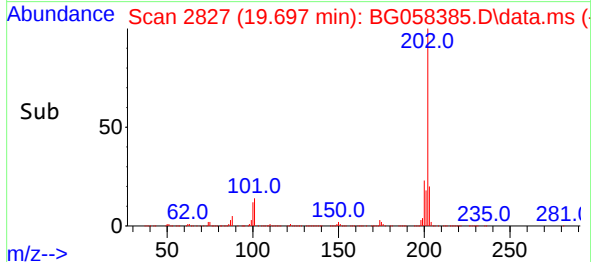


#85
Benzo(a)anthracene
Concen: 42.167 ng/ul
RT: 21.512 min Scan# 3136
Delta R.T. -0.000 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Tgt Ion:228 Resp: 689614
Ion Ratio Lower Upper
228 100
229 21.5 15.7 23.5
226 28.7 21.8 32.8

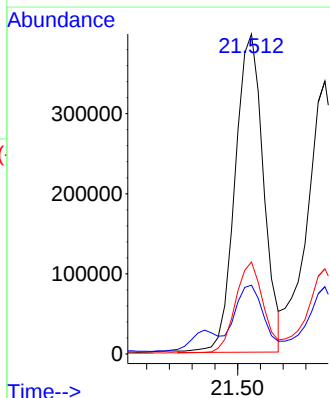



#86
Bis(2-ethylhexyl)phthalate
Concen: 2.314 ng/ul
RT: 21.412 min Scan# 3119
Delta R.T. -0.000 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Instrument :
BNA_G
ClientSampleId :
A46W9



Tgt Ion:149 Resp: 21618
Ion Ratio Lower Upper
149 100
167 26.8 21.6 32.4
279 3.3 3.0 4.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023



#87
Chrysene
Concen: 41.195 ng/ul m
RT: 21.577 min Scan# 3147
Delta R.T. -0.000 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11


Tgt Ion:228 Resp: 639041
Ion Ratio Lower Upper
228 100
226 31.2 24.0 36.0
229 24.6 15.8 23.8#

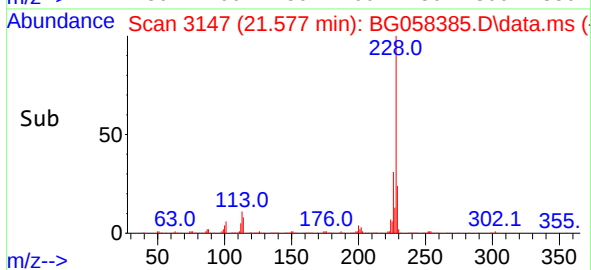



#90
Benzo(b)fluoranthene
Concen: 36.419 ng/ul
RT: 23.674 min Scan# 3504
Delta R.T. 0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Instrument :
BNA_G
ClientSampleId :
A46W9




Tgt Ion:252 Resp: 646742
Ion Ratio Lower Upper
252 100
253 23.4 17.9 26.9
125 10.3 6.7 10.1

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023




#91
Benzo(k)fluoranthene
Concen: 15.572 ng/ul m
RT: 23.727 min Scan# 3513
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Tgt Ion:252 Resp: 275804
Ion Ratio Lower Upper
252 100
253 22.9 18.3 27.5
125 10.7 7.4 11.0

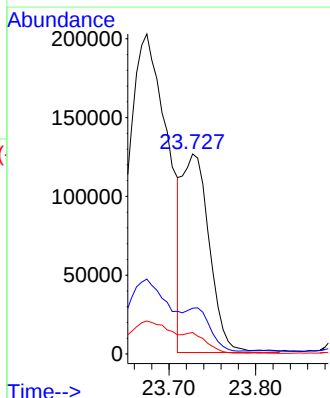



#93
Benzo(a)pyrene
Concen: 15.709 ng/ul
RT: 24.514 min Scan# 30
Delta R.T. -0.006 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11




Instrument :
BNA_G
ClientSampleId :
A46W9



Tgt Ion:252 Resp: 248110
Ion Ratio Lower Upper
252 100
253 23.7 17.4 26.0
125 9.7 7.7 11.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/22/2023
Supervised By :mohammad ahmed 07/22/2023



#94
Indeno(1,2,3-cd)pyrene
Concen: 9.809 ng/ul
RT: 28.228 min Scan# 4279
Delta R.T. -0.000 min
Lab File: BG058385.D
Acq: 21 Jul 2023 13:11


Tgt Ion:276 Resp: 204137
Ion Ratio Lower Upper
276 100
138 18.4 13.8 20.6
277 25.0 19.2 28.8

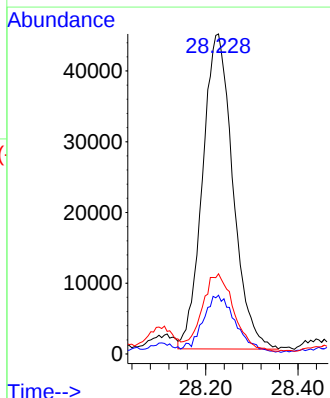



#95
 Dibenzo(a,h)anthracene
 Concen: 4.807 ng/ul
 RT: 28.263 min Scan# 41
 Delta R.T. -0.030 min
 Lab File: BG058385.D
 Acq: 21 Jul 2023 13:11

Instrument :
 BNA_G
 ClientSampleId :
 A46W9



Tgt Ion:278 Resp: 82029
 Ion Ratio Lower Upper
 278 100
 139 13.6 10.4 15.6
 279 27.8 18.4 27.6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2023
 Supervised By :mohammad ahmed 07/22/2023

