

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
 Data File : BG058380.D
 Acq On : 21 Jul 2023 9:38
 Operator : CG/JU
 Sample : PB154123BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK123

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.338	37	42	49	rVB2	17666	27963	1.74%	0.184%
2	3.743	107	111	128	rBV	207807	374425	23.30%	2.461%
3	4.078	166	168	176	rVB3	3159	4632	0.29%	0.030%
4	4.977	315	321	323	rBV3	998	1960	0.12%	0.013%
5	7.057	669	675	693	rBV	219684	389519	24.24%	2.561%
6	7.221	696	703	715	rVB	180698	309614	19.27%	2.035%
7	7.427	731	738	749	rBV	209931	371479	23.12%	2.442%
8	7.891	811	817	827	rBV	157509	275934	17.17%	1.814%
9	8.596	930	937	954	rBV	243437	454062	28.26%	2.985%
10	9.055	1007	1015	1030	rBV	207430	380456	23.68%	2.501%
11	9.777	1131	1138	1152	rBV	170346	306757	19.09%	2.017%
12	10.318	1223	1230	1246	rBV	236622	438418	27.29%	2.882%
13	10.694	1287	1294	1303	rBV	228474	404837	25.20%	2.661%
14	10.835	1310	1318	1330	rBV	245629	470182	29.26%	3.091%
15	12.286	1560	1565	1572	rVB3	3054	6007	0.37%	0.039%
16	13.414	1753	1757	1762	rBV2	2857	3991	0.25%	0.026%
17	13.937	1839	1846	1856	rBV	464870	721245	44.89%	4.741%
18	14.225	1888	1895	1906	rBV	551517	857765	53.39%	5.639%
19	14.530	1939	1947	1956	rBV	377091	571212	35.55%	3.755%
20	14.736	1976	1982	1999	rBV	136743	300135	18.68%	1.973%
21	15.523	2109	2116	2131	rBV	705975	1092425	67.99%	7.182%
22	15.641	2131	2136	2148	rVV	231361	350515	21.82%	2.304%
23	15.764	2153	2157	2163	rVB2	2913	4329	0.27%	0.028%
24	17.274	2408	2414	2424	rBV	502614	750262	46.70%	4.932%
25	17.374	2424	2431	2452	rVB2	800921	1231444	76.65%	8.096%
26	19.231	2743	2747	2752	rVV3	12346	17362	1.08%	0.114%
27	19.301	2755	2759	2766	rVB2	9378	14411	0.90%	0.095%
28	19.489	2785	2791	2792	rBV3	1305	2290	0.14%	0.015%
29	19.583	2803	2807	2810	rBV3	2431	2558	0.16%	0.017%
30	19.666	2814	2821	2836	rVV	1095664	1544497	96.13%	10.154%
31	20.153	2902	2904	2907	rBV4	1756	2112	0.13%	0.014%
32	21.170	3075	3077	3082	rBV5	5431	7799	0.49%	0.051%
33	21.223	3084	3086	3087	rBV2	2284	1779	0.11%	0.012%
34	21.270	3092	3094	3097	rBV4	2530	1814	0.11%	0.012%
35	21.528	3130	3138	3150	rBV2	499920	860808	53.58%	5.659%
36	21.699	3165	3167	3173	rVB6	6648	8981	0.56%	0.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
 Data File : BG058380.D
 Acq On : 21 Jul 2023 9:38
 Operator : CG/JU
 Sample : PB154123BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

37	22.292	3264	3268	3275	rVB8	9042	16148	1.01%	0.106%
38	22.545	3309	3311	3312	rVB2	3319	1627	0.10%	0.011%
39	22.956	3378	3381	3386	rVB4	6644	10886	0.68%	0.072%
40	23.502	3472	3474	3476	rBV2	2645	2397	0.15%	0.016%
41	23.690	3504	3506	3507	rBV2	3349	1975	0.12%	0.013%
42	23.731	3507	3513	3520	rVV5	12563	24610	1.53%	0.162%
43	24.448	3623	3635	3650	rBV2	568990	1606673	100.00%	10.562%
44	24.660	3660	3671	3686	rBV	335738	946294	58.90%	6.221%
45	25.494	3811	3813	3814	rBV2	2994	2060	0.13%	0.014%
46	25.735	3849	3854	3862	rVB5	10649	27039	1.68%	0.178%
47	28.602	4339	4342	4343	rBV3	3987	4931	0.31%	0.032%
48	29.155	4434	4436	4437	rBV2	3581	2732	0.17%	0.018%




Sum of corrected areas: 15211351

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
Data File : BG058380.D
Acq On : 21 Jul 2023 9:38
Operator : CG/JU
Sample : PB154123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

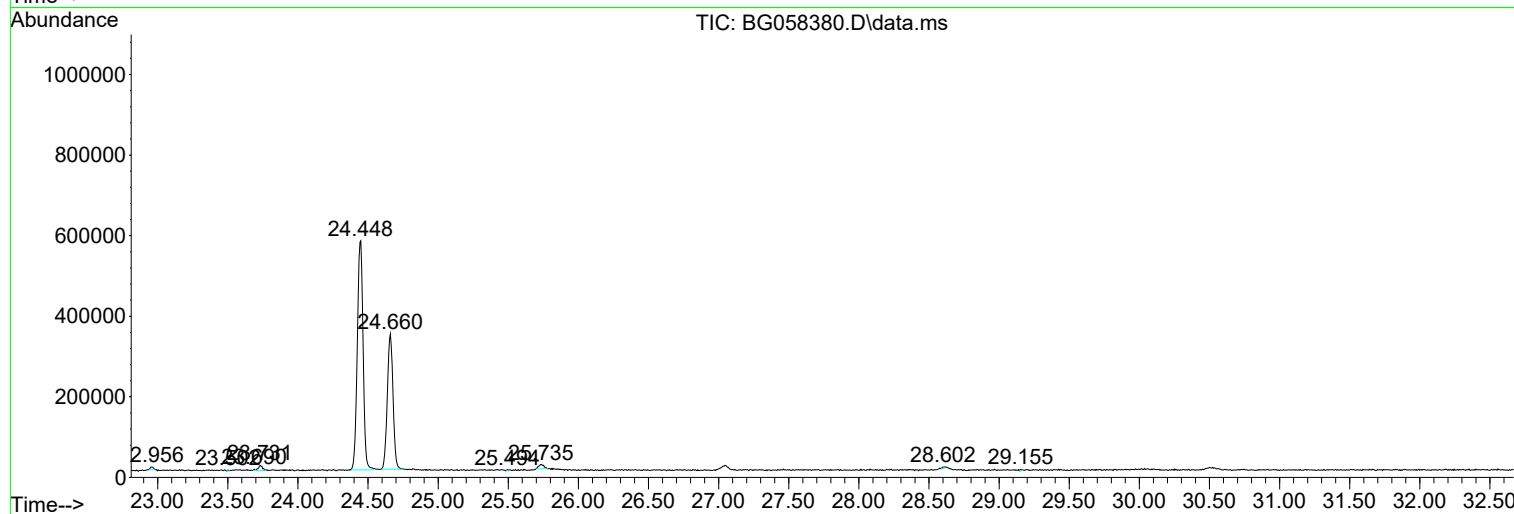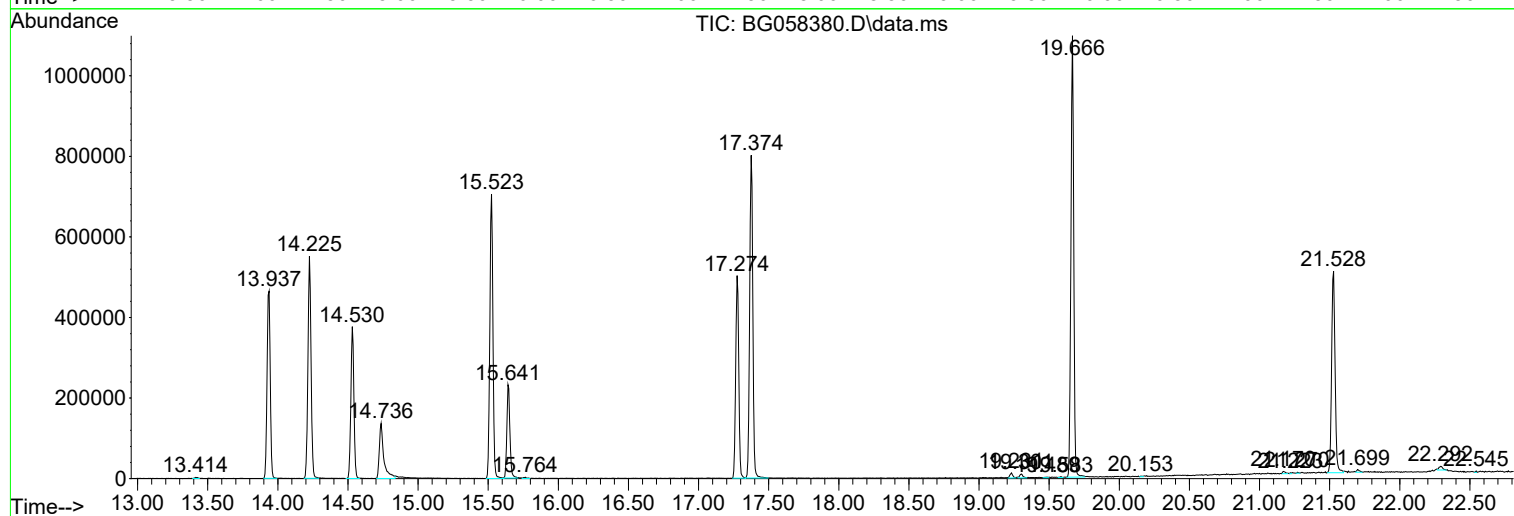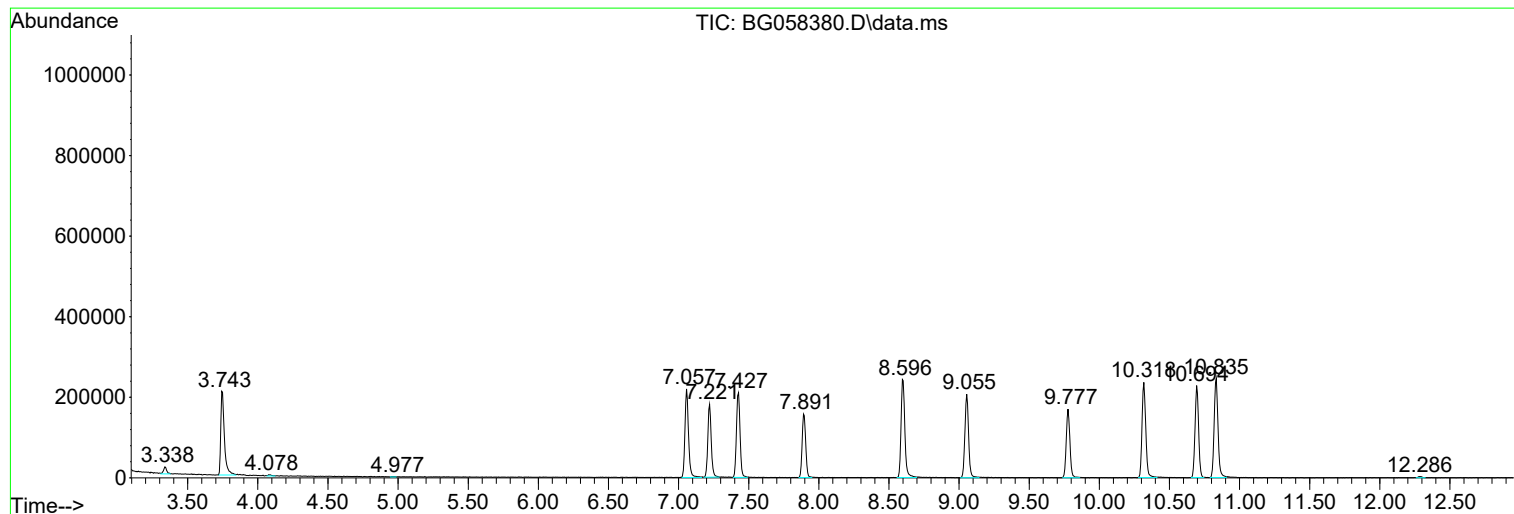

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
Data File : BG058380.D
Acq On : 21 Jul 2023 9:38
Operator : CG/JU
Sample : PB154123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
Data File : BG058380.D
Acq On : 21 Jul 2023 9:38
Operator : CG/JU
Sample : PB154123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc