

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
 Data File : BG058383.D
 Acq On : 21 Jul 2023 11:48
 Operator : CG/JU
 Sample : PB154123BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.335	38	42	49	rVB2	17534	26405	1.59%	0.165%
2	3.746	107	112	126	rBV	219092	375977	22.59%	2.352%
3	4.081	166	169	172	rBV2	3269	3972	0.24%	0.025%
4	7.060	669	676	693	rBV	222048	396954	23.85%	2.483%
5	7.218	695	703	715	rBV	182991	316321	19.00%	1.978%
6	7.424	731	738	752	rBV	215652	377597	22.69%	2.362%
7	7.894	811	818	833	rVB	161837	278002	16.70%	1.739%
8	8.599	931	938	959	rBV	260891	471624	28.33%	2.950%
9	9.052	1006	1015	1031	rBV	207368	387781	23.30%	2.425%
10	9.774	1131	1138	1147	rBV	166748	310364	18.65%	1.941%
11	10.315	1223	1230	1245	rBV	240038	451293	27.11%	2.823%
12	10.697	1287	1295	1303	rBV	233260	418689	25.15%	2.619%
13	10.832	1310	1318	1328	rBV	254749	480692	28.88%	3.006%
14	12.283	1560	1565	1572	rBV3	3117	5682	0.34%	0.036%
15	13.411	1753	1757	1763	rBV3	2843	4474	0.27%	0.028%
16	13.934	1840	1846	1856	rBV	521216	764465	45.93%	4.781%
17	14.228	1889	1896	1914	rBV2	551021	895492	53.80%	5.601%
18	14.533	1941	1948	1959	rVV	379221	601262	36.12%	3.761%
19	14.733	1976	1982	2001	rBV	147110	327986	19.71%	2.051%
20	14.980	2020	2024	2027	rVB2	1617	1879	0.11%	0.012%
21	15.526	2109	2117	2126	rBV	731595	1150464	69.12%	7.195%
22	15.644	2131	2137	2150	rVV	257751	385002	23.13%	2.408%
23	15.767	2154	2158	2162	rVB3	3463	5103	0.31%	0.032%
24	17.072	2370	2380	2384	rBV2	1327	3242	0.19%	0.020%
25	17.277	2408	2415	2425	rBV	526537	802353	48.20%	5.018%
26	17.377	2425	2432	2445	rVV	867830	1319689	79.29%	8.254%
27	19.228	2743	2747	2752	rBV3	12999	17461	1.05%	0.109%
28	19.298	2754	2759	2765	rVB	10930	17013	1.02%	0.106%
29	19.580	2805	2807	2812	rVB5	1530	2143	0.13%	0.013%
30	19.669	2812	2822	2833	rBV	1117131	1660624	99.77%	10.386%
31	21.032	3052	3054	3057	rBV4	1686	2060	0.12%	0.013%
32	21.173	3074	3078	3082	rBV5	4609	6549	0.39%	0.041%
33	21.349	3106	3108	3111	rBV3	2256	1895	0.11%	0.012%
34	21.525	3132	3138	3150	rBV2	529963	873556	52.48%	5.464%
35	21.701	3165	3168	3174	rVB7	6028	8993	0.54%	0.056%
36	22.107	3233	3237	3238	rBV4	3243	3099	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
 Data File : BG058383.D
 Acq On : 21 Jul 2023 11:48
 Operator : CG/JU
 Sample : PB154123BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK123

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

37	22.295	3264	3269	3274	rVB6	9971	19848	1.19%	0.124%
38	22.953	3378	3381	3387	rVB4	12253	20498	1.23%	0.128%
39	23.123	3408	3410	3413	rBV4	2734	2421	0.15%	0.015%
40	23.734	3509	3514	3519	rBV4	12682	24731	1.49%	0.155%
41	24.199	3592	3593	3595	rVB2	4032	2294	0.14%	0.014%
42	24.445	3624	3635	3650	rBV2	591297	1664469	100.00%	10.410%
43	24.657	3661	3671	3685	rVB	356884	991297	59.56%	6.200%
44	25.068	3739	3741	3743	rVB2	3874	2141	0.13%	0.013%
45	25.732	3849	3854	3855	rBV4	13499	21000	1.26%	0.131%
46	26.461	3977	3978	3980	rBV	4280	2643	0.16%	0.017%
47	27.001	4068	4070	4071	rBV2	5268	4553	0.27%	0.028%
48	27.036	4072	4076	4087	rVB7	16335	50031	3.01%	0.313%
49	28.605	4335	4343	4344	rBV7	10260	22509	1.35%	0.141%
50	31.079	4762	4764	4767	rBV4	2704	1892	0.11%	0.012%
51	31.161	4776	4778	4780	rBV3	2900	2307	0.14%	0.014%


Sum of corrected areas: 15988791

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
Data File : BG058383.D
Acq On : 21 Jul 2023 11:48
Operator : CG/JU
Sample : PB154123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

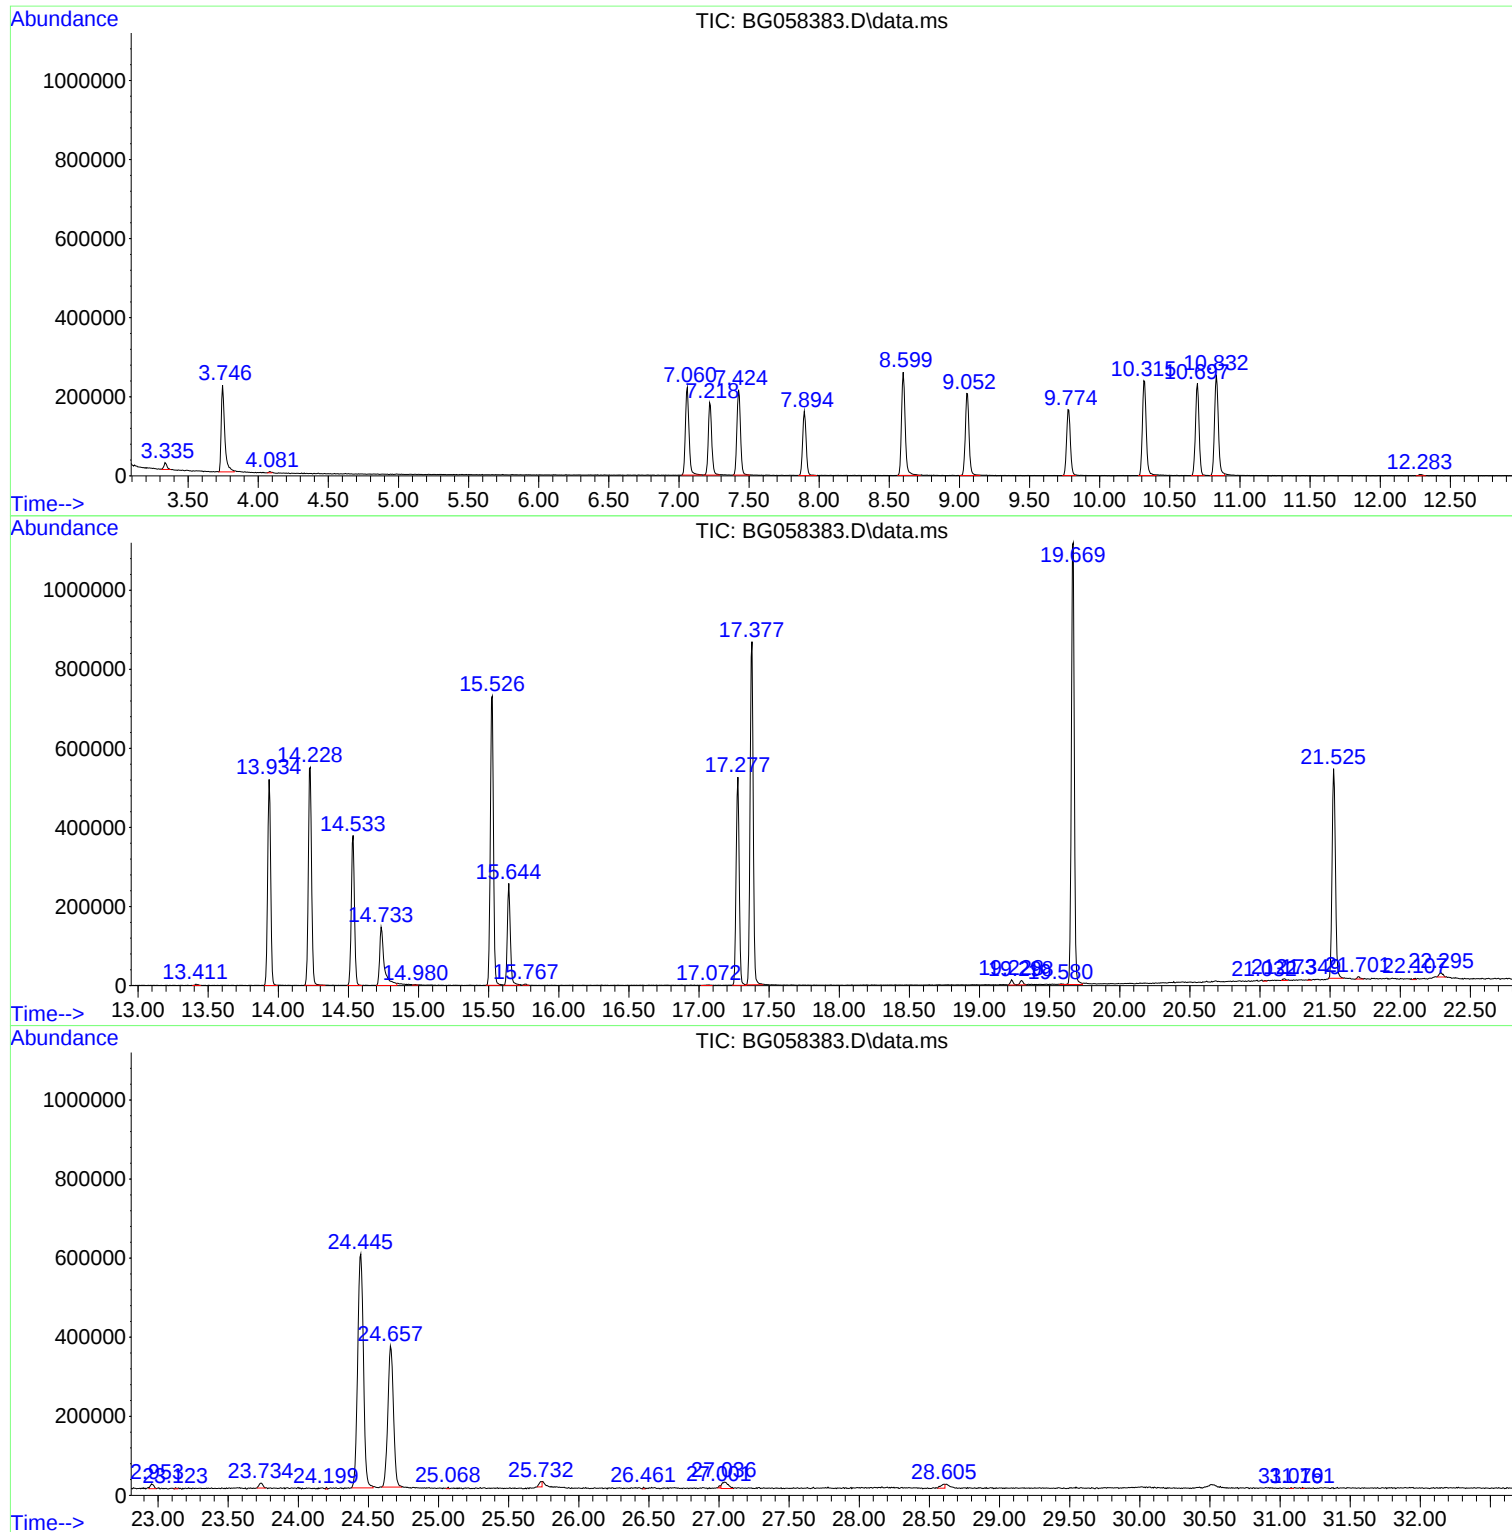

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
Data File : BG058383.D
Acq On : 21 Jul 2023 11:48
Operator : CG/JU
Sample : PB154123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072123\
Data File : BG058383.D
Acq On : 21 Jul 2023 11:48
Operator : CG/JU
Sample : PB154123BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc