




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
 Data File : BG058409.D
 Acq On : 22 Jul 2023 20:13
 Operator : CG/JU
 Sample : 03536-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW60

Manual IntegrationsAPPROVED

Quant Time: Jul 23 01:32:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

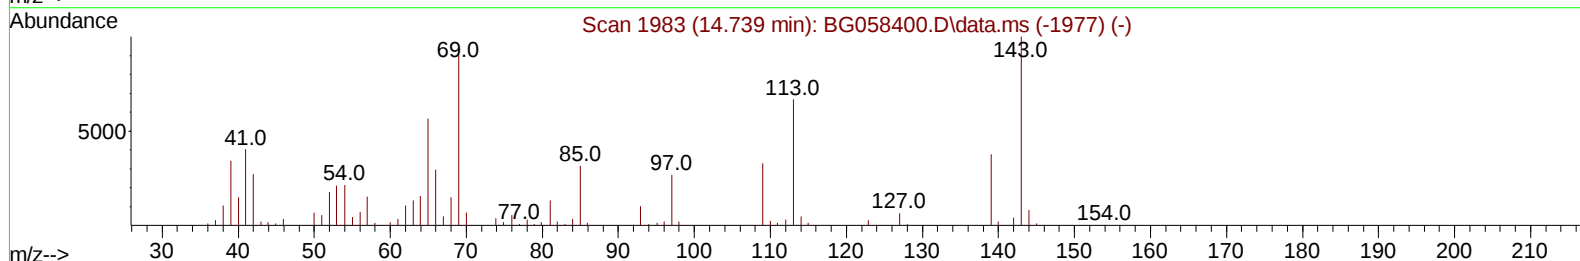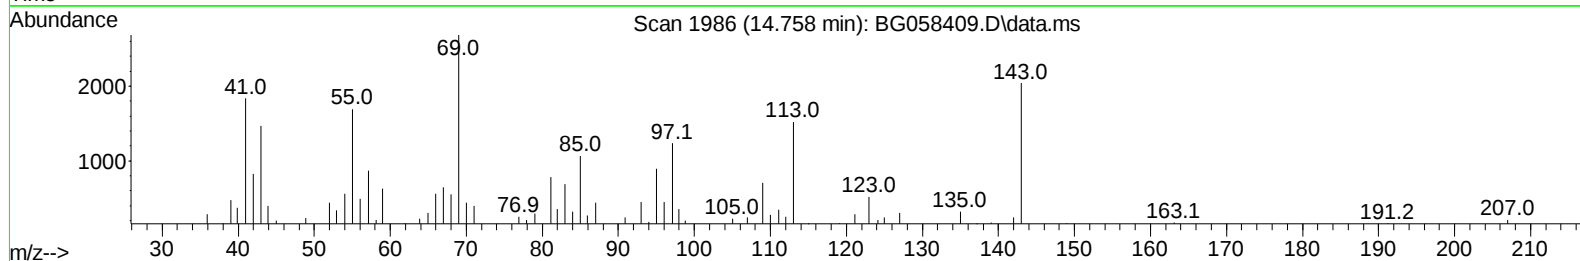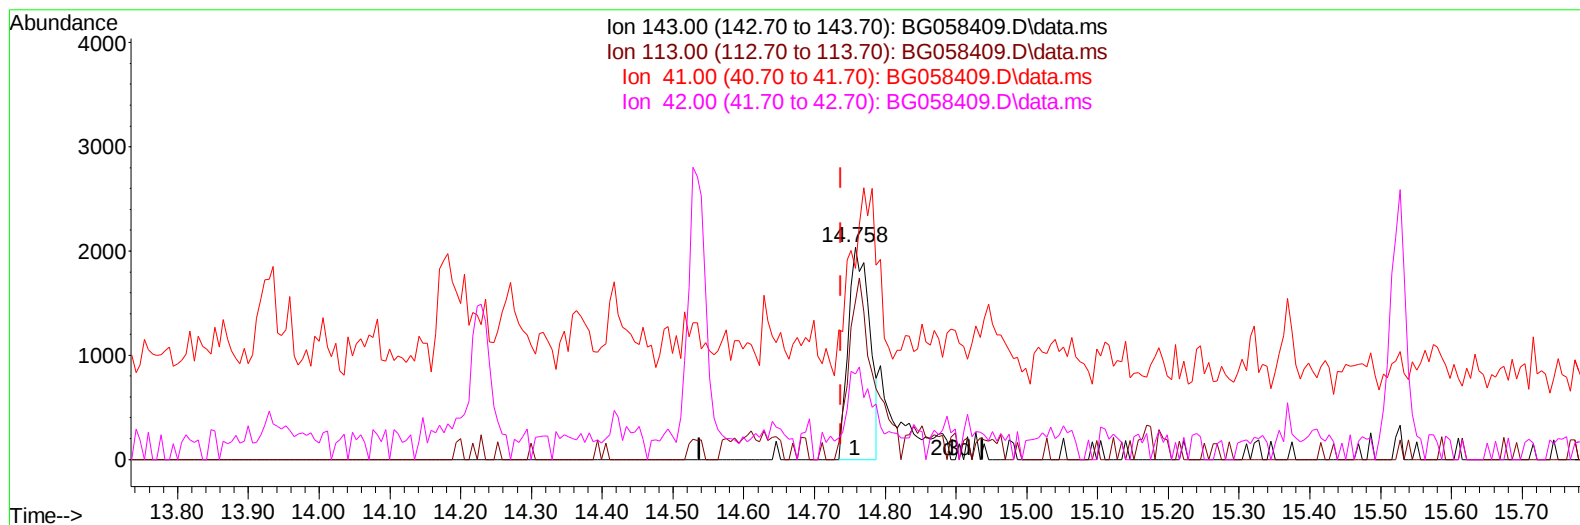

TIC: BG058409.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.758min (+ 0.020) 2.36 ng/ul

response 4277

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	67.80	74.55
41.00	46.40	89.95#
42.00	30.60	40.31#




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
 Data File : BG058409.D
 Acq On : 22 Jul 2023 20:13
 Operator : CG/JU
 Sample : 03536-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW60

Manual IntegrationsAPPROVED

Quant Time: Jul 23 01:32:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

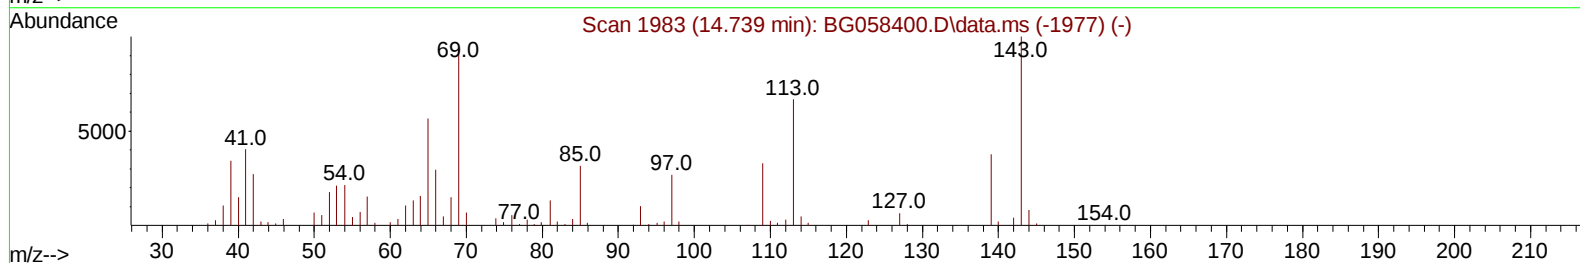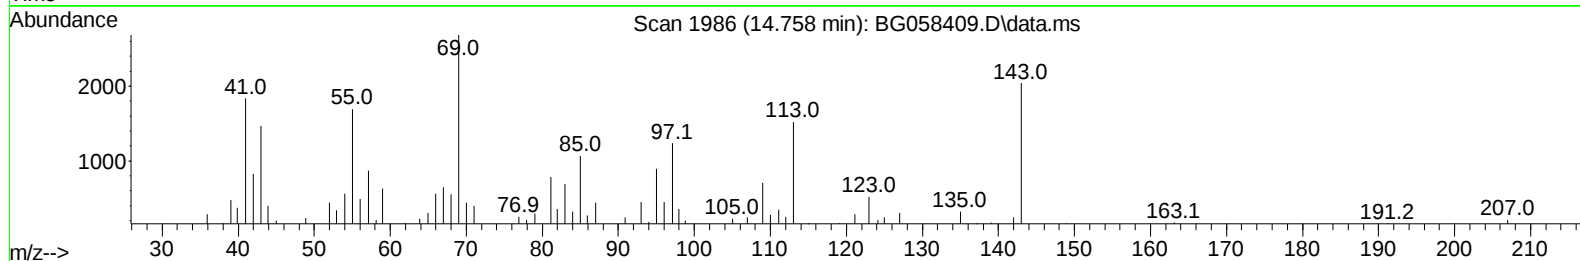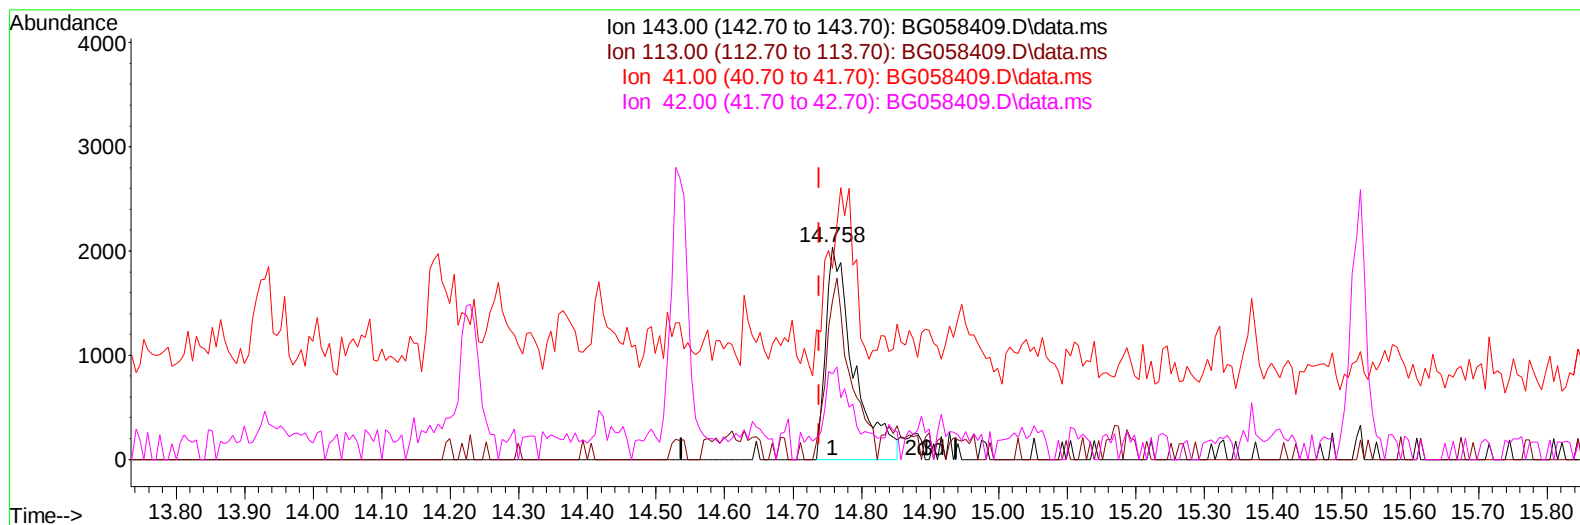

TIC: BG058409.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.758min (+ 0.020) 3.20 ng/ul m

response 5789

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	67.80	74.55
41.00	46.40	89.95#
42.00	30.60	40.31#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
 Data File : BG058409.D
 Acq On : 22 Jul 2023 20:13
 Operator : CG/JU
 Sample : 03536-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YBW60

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/24/2023
 Supervised By :mohammad ahmed 07/24/2023

Quant Time: Jul 23 02:41:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 18 02:19:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.895	152	58374	20.000	ng/ul	0.00
20) Naphthalene-d8	10.698	136	248657	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.534	164	155316	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.278	188	319794	20.000	ng/ul	0.00
79) Chrysene-d12	21.532	240	257486	20.000	ng/ul	0.00
88) Perylene-d12	24.681	264	312765	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.342	96	3151	1.987	ng/uL	0.00
4) Pyridine-d5	3.747	84	56158	11.930	ng/ul	0.00
7) Phenol-d5	7.067	99	57325	10.352	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.225	67	45617	13.180	ng/ul	0.00
11) 2-Chlorophenol-d4	7.431	132	43638	11.258	ng/ul	0.00
15) 4-Methylphenol-d8	8.612	113	9024	2.136	ng/ul	0.00
21) Nitrobenzene-d5	9.059	128	27271	14.632	ng/ul	0.00
24) 2-Nitrophenol-d4	9.775	143	23348	11.475	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	37851	9.704	ng/ul	0.00
31) 4-Chloroaniline-d4	10.856	131	3426	0.606	ng/ul	0.02
46) Dimethylphthalate-d6	13.935	166	173204	14.462	ng/ul	0.00
49) Acenaphthylene-d8	14.229	160	189133	15.069	ng/ul	0.00
54) 4-Nitrophenol-d4	14.758	143	5789m	3.201	ng/ul	0.02
60) Fluorene-d10	15.527	176	152310	15.360	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	114	0.070	ng/ul	0.00
73) Anthracene-d10	17.378	188	226734	16.409	ng/ul	0.00
81) Pyrene-d10	19.670	212	202713	13.329	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.464	264	134599	8.904	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
Data File : BG058409.D
Acq On : 22 Jul 2023 20:13
Operator : CG/JU
Sample : 03536-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YBW60

Manual IntegrationsAPPROVED

Quant Time: Jul 23 02:41:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 18 02:19:39 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/24/2023
Supervised By :mohammad ahmed 07/24/2023

