

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
 Data File : BG058421.D
 Acq On : 23 Jul 2023 5:15
 Operator : CG/JU
 Sample : 03537-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.338	40	42	46	rVB3	5509	5464	0.37%	0.037%
2	3.755	108	113	128	rBV	69188	140515	9.52%	0.946%
3	3.990	148	153	156	rBV4	7368	12226	0.83%	0.082%
4	4.084	166	169	175	rVB4	3681	5895	0.40%	0.040%
5	5.042	331	332	336	rVB2	1349	1544	0.10%	0.010%
6	7.063	669	676	686	rBV	50481	93570	6.34%	0.630%
7	7.221	696	703	715	rBV	192818	324306	21.96%	2.184%
8	7.427	731	738	748	rBV	183948	315717	21.38%	2.126%
9	7.897	811	818	829	rBV	221417	393124	26.63%	2.647%
10	8.602	930	938	949	rBV	138760	253855	17.19%	1.709%
11	9.055	1006	1015	1027	rBV	230906	416837	28.23%	2.807%
12	9.207	1039	1041	1046	rVB5	1528	2226	0.15%	0.015%
13	9.337	1058	1063	1065	rBV3	1029	1495	0.10%	0.010%
14	9.777	1130	1138	1153	rBV	152585	282611	19.14%	1.903%
15	10.018	1173	1179	1182	rBV4	762	1564	0.11%	0.011%
16	10.318	1224	1230	1242	rBV	229538	452550	30.65%	3.047%
17	10.694	1287	1294	1305	rVB	347594	630160	42.68%	4.243%
18	10.835	1310	1318	1328	rBV	227326	448648	30.39%	3.021%
19	12.280	1559	1564	1571	rVB2	3882	6092	0.41%	0.041%
20	13.414	1754	1757	1764	rBV4	3811	5494	0.37%	0.037%
21	13.937	1839	1846	1855	rBV	467091	699520	47.38%	4.710%
22	14.225	1888	1895	1905	rBV2	559193	897375	60.78%	6.043%
23	14.478	1933	1938	1941	rBV4	1160	2134	0.14%	0.014%
24	14.536	1941	1948	1964	rVB	526312	855357	57.93%	5.760%
25	14.766	1979	1987	1997	rBV4	12785	38973	2.64%	0.262%
26	15.371	2087	2090	2092	rVB3	1232	1508	0.10%	0.010%
27	15.524	2109	2116	2125	rBV	705451	1108816	75.10%	7.467%
28	15.653	2134	2138	2144	rVB2	16333	23815	1.61%	0.160%
29	15.764	2153	2157	2160	rBV4	2437	3054	0.21%	0.021%
30	15.888	2171	2178	2187	rBV	11973	18738	1.27%	0.126%
31	16.229	2233	2236	2242	rBV3	1621	3126	0.21%	0.021%
32	17.022	2365	2371	2374	rBV5	2408	4057	0.27%	0.027%
33	17.069	2378	2379	2383	rVB2	1518	1496	0.10%	0.010%
34	17.280	2408	2415	2425	rBV	659104	988870	66.97%	6.659%
35	17.374	2425	2431	2442	rVV	783685	1234921	83.64%	8.316%
36	17.451	2442	2444	2448	rVB2	4021	4241	0.29%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
 Data File : BG058421.D
 Acq On : 23 Jul 2023 5:15
 Operator : CG/JU
 Sample : 03537-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

37	17.762	2494	2497	2501	rVB3	2216	2558	0.17%	0.017%
38	17.938	2523	2527	2529	rVV4	1889	1828	0.12%	0.012%
39	17.979	2533	2534	2537	rBV3	1943	1489	0.10%	0.010%
40	18.162	2560	2565	2572	rBV3	17217	30542	2.07%	0.206%
41	18.232	2576	2577	2581	rVV2	3972	4466	0.30%	0.030%
42	18.450	2612	2614	2619	rVB4	1995	2935	0.20%	0.020%
43	18.585	2635	2637	2639	rBV3	1788	1682	0.11%	0.011%
44	18.790	2669	2672	2673	rBV2	1886	1697	0.11%	0.011%
45	19.084	2718	2722	2726	rBV7	3226	4075	0.28%	0.027%
46	19.231	2741	2747	2753	rBV2	13577	22195	1.50%	0.149%
47	19.307	2755	2760	2764	rBV	10825	16697	1.13%	0.112%
48	19.437	2781	2782	2790	rVV7	4118	7498	0.51%	0.050%
49	19.583	2803	2807	2809	rBV5	3109	3724	0.25%	0.025%
50	19.666	2815	2821	2830	rVV2	936192	1420423	96.20%	9.565%
51	19.971	2869	2873	2875	rBV5	3225	4054	0.27%	0.027%
52	20.618	2981	2983	2986	rBV4	8568	7877	0.53%	0.053%
53	20.952	3039	3040	3043	rBV3	6562	6076	0.41%	0.041%
54	20.994	3045	3047	3050	rVV4	9293	9576	0.65%	0.064%
55	21.528	3132	3138	3147	rBV2	595402	1005163	68.08%	6.769%
56	24.454	3627	3636	3651	rVB2	535025	1476496	100.00%	9.942%
57	24.672	3663	3673	3686	rVB	392331	1139552	77.18%	7.673%




Sum of corrected areas: 14850497

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
Data File : BG058421.D
Acq On : 23 Jul 2023 5:15
Operator : CG/JU
Sample : 03537-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

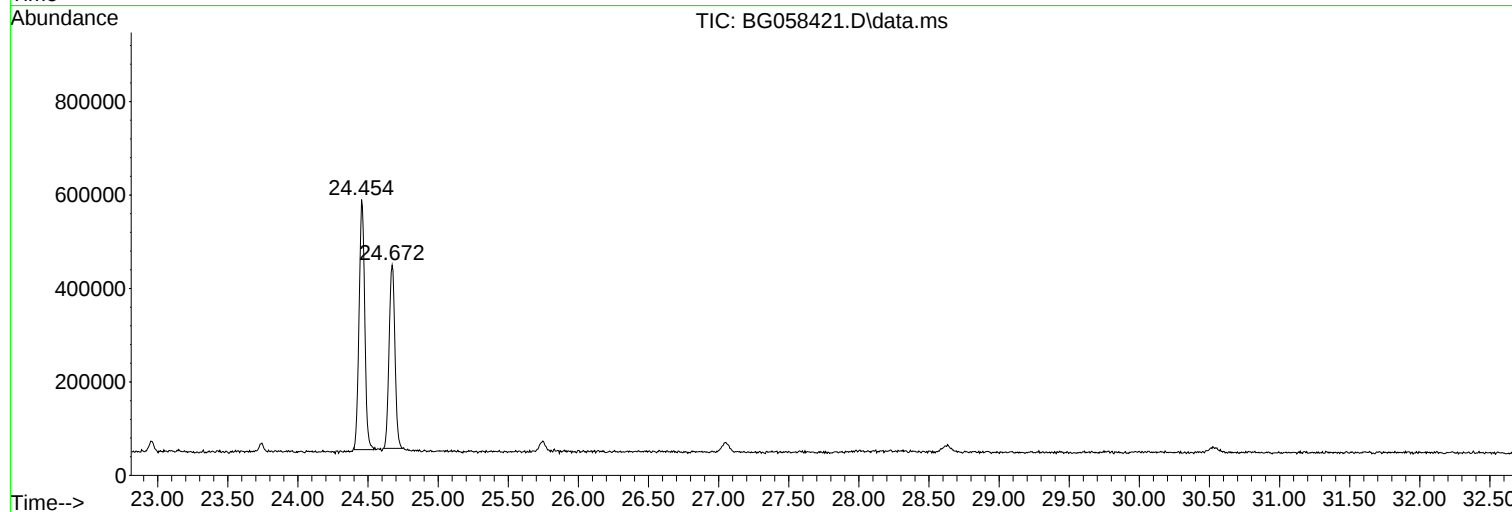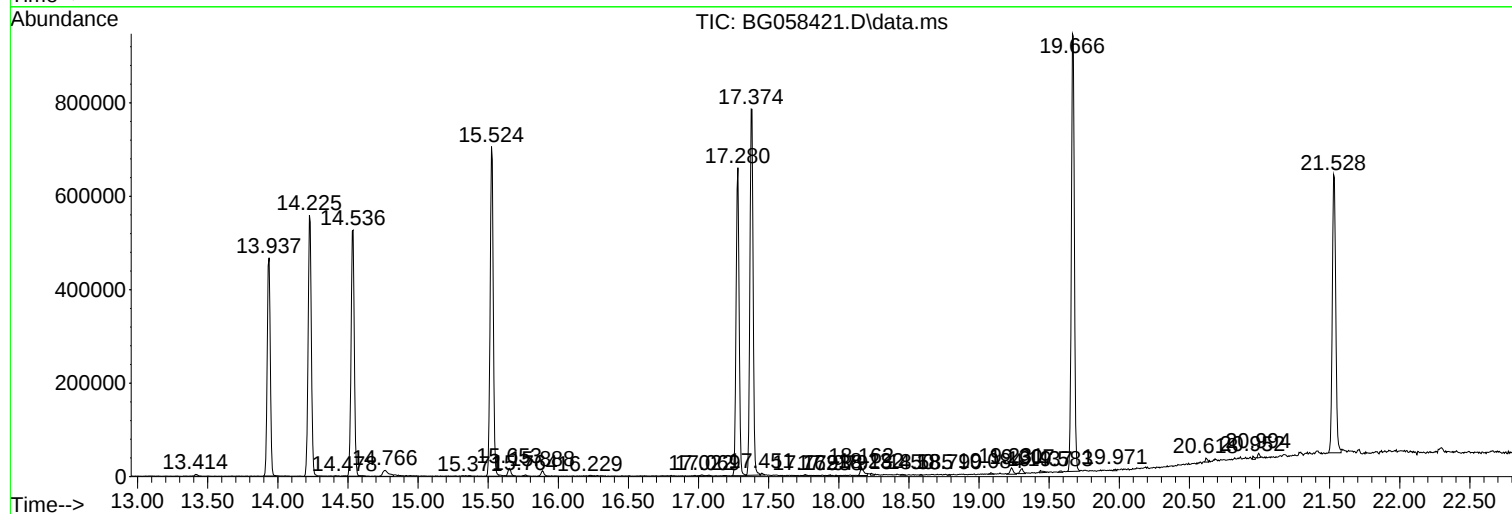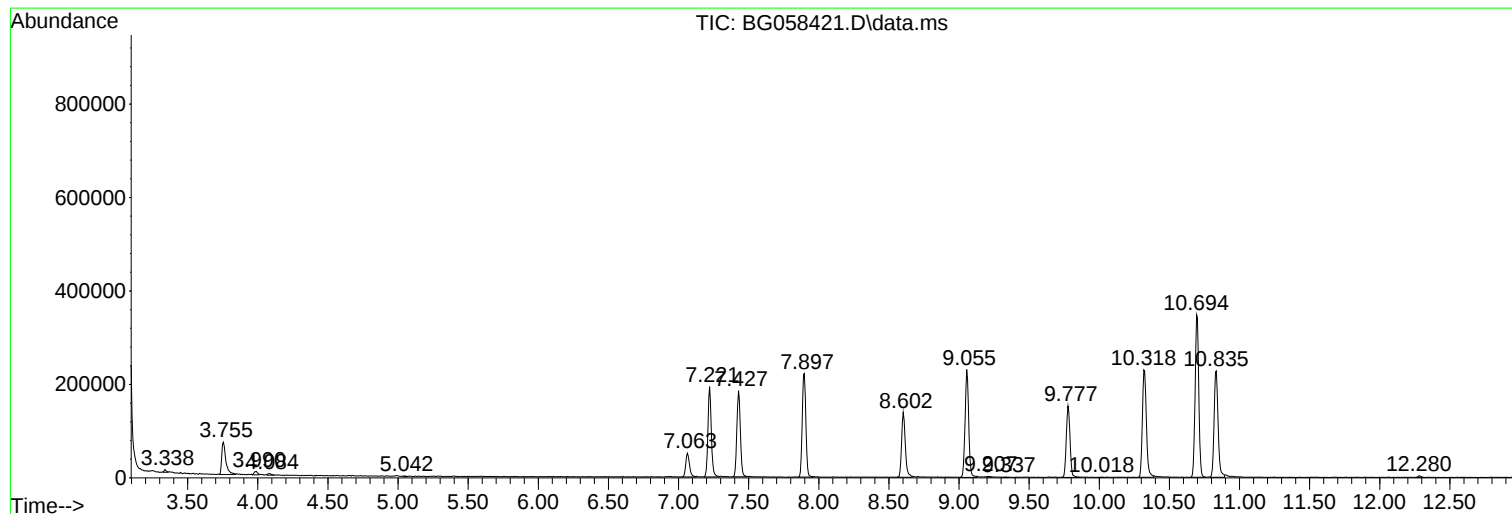

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
Data File : BG058421.D
Acq On : 23 Jul 2023 5:15
Operator : CG/JU
Sample : 03537-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072223\
Data File : BG058421.D
Acq On : 23 Jul 2023 5:15
Operator : CG/JU
Sample : 03537-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
