


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072318\
 Data File : BG035820.D
 Acq On : 23 Jul 2018 10:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

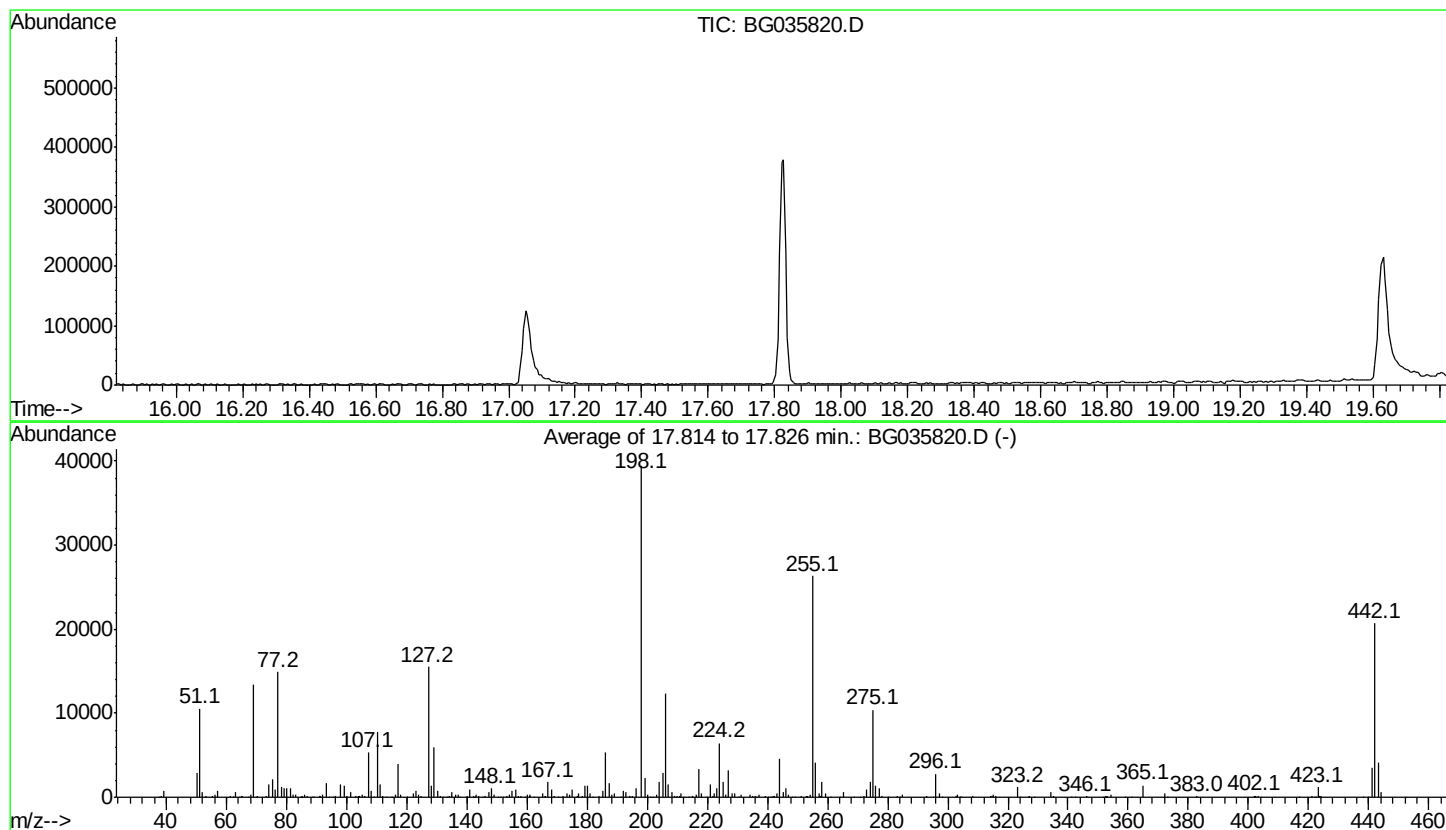

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	10556	PASS
68	69	0.00	2	1.8	246	PASS
69	198	0.00	100	33.9	13373	PASS
70	69	0.00	2	1.2	155	PASS
127	198	10	80	39.3	15516	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39461	PASS
199	198	5	9	5.8	2294	PASS
275	198	10	60	26.5	10438	PASS
365	198	1	100	3.6	1423	PASS
441	198	0.01	100	8.7	3444	PASS
442	198	50	100	52.4	20689	PASS
443	442	15	24	20.1	4159	PASS