

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072421\
 Data File : BG049437.D
 Acq On : 23 Jul 2021 23:17
 Operator : CG/JU
 Sample : PB137573BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK573

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG049437.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.080	3	7	14	rBV	23349	39546	5.38%	0.570%
2	3.227	30	32	34	rBV3	2611	2476	0.34%	0.036%
3	3.338	49	51	52	rVB2	2294	1165	0.16%	0.017%
4	3.426	63	66	70	rBV3	6079	8533	1.16%	0.123%
5	3.567	89	90	93	rVB	2255	1374	0.19%	0.020%
6	3.661	104	106	109	rBV3	1310	1486	0.20%	0.021%
7	3.791	125	128	132	rBV4	1255	2194	0.30%	0.032%
8	3.855	136	139	151	rBV	63592	127718	17.36%	1.841%
9	3.990	161	162	166	rVB2	1748	1493	0.20%	0.022%
10	4.919	318	320	323	rBV3	1139	1201	0.16%	0.017%
11	5.218	368	371	374	rVB2	1421	1817	0.25%	0.026%
12	5.289	378	383	386	rBV3	844	1554	0.21%	0.022%
13	5.759	461	463	465	rBV2	1667	1499	0.20%	0.022%
14	5.829	473	475	479	rVB2	1242	1214	0.17%	0.017%
15	6.140	522	528	529	rBV	916	1214	0.17%	0.017%
16	6.375	562	568	570	rBV	928	1549	0.21%	0.022%
17	6.898	656	657	660	rBV	1380	1144	0.16%	0.016%
18	7.086	685	689	693	rBV2	780	1490	0.20%	0.021%
19	7.198	701	708	715	rBV2	104395	184126	25.03%	2.654%
20	7.368	731	737	748	rBV	67293	117549	15.98%	1.694%
21	7.574	764	772	782	rBV2	104349	182074	24.75%	2.624%
22	7.850	816	819	823	rBV	650	1187	0.16%	0.017%
23	8.044	846	852	860	rVB	63835	112182	15.25%	1.617%
24	8.755	966	973	986	rBV	115385	212320	28.86%	3.060%
25	9.048	1019	1023	1026	rBV	883	1416	0.19%	0.020%
26	9.213	1043	1051	1062	rBV	103754	182235	24.77%	2.626%
27	9.941	1168	1175	1182	rVB2	88186	157595	21.42%	2.271%
28	10.170	1210	1214	1218	rBV2	1108	1244	0.17%	0.018%
29	10.482	1259	1267	1278	rBV	117231	220483	29.97%	3.178%
30	10.869	1326	1333	1345	rVB	84511	158492	21.55%	2.284%
31	10.999	1349	1355	1367	rVV	111050	212867	28.94%	3.068%
32	12.461	1599	1604	1606	rBV2	1559	2647	0.36%	0.038%
33	14.094	1875	1882	1889	rBV	258202	369896	50.29%	5.331%
34	14.388	1924	1932	1940	rBV	250061	388800	52.86%	5.603%
35	14.694	1976	1984	1991	rBV	140400	216654	29.45%	3.122%
36	14.887	2009	2017	2027	rBV2	103679	185217	25.18%	2.669%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072421\
 Data File : BG049437.D
 Acq On : 23 Jul 2021 23:17
 Operator : CG/JU
 Sample : PB137573BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK573

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

37	15.017	2038	2039	2043	rVB	1319	1193	0.16%	0.017%
38	15.686	2147	2153	2162	rVB	325976	482058	65.53%	6.947%
39	15.804	2166	2173	2181	rBV	108579	171816	23.36%	2.476%
40	15.933	2190	2195	2198	rBV2	3899	4891	0.66%	0.070%
41	16.474	2284	2287	2292	rBV	1426	1794	0.24%	0.026%
42	17.026	2375	2381	2382	rBV	1086	1260	0.17%	0.018%
43	17.443	2445	2452	2460	rBV	190856	285879	38.86%	4.120%
44	17.543	2463	2469	2477	rBV2	377064	569048	77.36%	8.201%
45	17.966	2539	2541	2544	rBV	1188	1084	0.15%	0.016%
46	18.107	2563	2565	2569	rBV	1121	1273	0.17%	0.018%
47	18.647	2652	2657	2659	rBV	760	1082	0.15%	0.016%
48	19.041	2722	2724	2728	rVB	928	1167	0.16%	0.017%
49	19.182	2745	2748	2750	rBV	1502	1479	0.20%	0.021%
50	19.293	2764	2767	2770	rVB	1192	1801	0.24%	0.026%
51	19.334	2772	2774	2777	rBV	1288	1634	0.22%	0.024%
52	19.464	2793	2796	2801	rVB	3942	5624	0.76%	0.081%
53	19.716	2837	2839	2845	rBV2	3694	5300	0.72%	0.076%
54	19.828	2852	2858	2867	rBV	493088	731027	99.38%	10.536%
55	20.022	2889	2891	2894	rBV2	1399	1431	0.19%	0.021%
56	20.092	2900	2903	2905	rBV2	1201	1352	0.18%	0.019%
57	20.163	2913	2915	2917	rBV2	1424	1169	0.16%	0.017%
58	20.198	2917	2921	2922	rVB3	2280	2341	0.32%	0.034%
59	20.216	2922	2924	2927	rBV2	2175	1772	0.24%	0.026%
60	20.310	2938	2940	2942	rBV2	2649	1662	0.23%	0.024%
61	20.427	2957	2960	2963	rBV3	1689	2021	0.27%	0.029%
62	20.527	2974	2977	2979	rBV3	1475	1673	0.23%	0.024%
63	20.568	2982	2984	2985	rBV2	2015	1202	0.16%	0.017%
64	20.709	3006	3008	3009	rBV2	1497	1158	0.16%	0.017%
65	20.762	3016	3017	3018	rBV	2133	1197	0.16%	0.017%
66	21.232	3095	3097	3100	rBV3	2042	2780	0.38%	0.040%
67	21.273	3102	3104	3105	rBV2	1549	1348	0.18%	0.019%
68	21.555	3150	3152	3154	rBV3	2447	1852	0.25%	0.027%
69	21.608	3157	3161	3164	rBV4	2607	4479	0.61%	0.065%
70	21.725	3174	3181	3186	rBV2	218770	365781	49.73%	5.272%
71	21.896	3208	3210	3212	rBV	2035	1886	0.26%	0.027%
72	21.978	3221	3224	3226	rBV3	2646	2763	0.38%	0.040%
73	22.001	3226	3228	3231	rVV4	2102	1934	0.26%	0.028%
74	22.066	3237	3239	3240	rBV2	2367	1084	0.15%	0.016%
75	22.154	3252	3254	3255	rBV	2641	1201	0.16%	0.017%
76	22.366	3289	3290	3292	rVB2	3253	1607	0.22%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072421\
 Data File : BG049437.D
 Acq On : 23 Jul 2021 23:17
 Operator : CG/JU
 Sample : PB137573BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK573

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
 Title : SVOA CALIBRATION

77	22.395	3293	3295	3297	rVV2	2368	1373	0.19%	0.020%
78	23.235	3432	3438	3439	rBV6	4889	5145	0.70%	0.074%
79	23.417	3467	3469	3471	rBV3	3046	2429	0.33%	0.035%
80	23.599	3498	3500	3501	rBV2	2089	1275	0.17%	0.018%
81	23.946	3557	3559	3560	rBV2	2805	2148	0.29%	0.031%
82	24.492	3650	3652	3655	rVB5	2574	2133	0.29%	0.031%
83	24.533	3657	3659	3660	rBV	1998	1179	0.16%	0.017%
84	24.627	3673	3675	3677	rBV2	2016	2030	0.28%	0.029%
85	24.774	3689	3700	3711	rBV	261291	735591	100.00%	10.601%
86	24.997	3727	3738	3750	rVB2	126304	371528	50.51%	5.354%
87	25.567	3833	3835	3837	rBV3	2493	2463	0.33%	0.035%
88	26.178	3933	3939	3940	rBV6	5694	7462	1.01%	0.108%
89	26.930	4066	4067	4069	rBV2	2528	1325	0.18%	0.019%
90	27.858	4224	4225	4228	rBV2	3133	2981	0.41%	0.043%
91	27.917	4233	4235	4236	rBV2	2027	1602	0.22%	0.023%
92	28.305	4300	4301	4303	rBV	2538	2019	0.27%	0.029%
93	28.487	4330	4332	4335	rBV4	3039	3121	0.42%	0.045%
94	29.103	4435	4437	4438	rBV2	2000	1541	0.21%	0.022%
95	29.321	4470	4474	4475	rBV4	2191	2475	0.34%	0.036%
96	29.338	4475	4477	4479	rBV3	1719	1088	0.15%	0.016%
97	29.444	4493	4495	4496	rBV2	2737	1814	0.25%	0.026%
98	29.521	4506	4508	4509	rVB2	2378	1410	0.19%	0.020%
99	29.814	4556	4558	4560	rBV	2376	3036	0.41%	0.044%
100	32.611	5032	5034	5036	rBV4	2410	2716	0.37%	0.039%


Sum of corrected areas: 6938638

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072421\
Data File : BG049437.D
Acq On : 23 Jul 2021 23:17
Operator : CG/JU
Sample : PB137573BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

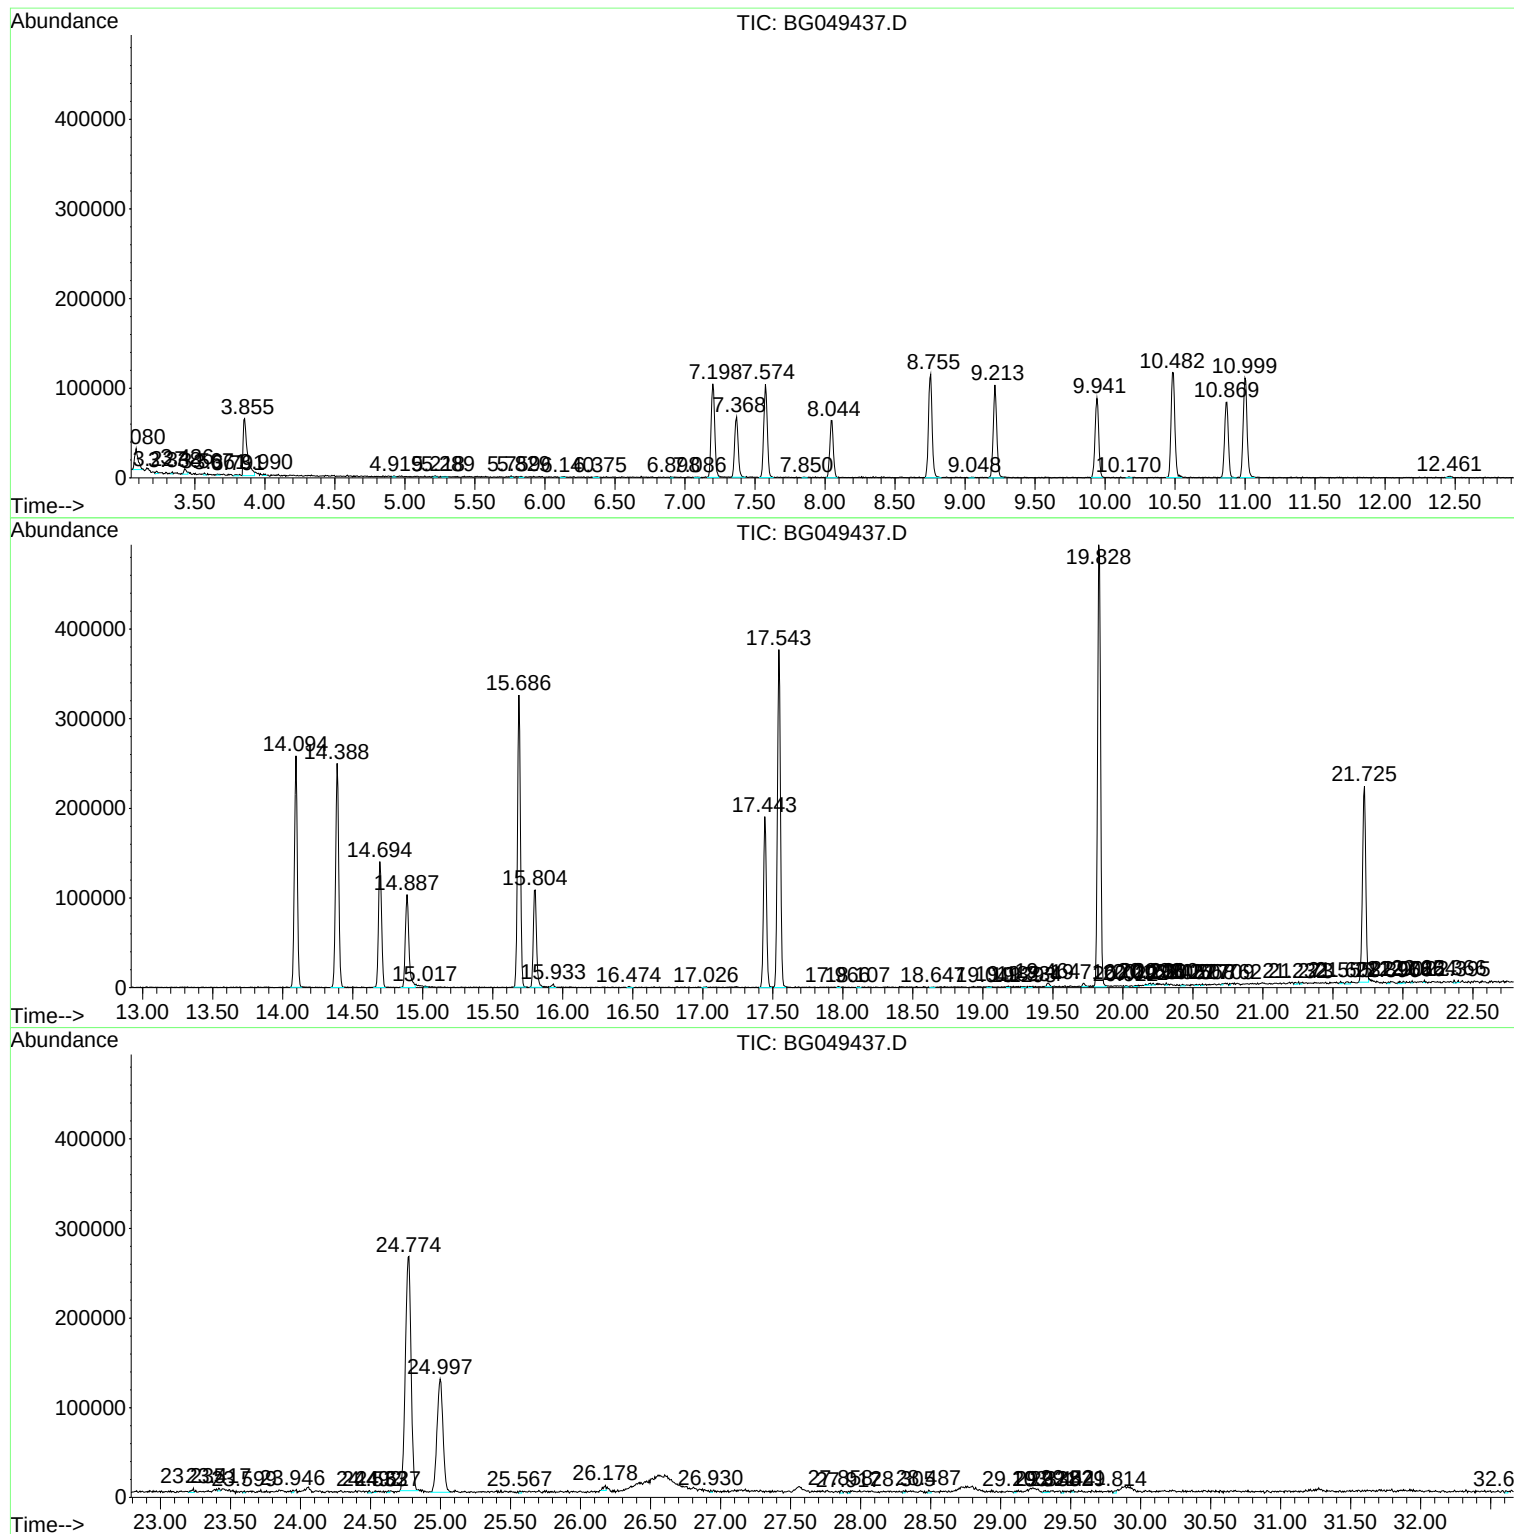

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072421\
Data File : BG049437.D
Acq On : 23 Jul 2021 23:17
Operator : CG/JU
Sample : PB137573BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic3.08 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.080	7.05 ng/ul	39546	1,4-Dichlorobenzene-d4	8.050

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclohexane	84	C6H12	000110-82-7	76
2		Cyclohexane	84	C6H12	000110-82-7	64
3		1-Pentene, 2-methyl-	84	C6H12	000763-29-1	64
4		Cyclohexane	84	C6H12	000110-82-7	59
5		Cyclohexane	84	C6H12	000110-82-7	59

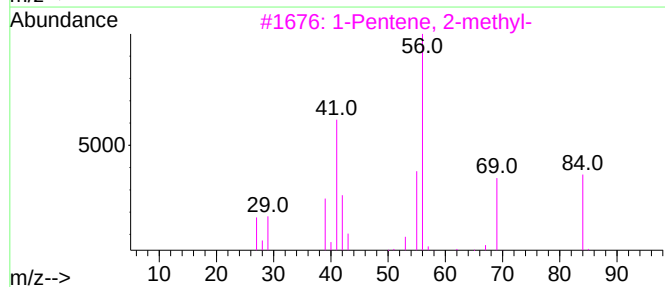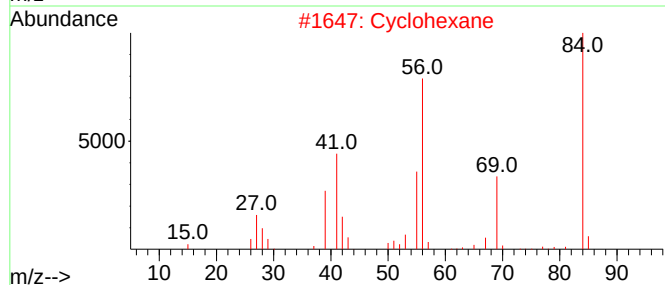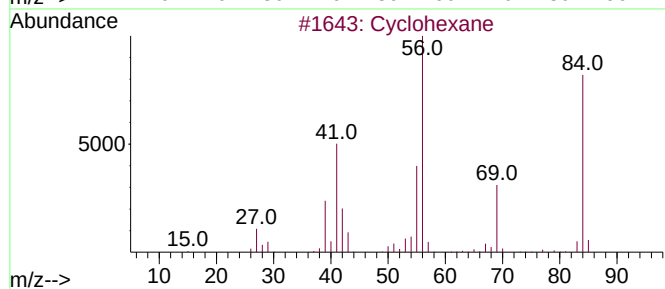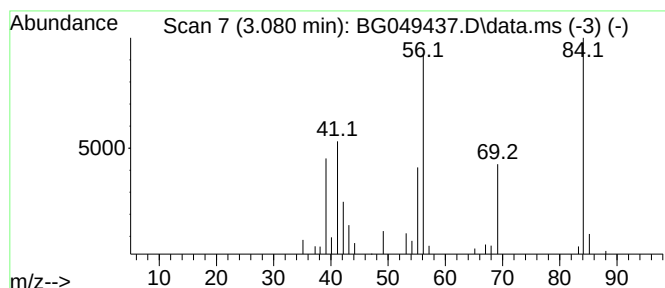

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072421\
Data File : BG049437.D
Acq On : 23 Jul 2021 23:17
Operator : CG/JU
Sample : PB137573BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK573

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	3.080	7.0	ng/ul	39546	1	8.050	112182	20.0