
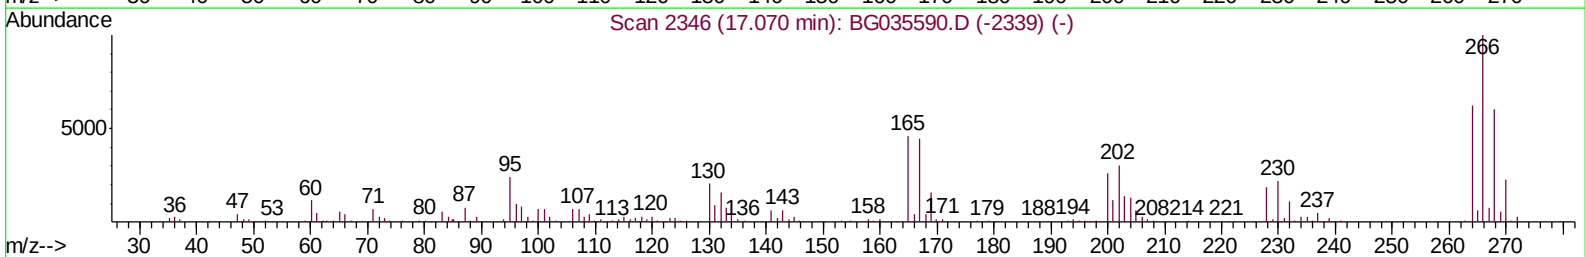
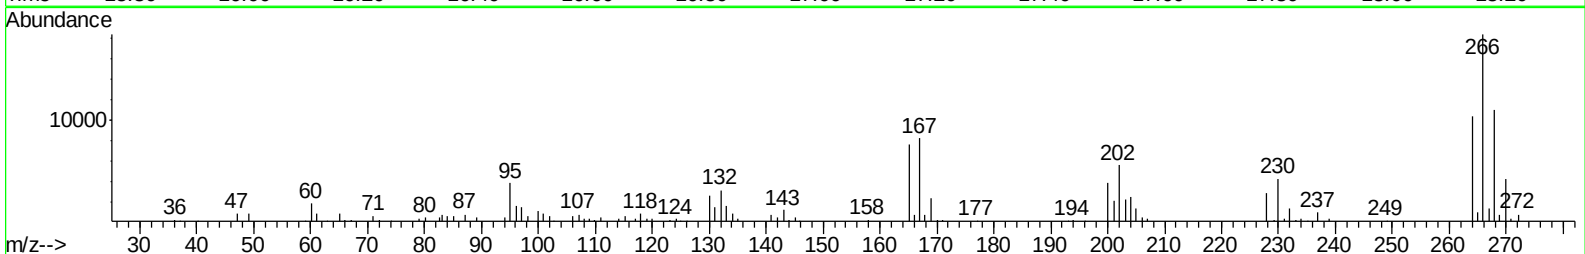


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072518\
Data File : BG035874.D
Acq On : 25 Jul 2018 15:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 06:47:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

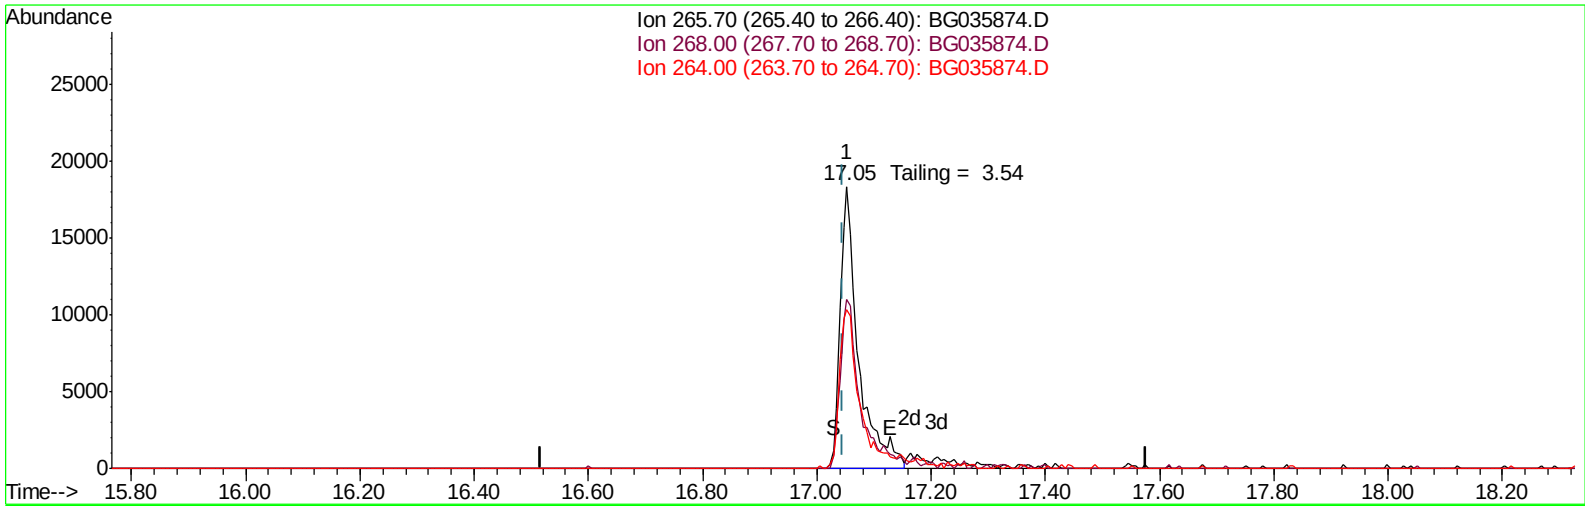

TIC: BG035874.D

(69) Pentachlorophenol (C)




17.052min (+0.005) 56435.94ng

response 39016

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.81
264.00	62.00	56.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072518\
Data File : BG035874.D
Acq On : 25 Jul 2018 15:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 06:47:36 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

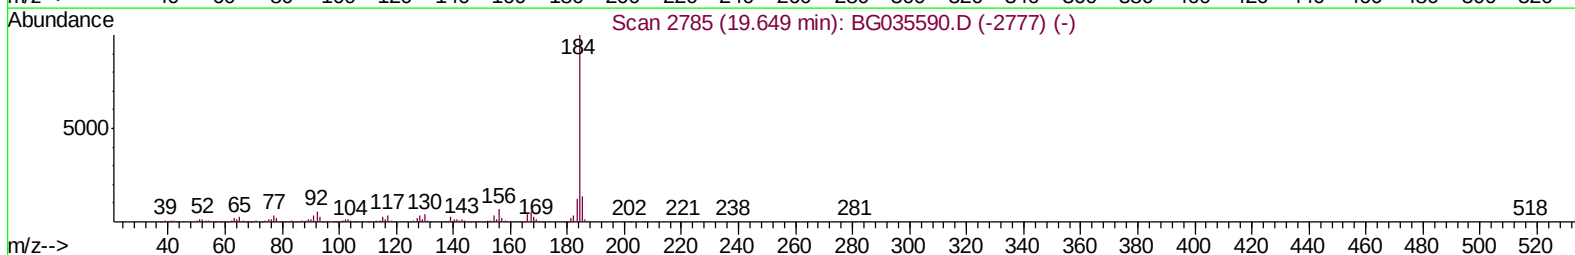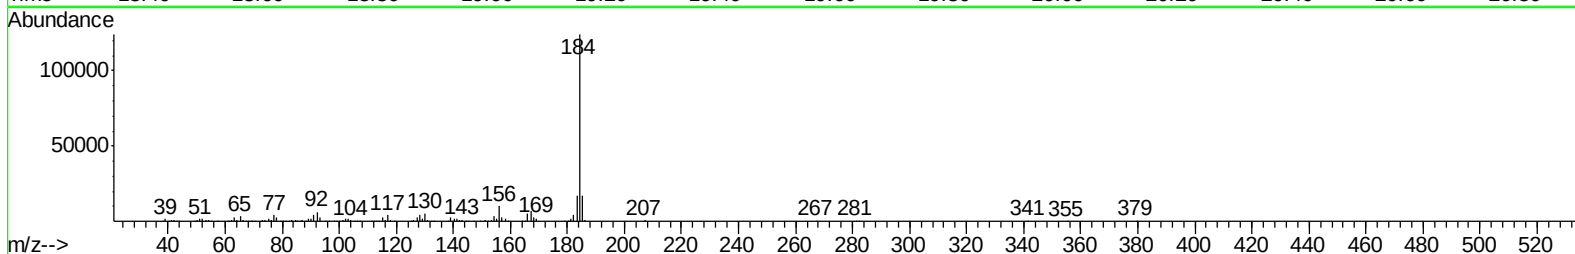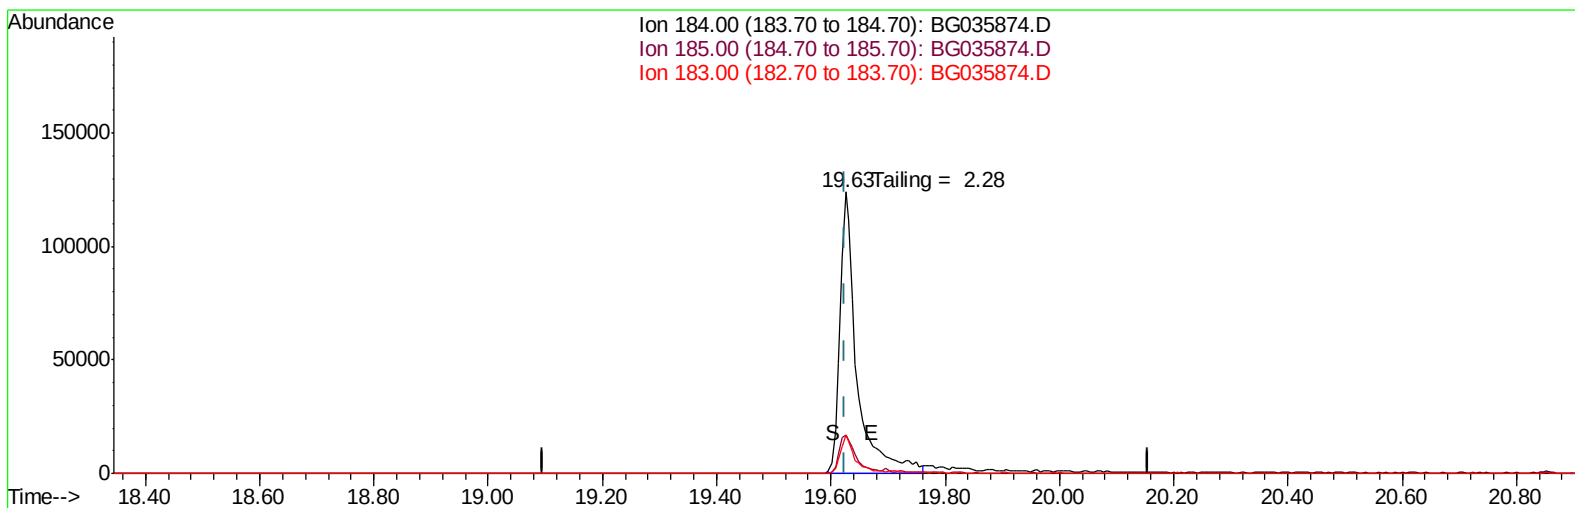

TIC: BG035874.D

(76) Benzidine

19.625min (-0.001) 128040.04ng

response 245733

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.78
183.00	13.30	13.82
0.00	0.00	0.00