
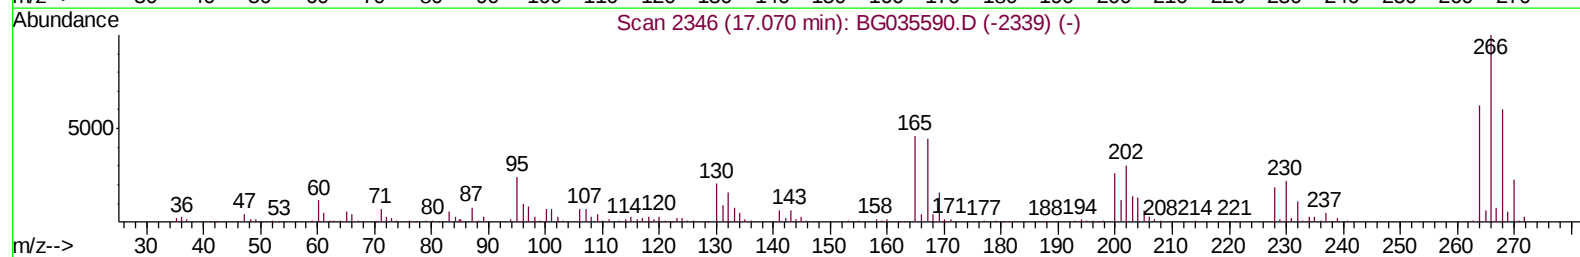
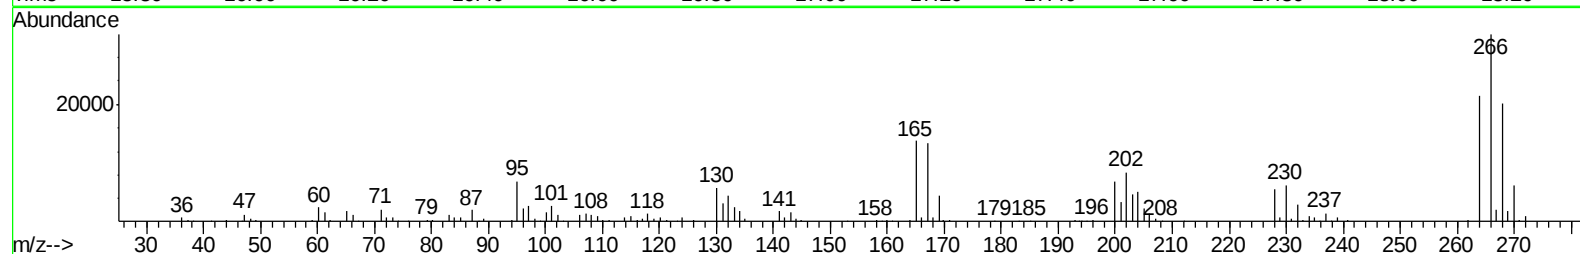


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072518\
Data File : BG035893.D
Acq On : 26 Jul 2018 4:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 06:39:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

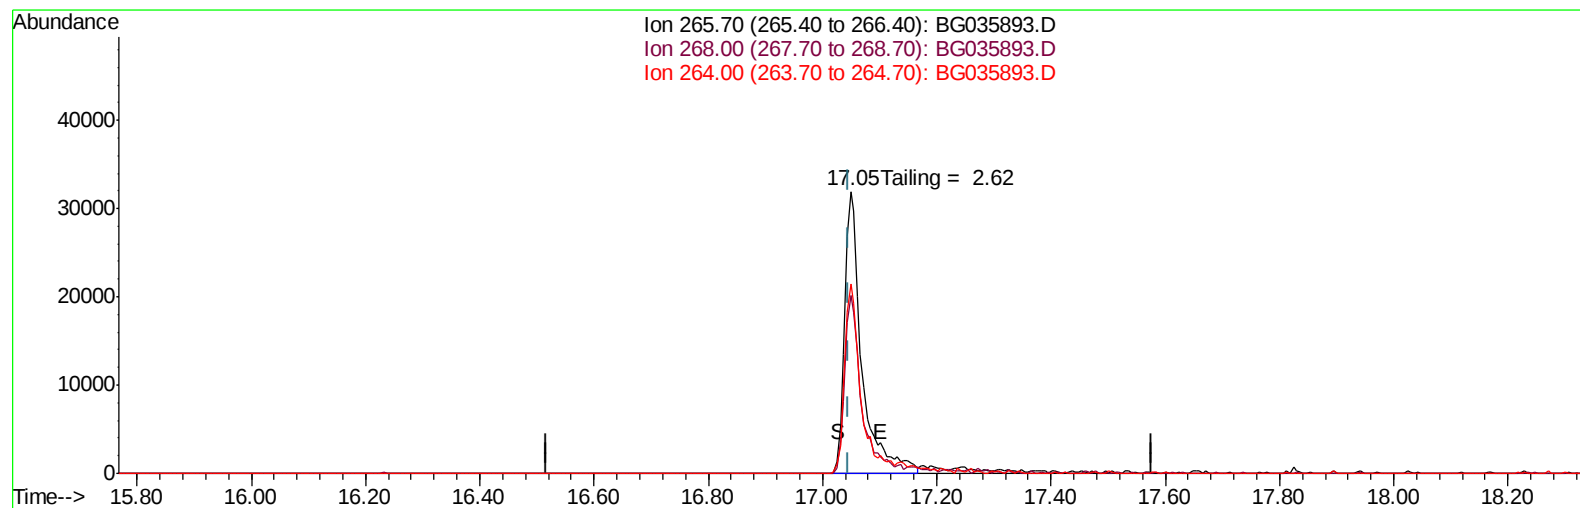

TIC: BG035893.D

(69) Pentachlorophenol (C)




17.049min (+0.001) 13025.08ng

response 67298

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.23
264.00	62.00	67.29
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072518\
 Data File : BG035893.D
 Acq On : 26 Jul 2018 4:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 06:39:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 25 11:04:14 2018
 Response via : Initial Calibration

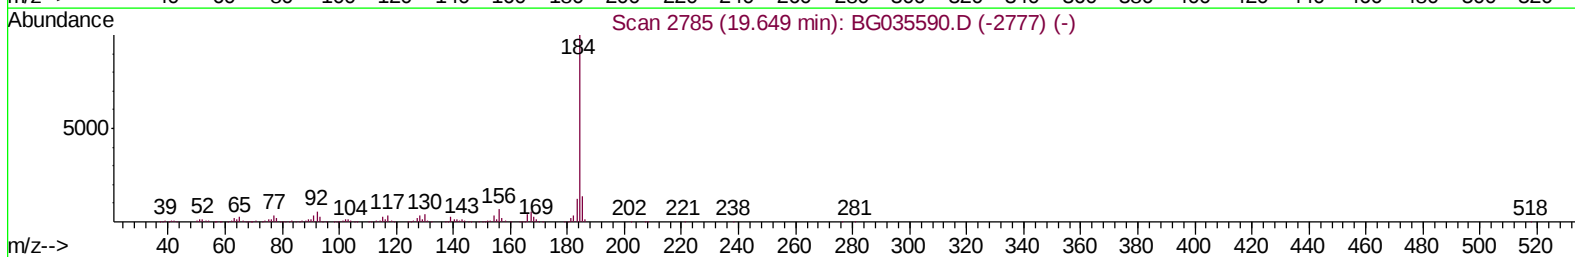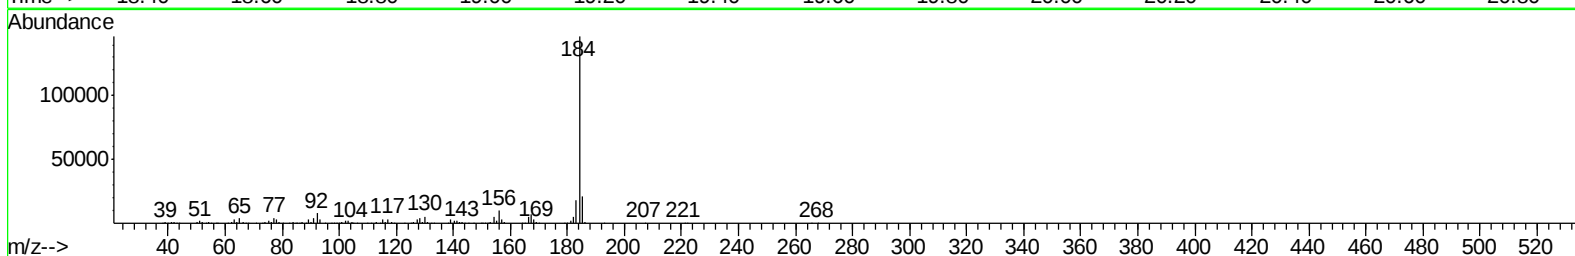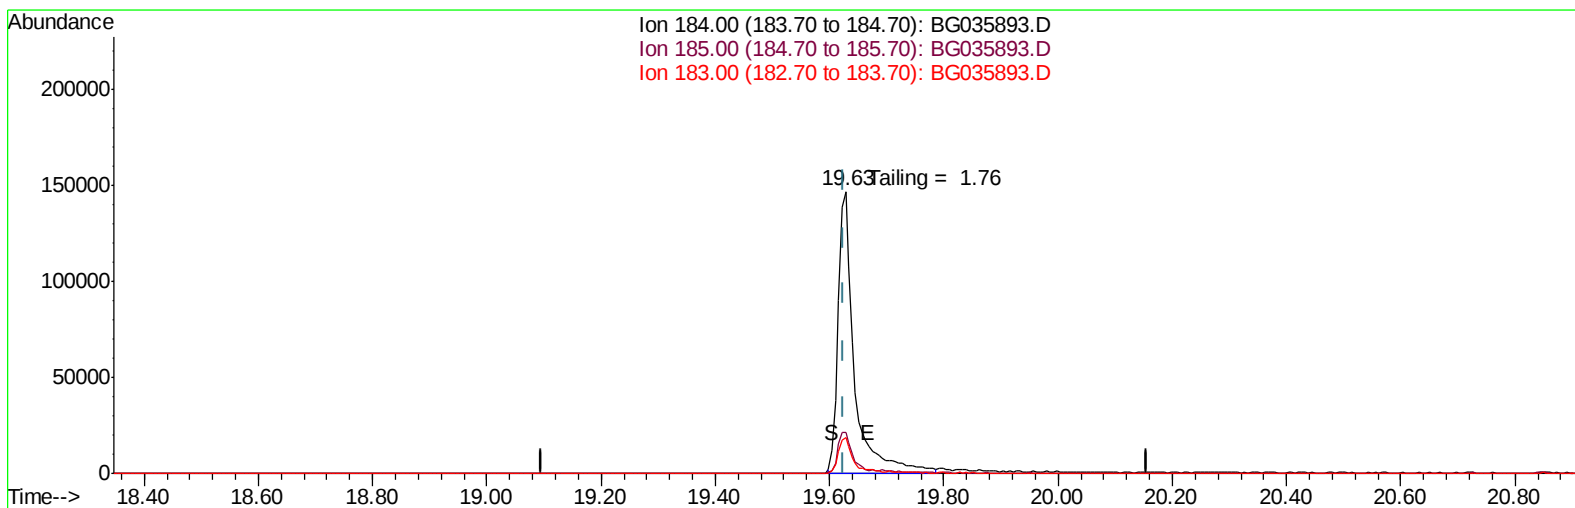

TIC: BG035893.D

(76) Benzidine

19.628min (+0.001) 26847.56ng

response 293625

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.41
183.00	13.30	12.63
0.00	0.00	0.00