

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG072518\
 Data File : BG035908.D
 Acq On : 26 Jul 2018 14:00
 Operator : JU/SJ
 Sample : J4123-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RO-1-3

Quant Time: Jul 26 14:47:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 25 11:04:14 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	33601	20.00	ng	0.00
21) Naphthalene-d8	10.83	136	127762	20.00	ng	0.00
38) Acenaphthene-d10	14.65	164	95657	20.00	ng	0.00
63) Phenanthrene-d10	17.39	188	294098	20.00	ng	0.00
75) Chrysene-d12	21.66	240	319199	20.00	ng	0.00
86) Perylene-d12	24.86	264	233239	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	271284	134.04	ng	0.00
7) Phenol-d6	7.19	99	361436	119.70	ng	0.00
23) Nitrobenzene-d5	9.19	82	283932	92.84	ng	0.00
41) 2,4,6-Tribromophenol	16.14	330	212452	168.50	ng	0.00
44) 2-Fluorobiphenyl	13.27	172	695832	97.46	ng	0.00
78) Terphenyl-d14	20.00	244	1501514	103.69	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG072518\
Data File : BG035908.D
Acq On : 26 Jul 2018 14:00
Operator : JU/SJ
Sample : J4123-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RO-1-3

Quant Time: Jul 26 14:47:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

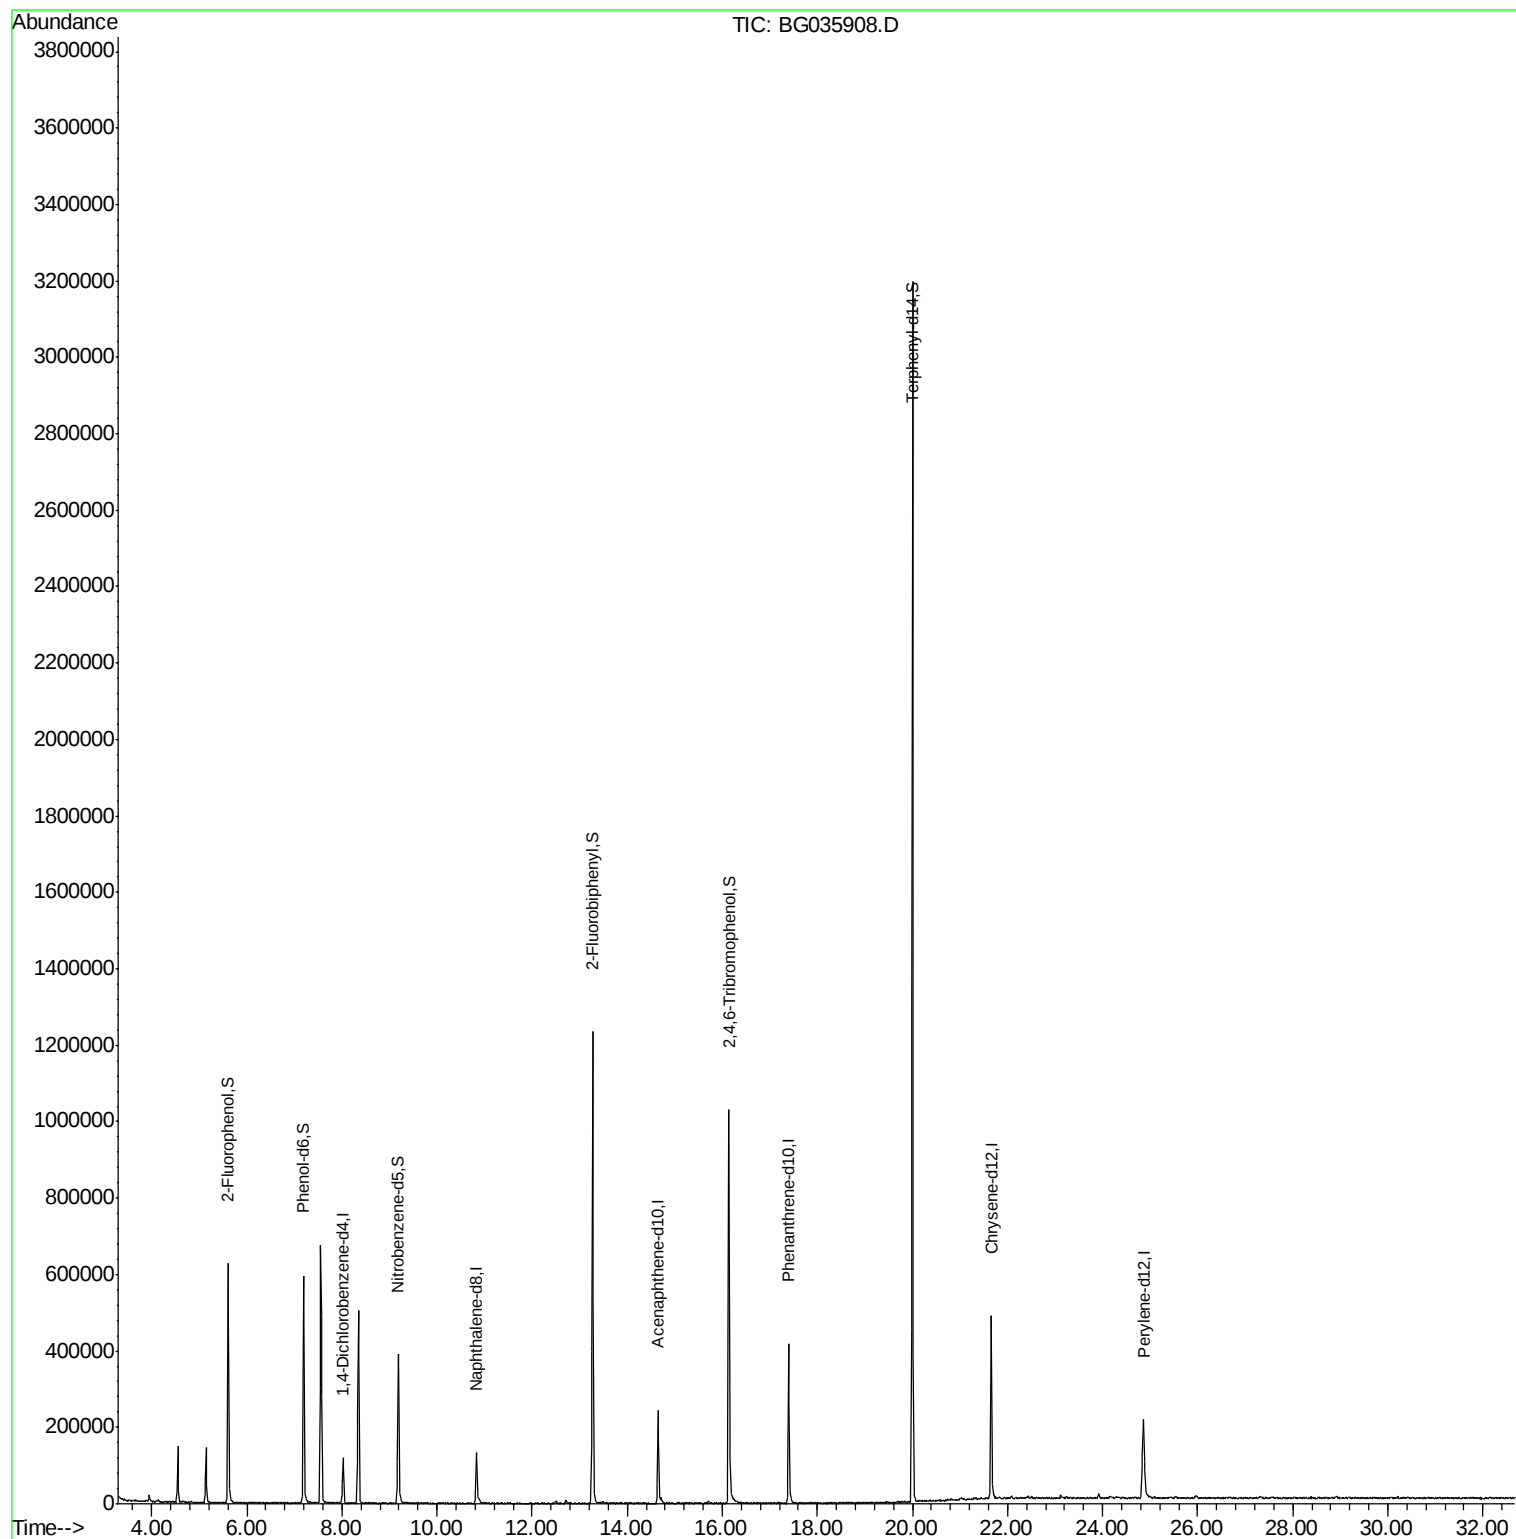




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.03 min Scan# 807
Delta R.T. 0.00 min
Lab File: BG035908.D
Acq: 26 Jul 2018 14:00

Instrument :
BNA_G
ClientSampleId :
RO-1-3

Tot Ion:152 Resp: 33601
Ion Ratio Lower Upper
152 100
150 147.4 126.6 189.8
115 67.9 53.0 79.4

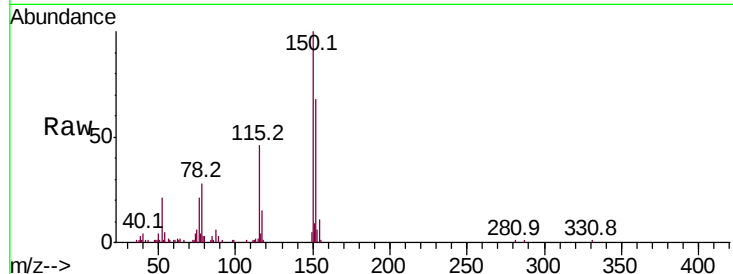


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

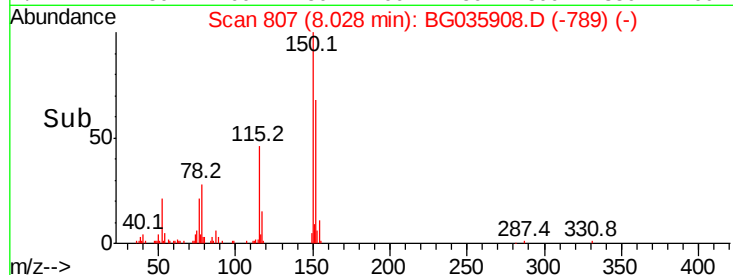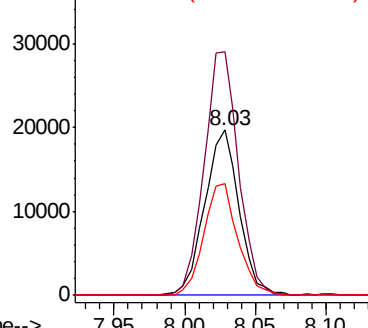



#5


2-Fluorophenol
Concen: 134.042 ng
RT: 5.61 min Scan# 395
Delta R.T. 0.00 min
Lab File: BG035908.D
Acq: 26 Jul 2018 14:00

Tgt Ion:112 Resp: 271284
Ion Ratio Lower Upper
112 100
64 64.1 56.3 84.5
63 34.9 30.1 45.1

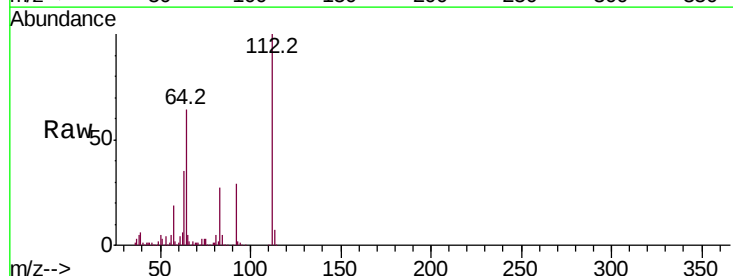

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

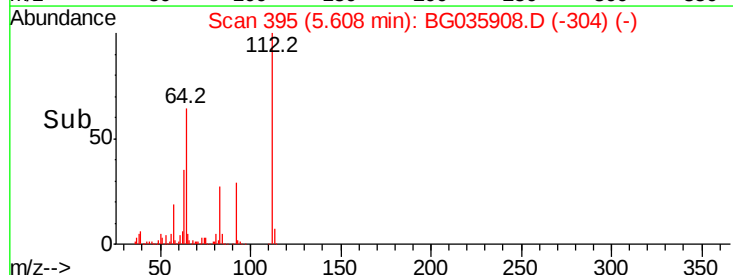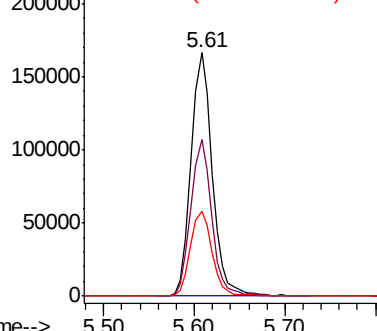

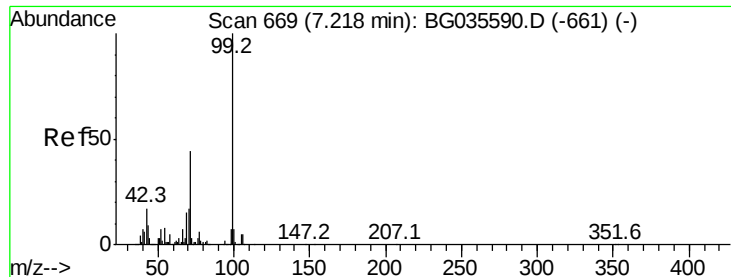

#7

Phenol-d6

Concen: 119.697 ng

RT: 7.19 min Scan# 665

Delta R.T. -0.00 min

Lab File: BG035908.D

Acq: 26 Jul 2018 14:00

Instrument :

BNA_G

ClientSampleId :

RO-1-3


Tot Ion: 99 Resp: 361436

Ion Ratio Lower Upper

99 100

42 17.1 14.1 21.1




71 42.3 26.1 39.1#

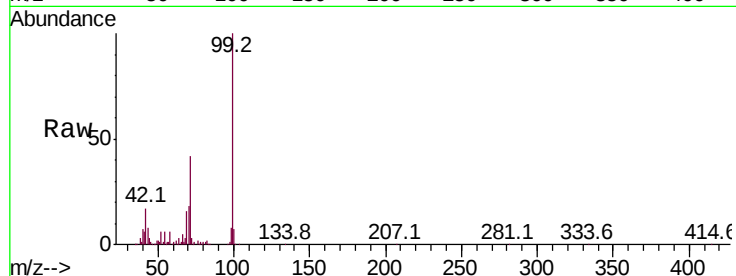

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

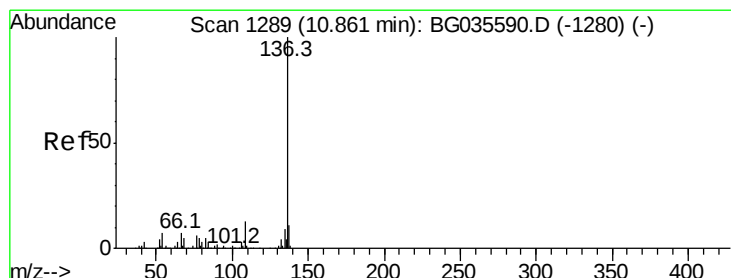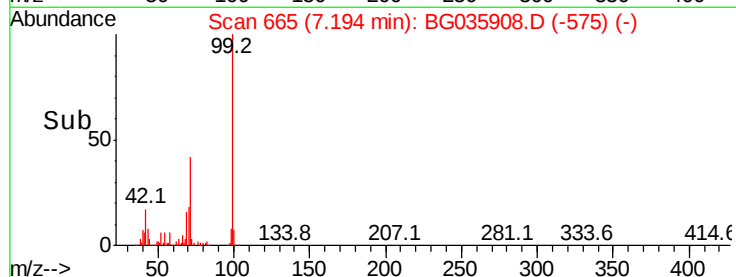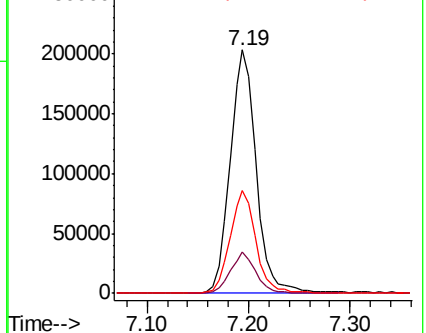

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.83 min Scan# 1284

Delta R.T. -0.00 min

Lab File: BG035908.D

Acq: 26 Jul 2018 14:00

Tgt Ion: 136 Resp: 127762


Ion Ratio Lower Upper

136 100

137 9.4 9.2 13.8

54 7.5 10.3 15.5#

68 6.1 4.5 6.7


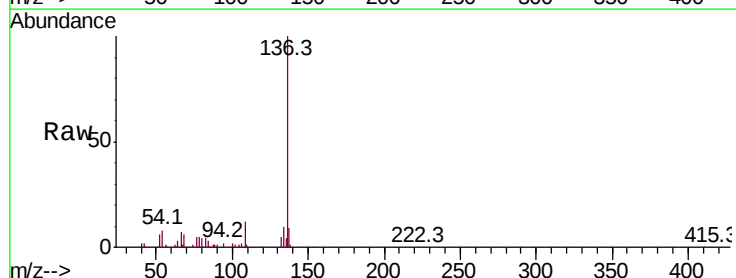



Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC



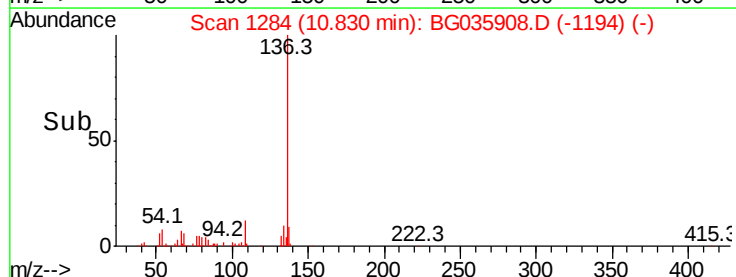
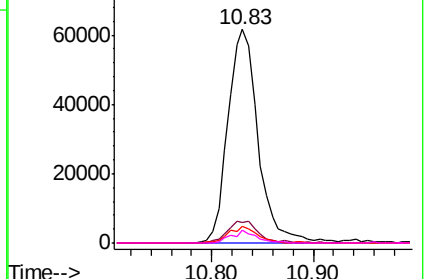


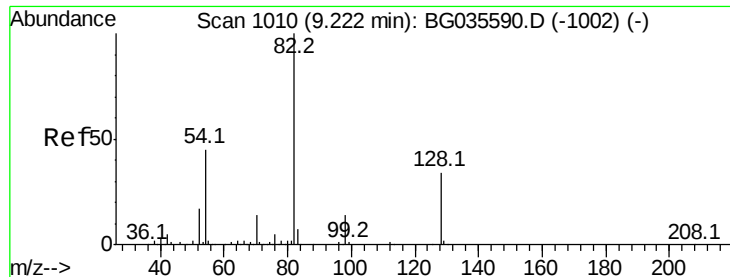

#23
Nitrobenzene-d5
Concen: 92.838 ng
RT: 9.19 min Scan# 1005
Delta R.T. 0.00 min
Lab File: BG035908.D
Acq: 26 Jul 2018 14:00




Instrument :
BNA_G
ClientSampleId :
RO-1-3

Tot Ion	Ratio	Lower	Upper
82	100		
128	33.6	29.7	44.5
54	41.7	43.1	64.7#

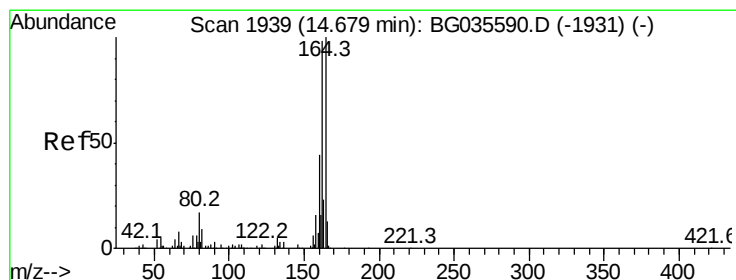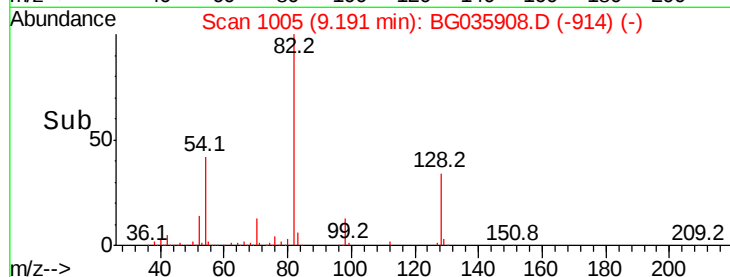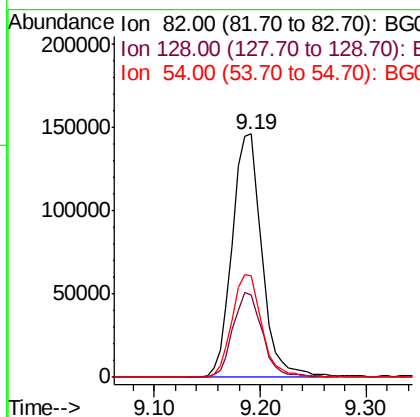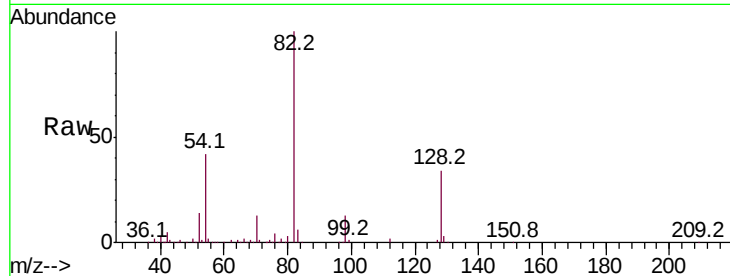

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.65 min Scan# 1934
Delta R.T. -0.00 min
Lab File: BG035908.D
Acq: 26 Jul 2018 14:00

Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.3	78.8	118.2
160	46.4	35.4	53.0


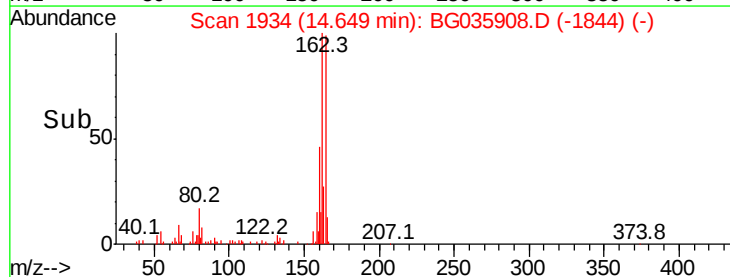
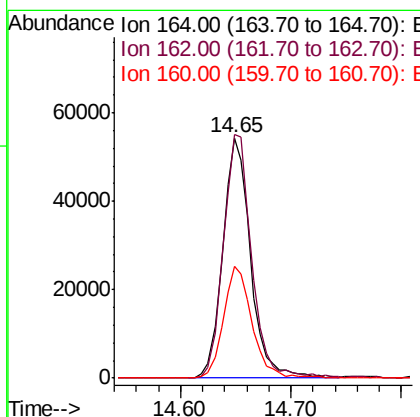
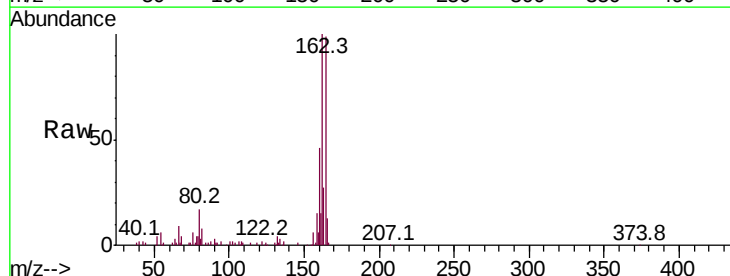




#41
2,4,6-Tribromophenol
Concen: 168.503 ng
RT: 16.14 min Scan# 2188
Delta R.T. -0.00 min
Lab File: BG035908.D
Acq: 26 Jul 2018 14:00




Instrument :
BNA_G
ClientSampleId :
RO-1-3


Tot Ion	Ratio	Lower	Upper
330	100		
332	98.3	77.0	115.6
141	40.2	25.2	37.8#

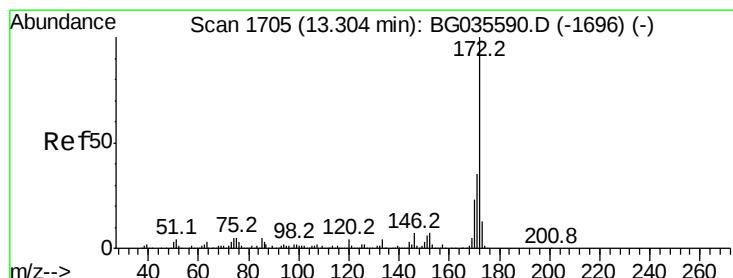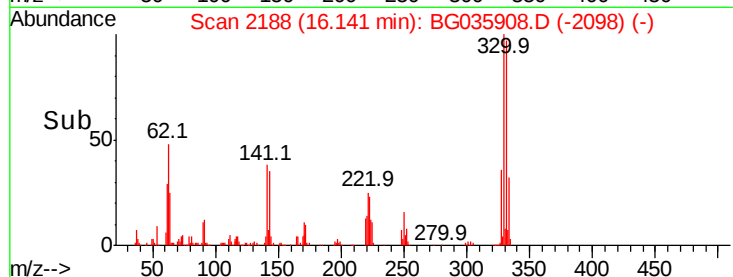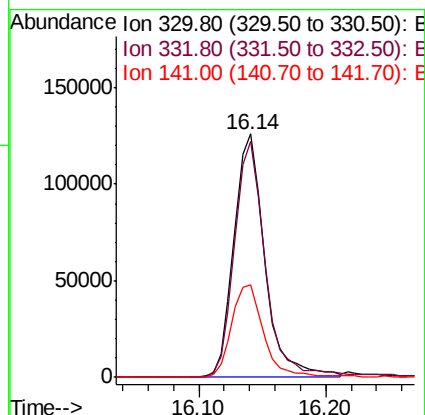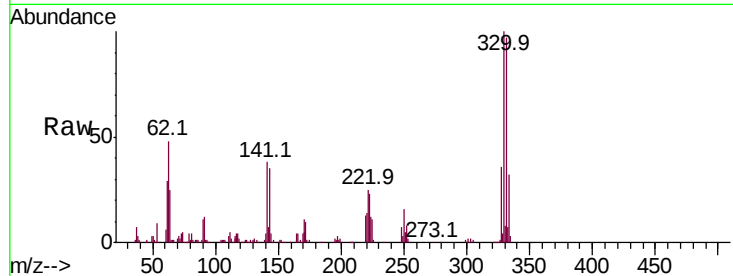

#44
2-Fluorobiphenyl
Concen: 97.456 ng
RT: 13.27 min Scan# 1700
Delta R.T. -0.00 min
Lab File: BG035908.D
Acq: 26 Jul 2018 14:00

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.3	30.0	45.0
170	23.2	19.5	29.3


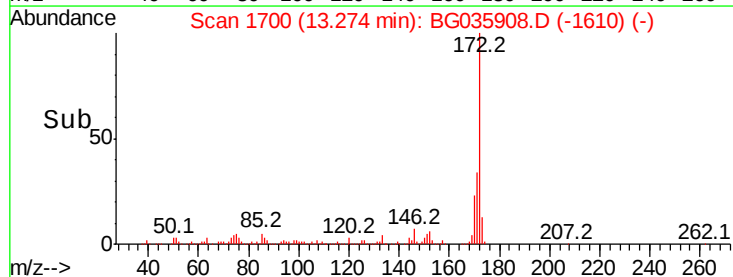
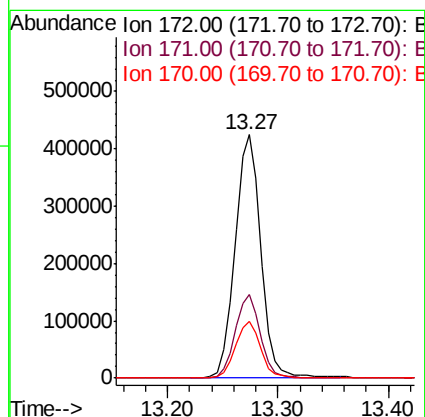
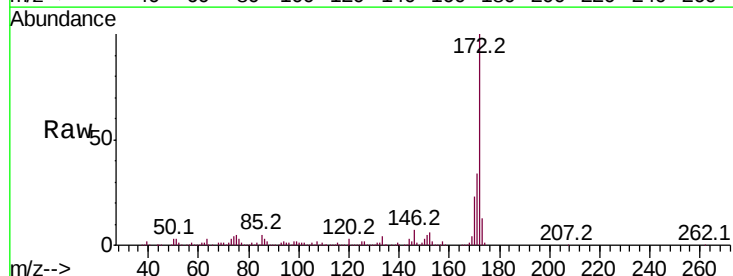


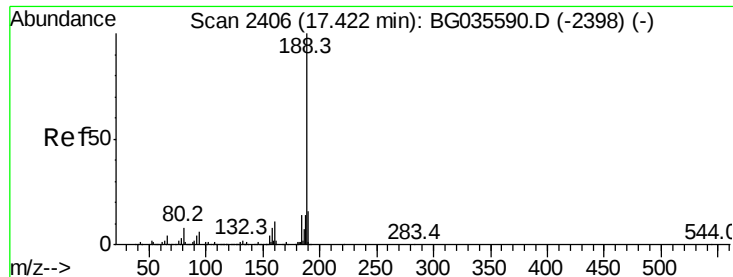

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.39 min Scan# 2401
Delta R.T. -0.00 min
Lab File: BG035908.D
Acq: 26 Jul 2018 14:00




Instrument :
BNA_G
ClientSampleId :
RO-1-3

Tot Ion:188 Resp: 294098
Ion Ratio Lower Upper
188 100
94 6.1 6.9 10.3#
80 7.5 7.7 11.5#

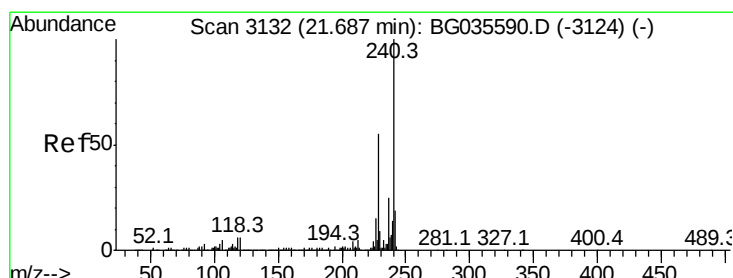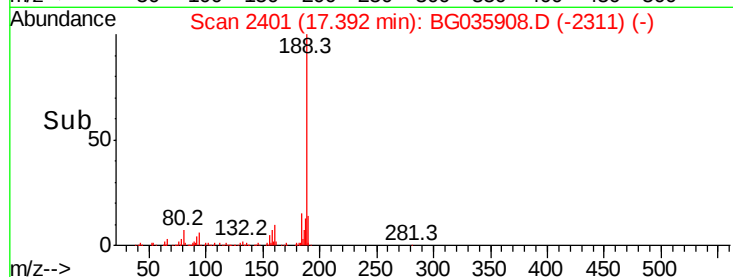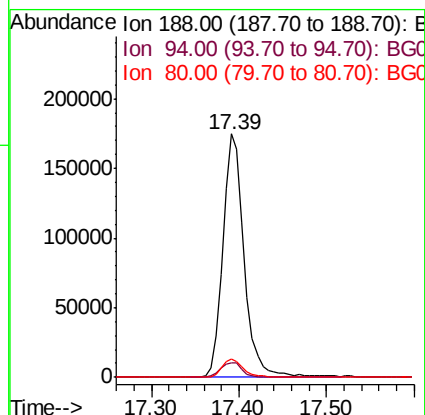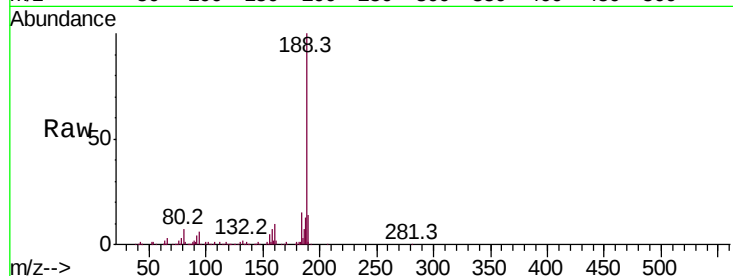

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.66 min Scan# 3127
Delta R.T. -0.00 min
Lab File: BG035908.D
Acq: 26 Jul 2018 14:00

Tgt Ion:240 Resp: 319199
Ion Ratio Lower Upper
240 100
120 5.3 6.8 10.2#
236 25.8 20.9 31.3

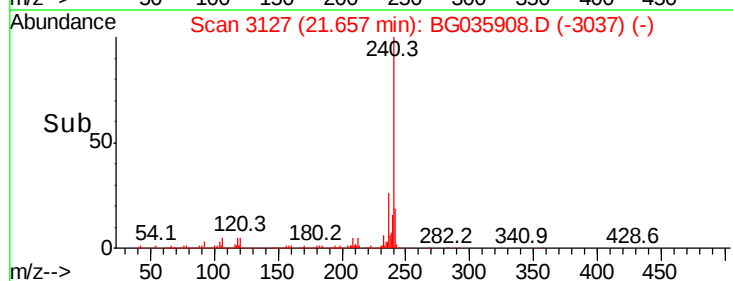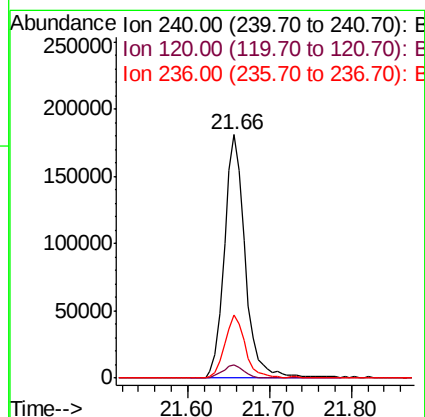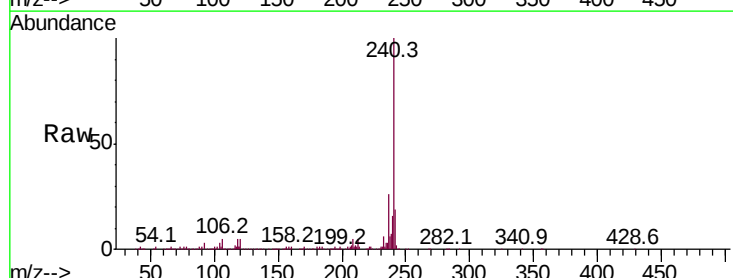



#78

Terphenyl-d14

Concen: 103.690 ng

RT: 20.00 min Scan# 2845

Delta R.T. -0.00 min

Lab File: BG035908.D

Acq: 26 Jul 2018 14:00

Instrument :

BNA_G

ClientSampled :

RO-1-3


Tot Ion:244 Resp: 1501514

Ion Ratio Lower Upper

244 100

212 9.4 5.8 8.8#




122 7.4 7.0 10.4

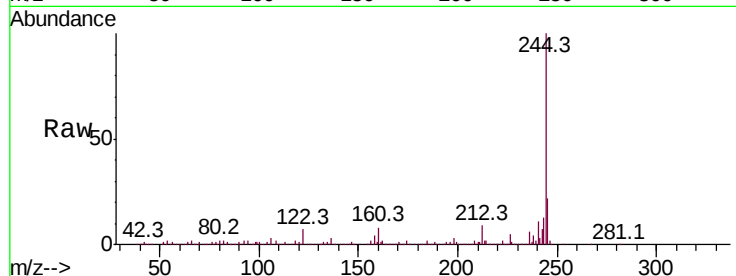

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

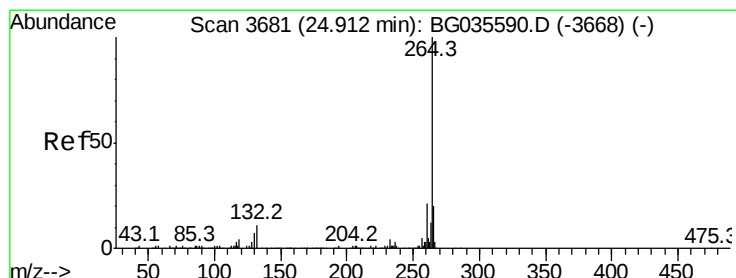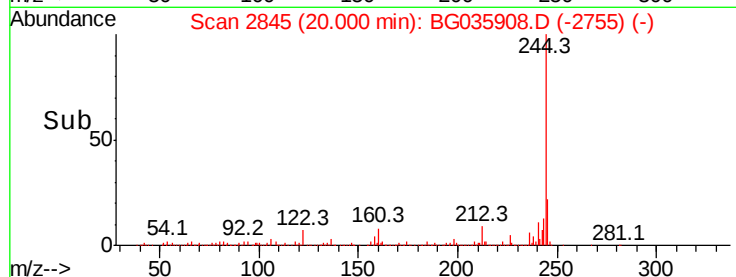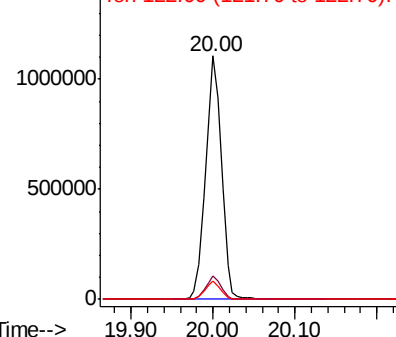

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.86 min Scan# 3672

Delta R.T. -0.00 min

Lab File: BG035908.D

Acq: 26 Jul 2018 14:00


Tgt Ion:264 Resp: 233239

Ion Ratio Lower Upper

264 100

260 24.4 17.4 26.0

265 22.1 17.7 26.5

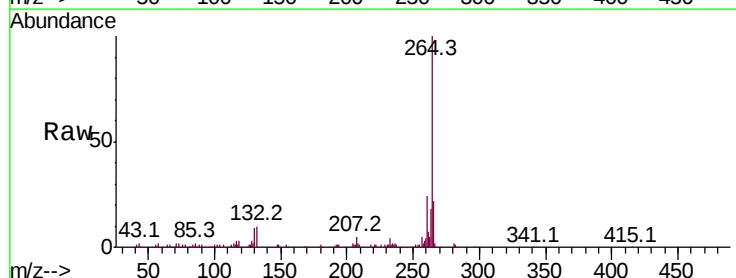

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

