

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG072518\
 Data File : BG035869.D
 Acq On : 25 Jul 2018 11:57
 Operator : JU/SJ
 Sample : J3762-09
 Misc : MDL 1PPM
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MDL-WATER-03-QT3-2018

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.609	388	395	408	rBV	629031	1094930	27.62%	6.778%
2	7.195	658	665	678	rBV	635030	1159032	29.24%	7.175%
3	7.565	719	728	741	rBV	637801	1160912	29.29%	7.187%
4	8.029	799	807	819	rVB	141837	262331	6.62%	1.624%
5	8.352	854	862	874	rVB	546070	968232	24.43%	5.994%
6	9.186	996	1004	1018	rBV	387045	769293	19.41%	4.762%
7	10.831	1273	1284	1292	rBV	165104	323061	8.15%	2.000%
8	13.275	1692	1700	1711	rBV	1223056	1938431	48.91%	12.000%
9	14.650	1927	1934	1942	rBV2	285958	474960	11.98%	2.940%
10	15.695	2107	2112	2119	rBV4	25239	45131	1.14%	0.279%
11	16.136	2177	2187	2202	rBV	970802	1559420	39.34%	9.654%
12	17.393	2393	2401	2407	rBV	408417	655929	16.55%	4.061%
13	19.449	2745	2751	2759	rBV2	22008	40288	1.02%	0.249%
14	19.807	2807	2812	2819	rBV	25192	42935	1.08%	0.266%
15	20.001	2839	2845	2857	rBV	2974610	3963626	100.00%	24.538%
16	21.658	3118	3127	3133	rBV	463555	839001	21.17%	5.194%
17	23.126	3371	3377	3383	rBV6	22655	43421	1.10%	0.269%
18	23.913	3506	3511	3521	rVB5	31460	78107	1.97%	0.484%
19	24.853	3660	3671	3684	rBV3	244870	734221	18.52%	4.545%


Sum of corrected areas: 16153261

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG072518\
Data File : BG035869.D
Acq On : 25 Jul 2018 11:57
Operator : JU/SJ
Sample : J3762-09
Misc : MDL 1PPM
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MDL-WATER-03-QT3-2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

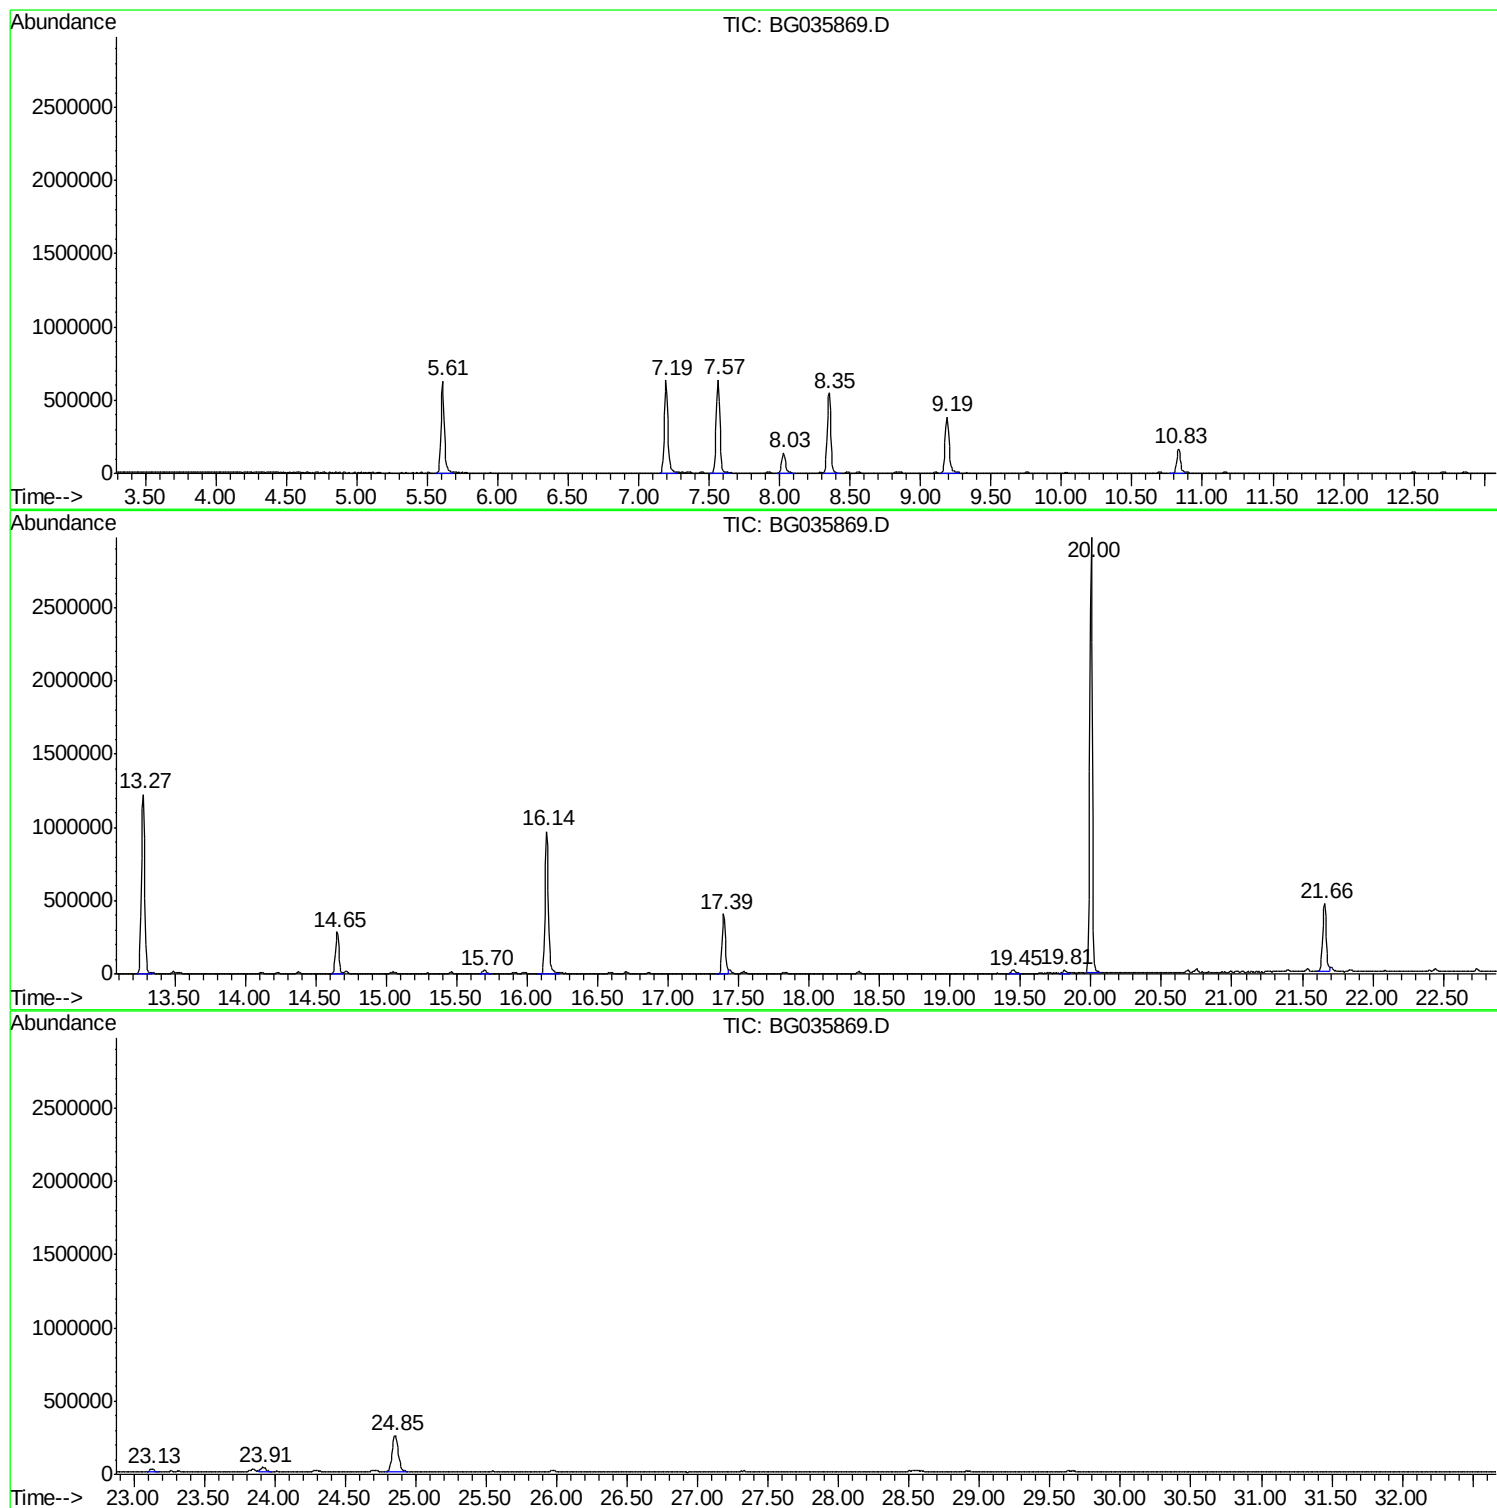

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG072518\
Data_File : BG035869.D
Acq_On : 25-Jul-2018 11:577
Operator : JU/SJJ
Sample : J3762-099
Misc : MDL_1PPMM
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
MDL-WATER-03-QT3-2018

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
