


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072518\
 Data File : BG035874.D
 Acq On : 25 Jul 2018 15:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

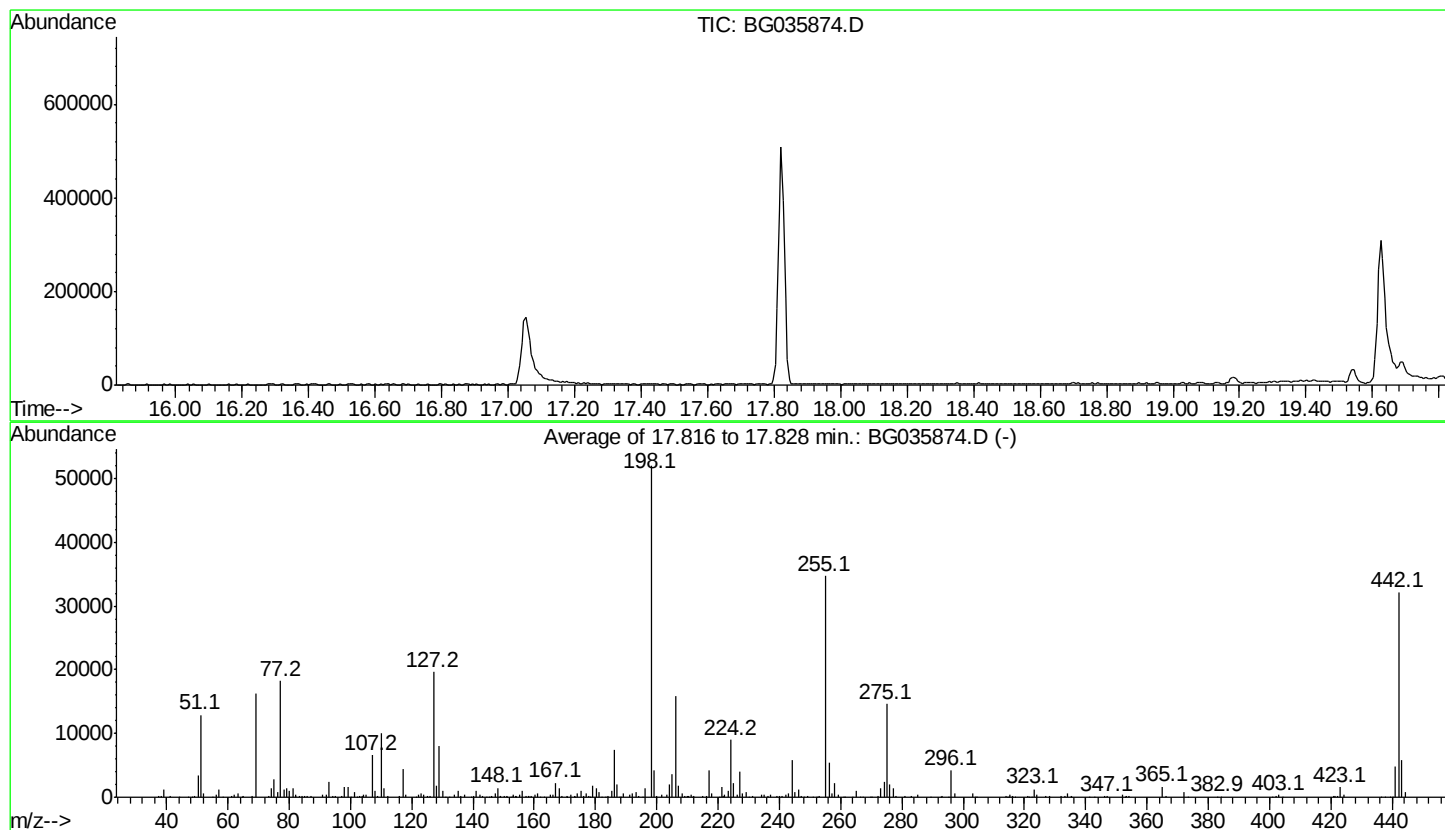

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.9	12949	PASS
68	69	0.00	2	0.7	113	PASS
69	198	0.00	100	31.5	16364	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.7	19632	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52008	PASS
199	198	5	9	8.1	4206	PASS
275	198	10	60	28.0	14566	PASS
365	198	1	100	3.2	1682	PASS
441	198	0.01	100	9.3	4850	PASS
442	198	50	100	61.7	32106	PASS
443	442	15	24	18.3	5886	PASS