


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072518\
 Data File : BG035893.D
 Acq On : 26 Jul 2018 4:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

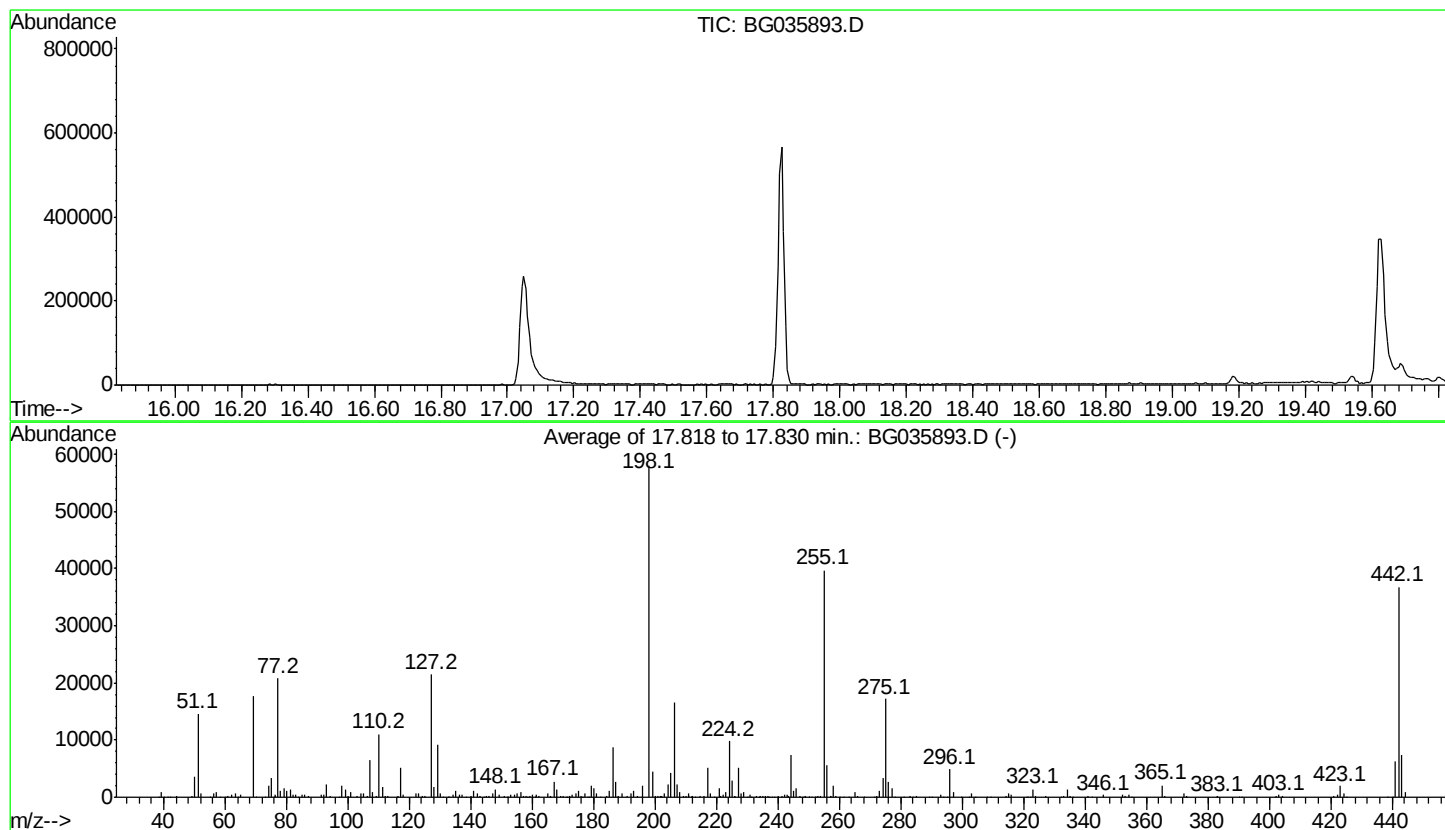

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	14629	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.5	17666	PASS
70	69	0.00	2	0.3	55	PASS
127	198	10	80	37.0	21436	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58000	PASS
199	198	5	9	7.9	4590	PASS
275	198	10	60	29.7	17224	PASS
365	198	1	100	3.6	2112	PASS
441	198	0.01	100	11.0	6364	PASS
442	198	50	100	63.4	36765	PASS
443	442	15	24	19.9	7330	PASS