

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072523\
 Data File : BG058455.D
 Acq On : 25 Jul 2023 21:03
 Operator : CG/JU
 Sample : 03537-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.238	21	25	30	rBV2	11457	15575	0.90%	0.106%
2	3.655	92	96	109	rVB	55126	98366	5.69%	0.667%
3	3.890	133	136	142	rVB5	6455	9576	0.55%	0.065%
4	3.984	150	152	157	rVB4	2816	3663	0.21%	0.025%
5	6.986	658	663	674	rVB2	42496	74265	4.30%	0.503%
6	7.145	684	690	699	rBV	167742	285344	16.51%	1.934%
7	7.345	718	724	738	rBV	151292	266643	15.43%	1.807%
8	7.815	797	804	816	rBV	158280	272191	15.75%	1.845%
9	8.526	919	925	939	rBV	119219	224697	13.00%	1.523%
10	8.978	995	1002	1012	rBV	197095	355287	20.56%	2.408%
11	9.701	1117	1125	1137	rBV	153715	282774	16.36%	1.916%
12	10.241	1210	1217	1234	rBV	220863	419077	24.25%	2.840%
13	10.617	1273	1281	1290	rBV	259521	447757	25.91%	3.035%
14	10.758	1298	1305	1319	rBV	178435	378187	21.88%	2.563%
15	12.221	1548	1554	1556	rBV2	2271	3123	0.18%	0.021%
16	13.349	1739	1746	1752	rVB	3526	5542	0.32%	0.038%
17	13.866	1828	1834	1849	rBV	511625	739872	42.81%	5.014%
18	14.154	1876	1883	1896	rBV	584255	930928	53.87%	6.309%
19	14.460	1929	1935	1948	rVB	426041	670227	38.78%	4.542%
20	14.701	1967	1976	1979	rBV4	4010	8582	0.50%	0.058%
21	14.754	1984	1985	1990	rVB2	1541	1930	0.11%	0.013%
22	15.453	2098	2104	2120	rBV	785916	1204003	69.67%	8.160%
23	15.576	2120	2125	2138	rVV	149437	256139	14.82%	1.736%
24	15.688	2141	2144	2150	rVV5	3919	7638	0.44%	0.052%
25	15.817	2161	2166	2171	rVV	12482	16940	0.98%	0.115%
26	16.017	2195	2200	2203	rBV2	1436	1919	0.11%	0.013%
27	16.164	2222	2225	2228	rBV3	1995	2362	0.14%	0.016%
28	16.916	2348	2353	2356	rVB5	1323	2148	0.12%	0.015%
29	16.957	2356	2360	2363	rBV3	2770	3993	0.23%	0.027%
30	17.204	2396	2402	2412	rBV	543415	836046	48.38%	5.666%
31	17.304	2412	2419	2430	rVV	914656	1416725	81.97%	9.601%
32	17.386	2431	2433	2437	rVB4	5163	6160	0.36%	0.042%
33	17.703	2482	2487	2490	rBV5	1907	3910	0.23%	0.026%
34	18.103	2550	2555	2560	rBV4	17395	35205	2.04%	0.239%
35	18.161	2562	2565	2569	rVB3	4778	7626	0.44%	0.052%
36	18.385	2600	2603	2607	rVV4	2093	3192	0.18%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072523\
 Data File : BG058455.D
 Acq On : 25 Jul 2023 21:03
 Operator : CG/JU
 Sample : 03537-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BH312

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

37	18.984	2701	2705	2708	rBV3	1290	2325	0.13%	0.016%
38	19.013	2708	2710	2714	rVV5	2268	3309	0.19%	0.022%
39	19.160	2728	2735	2742	rBV4	13738	22496	1.30%	0.152%
40	19.237	2743	2748	2752	rBV3	9233	16159	0.93%	0.110%
41	19.389	2770	2774	2776	rBV4	5002	6924	0.40%	0.047%
42	19.519	2793	2796	2802	rBV7	4530	7188	0.42%	0.049%
43	19.595	2803	2809	2823	rVV	1128656	1645377	95.20%	11.151%
44	19.912	2861	2863	2864	rBV2	3011	2719	0.16%	0.018%
45	20.559	2969	2973	2975	rBV5	8570	11211	0.65%	0.076%
46	20.923	3033	3035	3039	rBV5	9607	9719	0.56%	0.066%
47	21.446	3118	3124	3143	rVB	518033	883374	51.11%	5.987%
48	23.608	3489	3492	3502	rVB6	19042	38225	2.21%	0.259%
49	24.301	3600	3610	3622	rBV2	639770	1728256	100.00%	11.713%
50	24.513	3636	3646	3662	rVB	367526	1018759	58.95%	6.904%
51	24.736	3682	3684	3686	rBV2	6432	4495	0.26%	0.030%
52	25.564	3821	3825	3836	rVB4	24232	57391	3.32%	0.389%




Sum of corrected areas: 14755539

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072523\
Data File : BG058455.D
Acq On : 25 Jul 2023 21:03
Operator : CG/JU
Sample : 03537-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

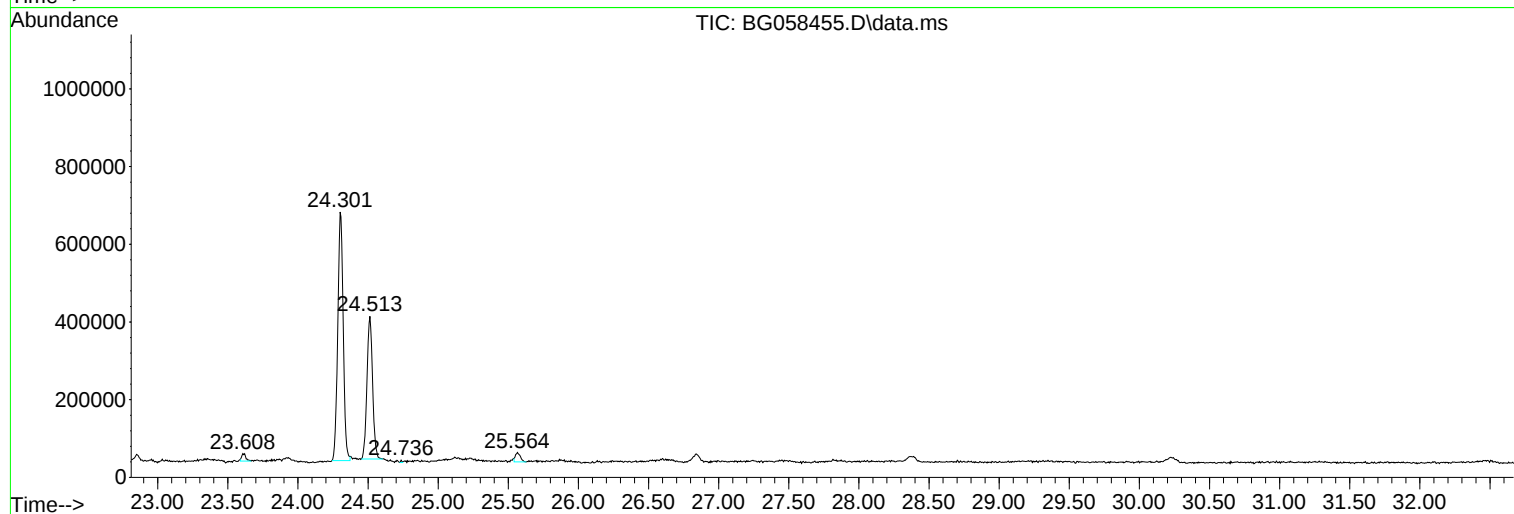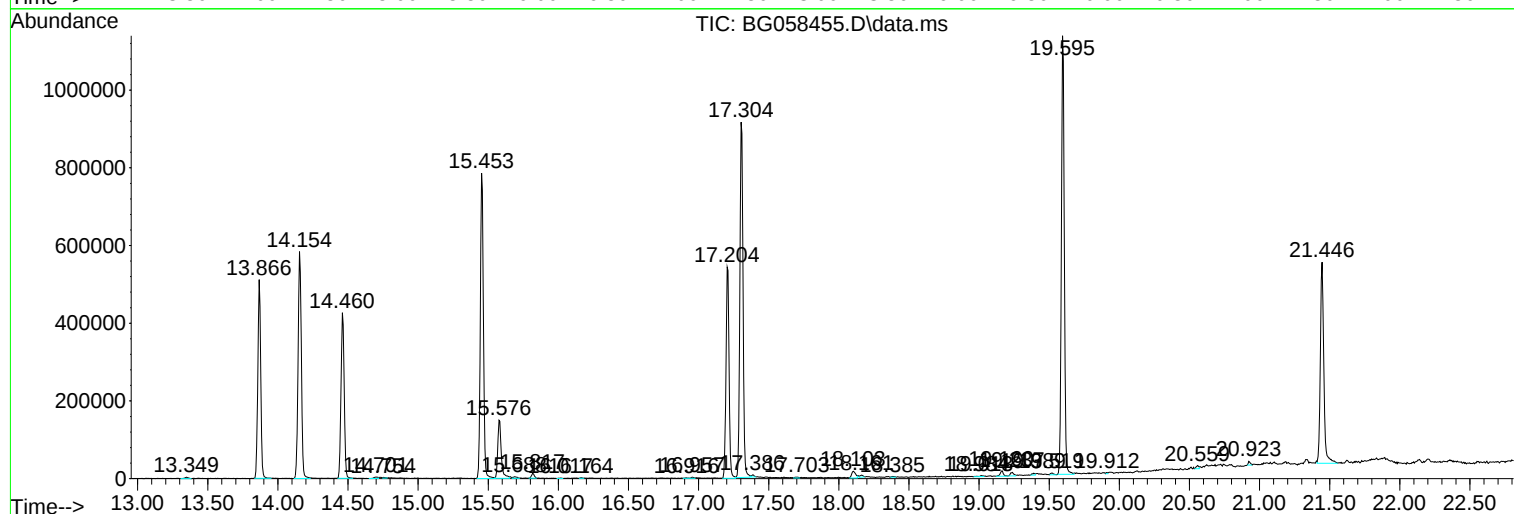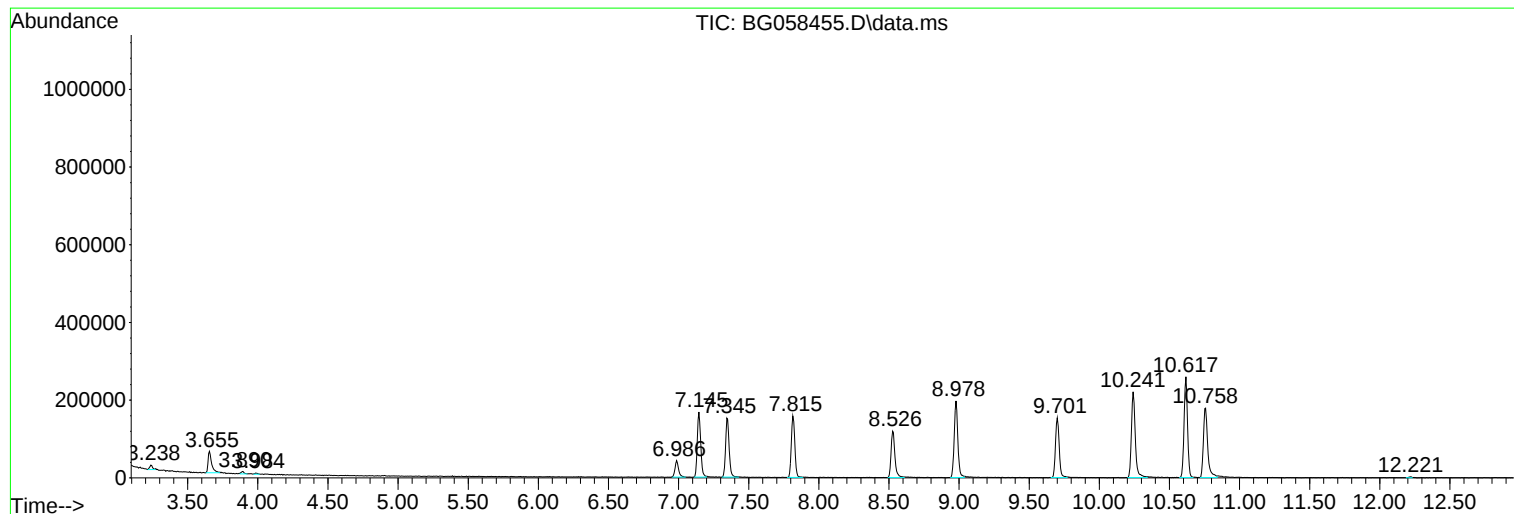

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072523\
Data File : BG058455.D
Acq On : 25 Jul 2023 21:03
Operator : CG/JU
Sample : 03537-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072523\
Data File : BG058455.D
Acq On : 25 Jul 2023 21:03
Operator : CG/JU
Sample : 03537-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BH312

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc