

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
 Data File : BG058483.D
 Acq On : 26 Jul 2023 17:50
 Operator : MA/JU
 Sample : PB154144BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	32	rVB	19980	29072	1.58%	0.147%
2	3.651	91	96	114	rBV	262614	518798	28.15%	2.630%
3	3.992	151	154	161	rVB3	4097	6778	0.37%	0.034%
4	4.456	231	233	236	rBV4	1818	2350	0.13%	0.012%
5	5.103	341	343	350	rBV4	1376	2442	0.13%	0.012%
6	6.983	656	663	679	rBV	293466	530535	28.79%	2.690%
7	7.147	684	691	704	rVB	246377	416053	22.58%	2.109%
8	7.347	718	725	736	rBV	299163	524108	28.44%	2.657%
9	7.817	798	805	816	rVB	195693	347193	18.84%	1.760%
10	8.528	919	926	944	rBV	369712	692127	37.56%	3.509%
11	8.980	995	1003	1015	rBV	308054	552615	29.99%	2.802%
12	9.703	1118	1126	1137	rBV	242719	452488	24.55%	2.294%
13	9.785	1139	1140	1146	rVB	2458	2057	0.11%	0.010%
14	10.244	1209	1218	1241	rBV	349326	702040	38.10%	3.559%
15	10.443	1249	1252	1258	rVB4	1083	1848	0.10%	0.009%
16	10.620	1268	1282	1291	rBV	319623	585869	31.79%	2.970%
17	10.755	1297	1305	1321	rBV	348214	710074	38.53%	3.600%
18	12.212	1547	1553	1562	rBV3	3793	7952	0.43%	0.040%
19	13.358	1741	1748	1752	rBV3	3380	5902	0.32%	0.030%
20	13.869	1828	1835	1851	rBV	738641	1087717	59.03%	5.515%
21	14.157	1877	1884	1897	rBV	847791	1352728	73.41%	6.858%
22	14.462	1929	1936	1945	rBV	558125	853236	46.30%	4.326%
23	14.680	1967	1973	1992	rBV	70486	217593	11.81%	1.103%
24	15.455	2098	2105	2120	rBV	1049159	1627067	88.29%	8.249%
25	15.579	2120	2126	2140	rVV	121610	213052	11.56%	1.080%
26	15.696	2144	2146	2154	rVB2	5514	8016	0.43%	0.041%
27	17.206	2397	2403	2413	rBV	618910	924429	50.16%	4.687%
28	17.306	2413	2420	2436	rVV	1005804	1556484	84.46%	7.891%
29	19.163	2730	2736	2740	rBV2	13635	18915	1.03%	0.096%
30	19.233	2744	2748	2756	rVV3	8971	14849	0.81%	0.075%
31	19.527	2792	2798	2801	rBV7	2151	4382	0.24%	0.022%
32	19.597	2804	2810	2828	rVV	1223419	1735241	94.16%	8.798%
33	20.479	2958	2960	2965	rBV5	1809	3296	0.18%	0.017%
34	20.555	2971	2973	2977	rBV3	4472	5955	0.32%	0.030%
35	20.755	3005	3007	3009	rBV3	2799	1978	0.11%	0.010%
36	20.843	3020	3022	3028	rBV6	2391	4012	0.22%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
 Data File : BG058483.D
 Acq On : 26 Jul 2023 17:50
 Operator : MA/JU
 Sample : PB154144BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

37	21.336	3102	3106	3112	rVB3	11864	17063	0.93%	0.087%
38	21.448	3118	3125	3144	rBV	504442	892363	48.42%	4.524%
39	22.194	3250	3252	3257	rVB4	5762	8087	0.44%	0.041%
40	22.347	3276	3278	3280	rBV3	3530	3002	0.16%	0.015%
41	22.482	3299	3301	3307	rVB	9720	12266	0.67%	0.062%
42	22.858	3360	3365	3372	rVB5	13112	23256	1.26%	0.118%
43	23.534	3477	3480	3482	rBV3	7771	9918	0.54%	0.050%
44	23.616	3488	3494	3500	rVB5	25471	53229	2.89%	0.270%
45	24.309	3601	3612	3635	rBV2	571454	1842784	100.00%	9.343%
46	24.515	3637	3647	3662	rVV	306036	949002	51.50%	4.811%
47	25.573	3820	3827	3835	rVB5	23785	63146	3.43%	0.320%
48	26.436	3972	3974	3976	rBV3	2865	2311	0.13%	0.012%
49	26.842	4035	4043	4056	rVB7	21148	78809	4.28%	0.400%
50	28.387	4297	4306	4314	rVB7	14143	45275	2.46%	0.230%
51	28.516	4326	4328	4330	rBV3	3134	2442	0.13%	0.012%
52	30.026	4583	4585	4586	rBV2	2816	2044	0.11%	0.010%




Sum of corrected areas: 19724248

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
Data File : BG058483.D
Acq On : 26 Jul 2023 17:50
Operator : MA/JU
Sample : PB154144BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK144

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

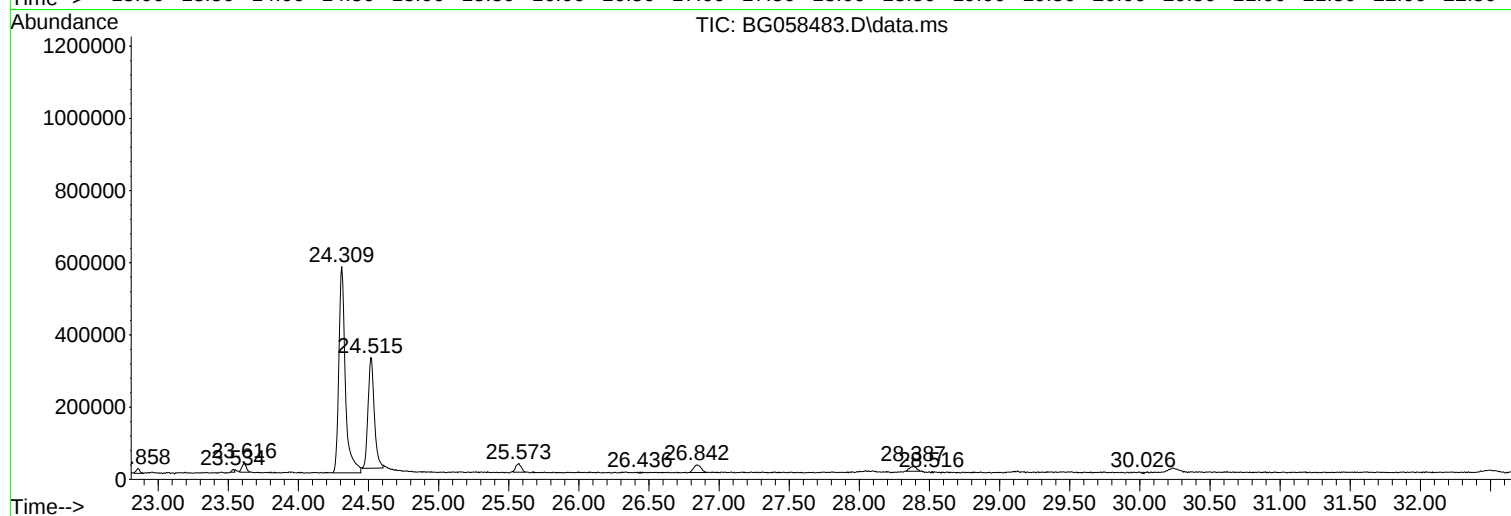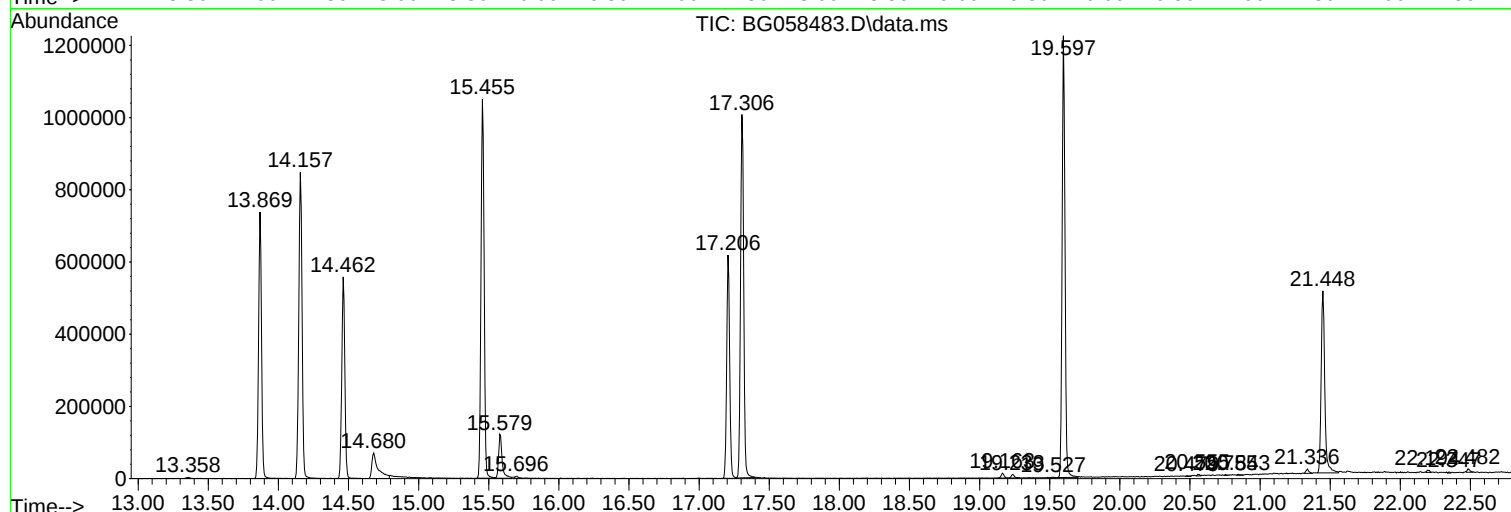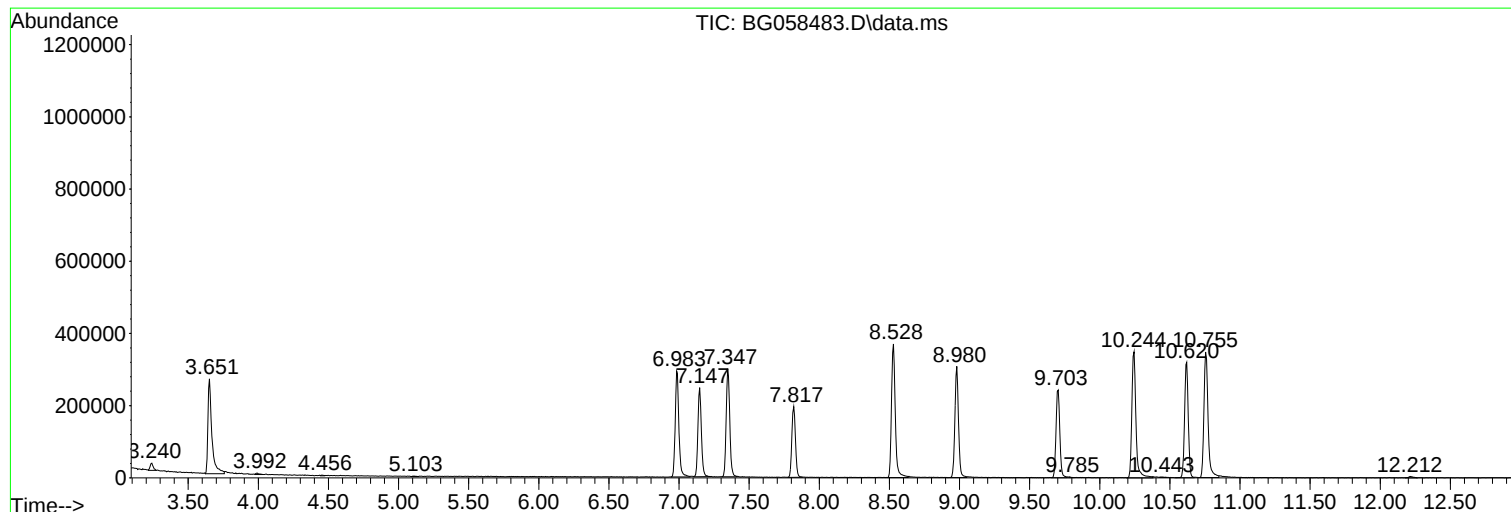

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
Data File : BG058483.D
Acq On : 26 Jul 2023 17:50
Operator : MA/JU
Sample : PB154144BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK144

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
Data File : BG058483.D
Acq On : 26 Jul 2023 17:50
Operator : MA/JU
Sample : PB154144BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK144

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------