

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
 Data File : BG058491.D
 Acq On : 26 Jul 2023 23:23
 Operator : MA/JU
 Sample : 03553-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4701

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	31	rVB2	13136	17792	0.87%	0.110%
2	3.651	92	96	110	rBV	69855	136286	6.70%	0.839%
3	3.892	132	137	142	rVB3	7664	12090	0.59%	0.074%
4	6.983	657	663	672	rBV	44227	78083	3.84%	0.481%
5	7.141	683	690	705	rBV	210150	364841	17.93%	2.247%
6	7.347	719	725	735	rBV	182188	323267	15.88%	1.991%
7	7.817	799	805	812	rBV	137204	239164	11.75%	1.473%
8	7.876	812	815	822	rVB2	4148	6864	0.34%	0.042%
9	8.528	919	926	940	rBV	125899	245579	12.07%	1.512%
10	8.975	995	1002	1015	rBV	239192	444368	21.83%	2.736%
11	9.133	1026	1029	1031	rBV4	1752	2218	0.11%	0.014%
12	9.380	1067	1071	1077	rVB5	3093	5083	0.25%	0.031%
13	9.697	1118	1125	1137	rBV	188314	350848	17.24%	2.161%
14	10.238	1211	1217	1237	rBV	244520	501944	24.66%	3.091%
15	10.614	1273	1281	1289	rBV	207095	375266	18.44%	2.311%
16	10.755	1296	1305	1323	rBV	235283	491684	24.16%	3.028%
17	11.871	1491	1495	1502	rBV2	3520	5359	0.26%	0.033%
18	12.224	1549	1555	1560	rBV2	2821	5664	0.28%	0.035%
19	13.352	1740	1747	1753	rBV3	4341	7259	0.36%	0.045%
20	13.869	1828	1835	1846	rBV	594968	897715	44.11%	5.528%
21	14.157	1876	1884	1905	rBV	686220	1108859	54.48%	6.829%
22	14.462	1929	1936	1946	rBV	356245	554446	27.24%	3.414%
23	14.727	1973	1981	1984	rBV5	3076	7987	0.39%	0.049%
24	15.455	2098	2105	2120	rBV	934956	1439295	70.72%	8.863%
25	15.579	2120	2126	2139	rVV	131538	225643	11.09%	1.390%
26	15.696	2143	2146	2150	rVB3	4754	6392	0.31%	0.039%
27	15.820	2161	2167	2171	rBV2	6229	11008	0.54%	0.068%
28	15.867	2171	2175	2179	rVB	6271	8993	0.44%	0.055%
29	16.959	2356	2361	2364	rBV4	4624	5793	0.28%	0.036%
30	17.206	2396	2403	2412	rBV	476682	723213	35.53%	4.454%
31	17.306	2412	2420	2433	rBV	1059690	1641222	80.64%	10.107%
32	17.482	2444	2450	2456	rVB	26626	35758	1.76%	0.220%
33	17.829	2505	2509	2512	rBV3	2091	3062	0.15%	0.019%
34	18.164	2561	2566	2572	rVV	50158	68224	3.35%	0.420%
35	18.240	2575	2579	2586	rBV2	3469	5660	0.28%	0.035%
36	18.346	2594	2597	2599	rBV3	3716	3977	0.20%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
 Data File : BG058491.D
 Acq On : 26 Jul 2023 23:23
 Operator : MA/JU
 Sample : 03553-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4701

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

37	18.387	2599	2604	2609	rVV3	4402	8588	0.42%	0.053%
38	18.951	2696	2700	2703	rVB3	1321	2037	0.10%	0.013%
39	19.016	2708	2711	2715	rBV2	1979	2641	0.13%	0.016%
40	19.157	2730	2735	2741	rVB2	14803	22593	1.11%	0.139%
41	19.233	2741	2748	2759	rBV	12529	24555	1.21%	0.151%
42	19.515	2790	2796	2801	rBV3	6448	12299	0.60%	0.076%
43	19.597	2803	2810	2819	rBV	1375581	1947934	95.71%	11.996%
44	20.120	2898	2899	2904	rVB4	2563	2541	0.12%	0.016%
45	20.555	2970	2973	2976	rBV4	3805	4458	0.22%	0.027%
46	20.620	2980	2984	2987	rBV4	3008	5339	0.26%	0.033%
47	20.796	3011	3014	3018	rBV5	3309	4179	0.21%	0.026%
48	20.925	3033	3036	3041	rVB5	10960	13921	0.68%	0.086%
49	21.337	3102	3106	3109	rBV2	16624	20710	1.02%	0.128%
50	21.448	3118	3125	3133	rBV	436889	757861	37.24%	4.667%
51	22.200	3248	3253	3258	rVB6	7761	11678	0.57%	0.072%
52	22.852	3359	3364	3368	rBV6	10104	18116	0.89%	0.112%
53	23.287	3436	3438	3439	rBV2	2994	2203	0.11%	0.014%
54	23.616	3488	3494	3499	rBV4	16150	33103	1.63%	0.204%
55	24.304	3600	3611	3636	rBV2	622357	2035270	100.00%	12.533%
56	24.515	3637	3647	3663	rVB	270505	830375	40.80%	5.114%
57	25.567	3819	3826	3834	rVB3	18678	50613	2.49%	0.312%
58	26.836	4036	4042	4052	rVB6	19269	60390	2.97%	0.372%
59	27.447	4144	4146	4148	rVB3	3079	2060	0.10%	0.013%
60	29.838	4551	4553	4554	rBV2	3110	2139	0.11%	0.013%
61	30.920	4735	4737	4738	rBV2	2830	2151	0.11%	0.013%




Sum of corrected areas: 16238660

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
Data File : BG058491.D
Acq On : 26 Jul 2023 23:23
Operator : MA/JU
Sample : 03553-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4701

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

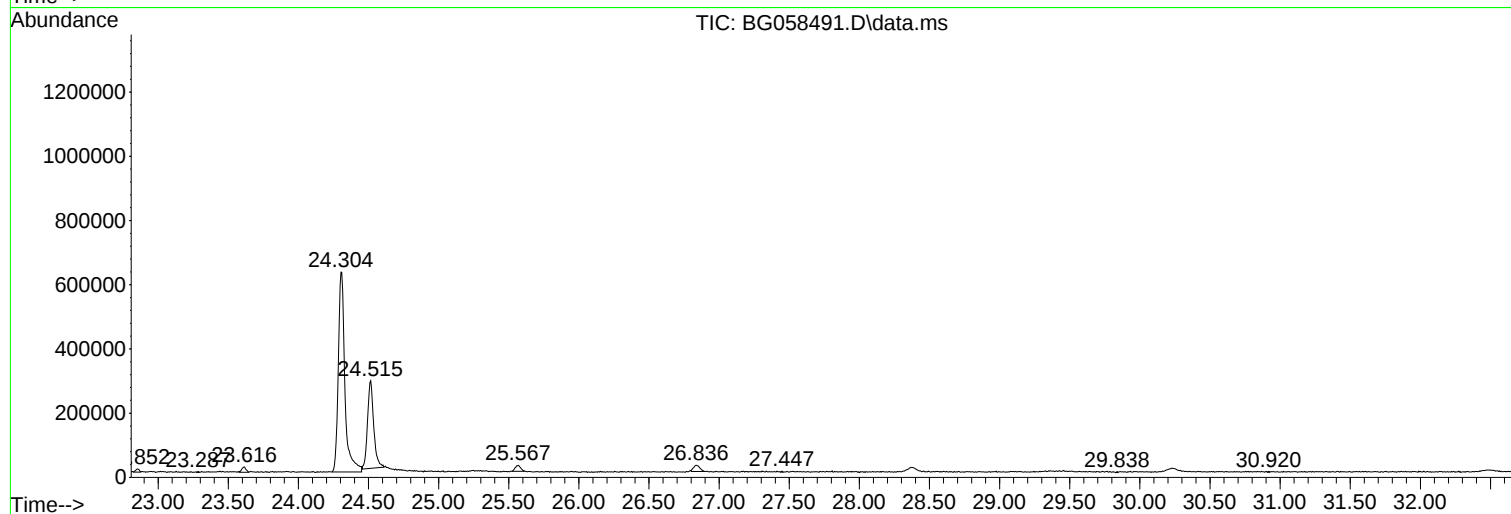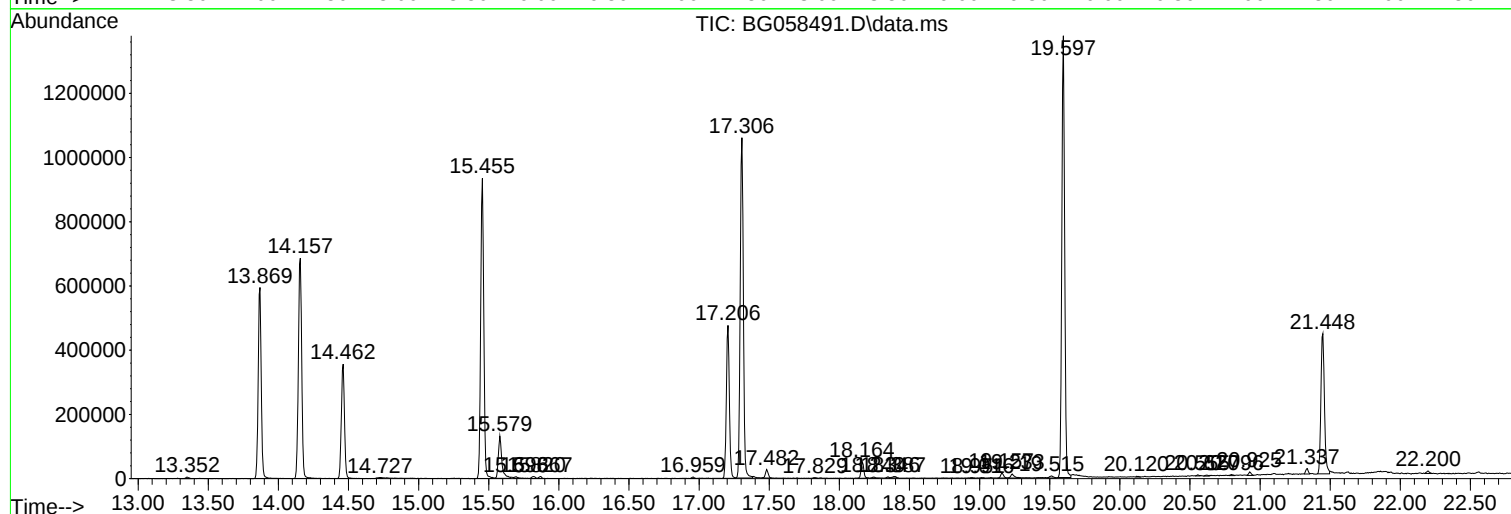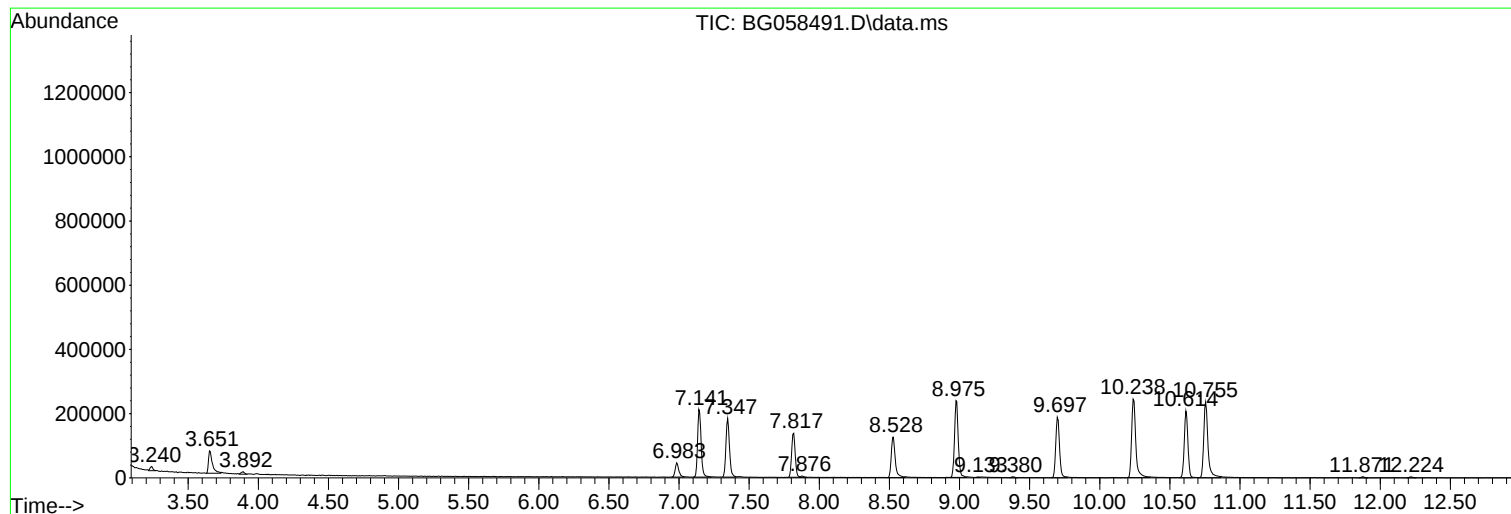

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
Data File : BG058491.D
Acq On : 26 Jul 2023 23:23
Operator : MA/JU
Sample : 03553-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4701

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
Data File : BG058491.D
Acq On : 26 Jul 2023 23:23
Operator : MA/JU
Sample : 03553-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4701

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc