
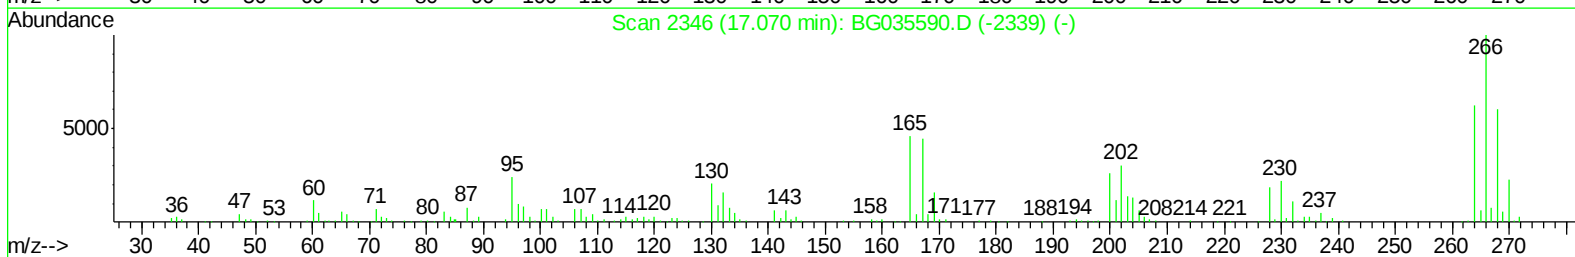
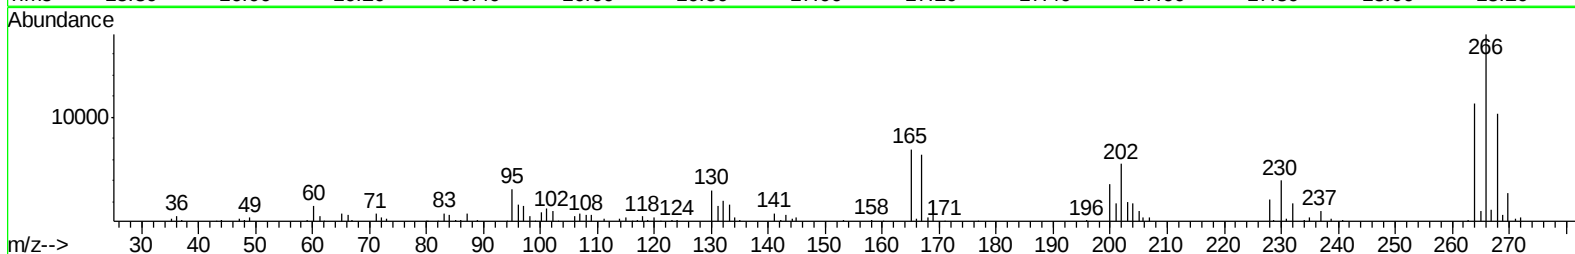


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG072618\  
Data File : BG035911.D  
Acq On : 26 Jul 2018 16:35  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 06:04:09 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG071218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 25 11:04:14 2018  
Response via : Initial Calibration

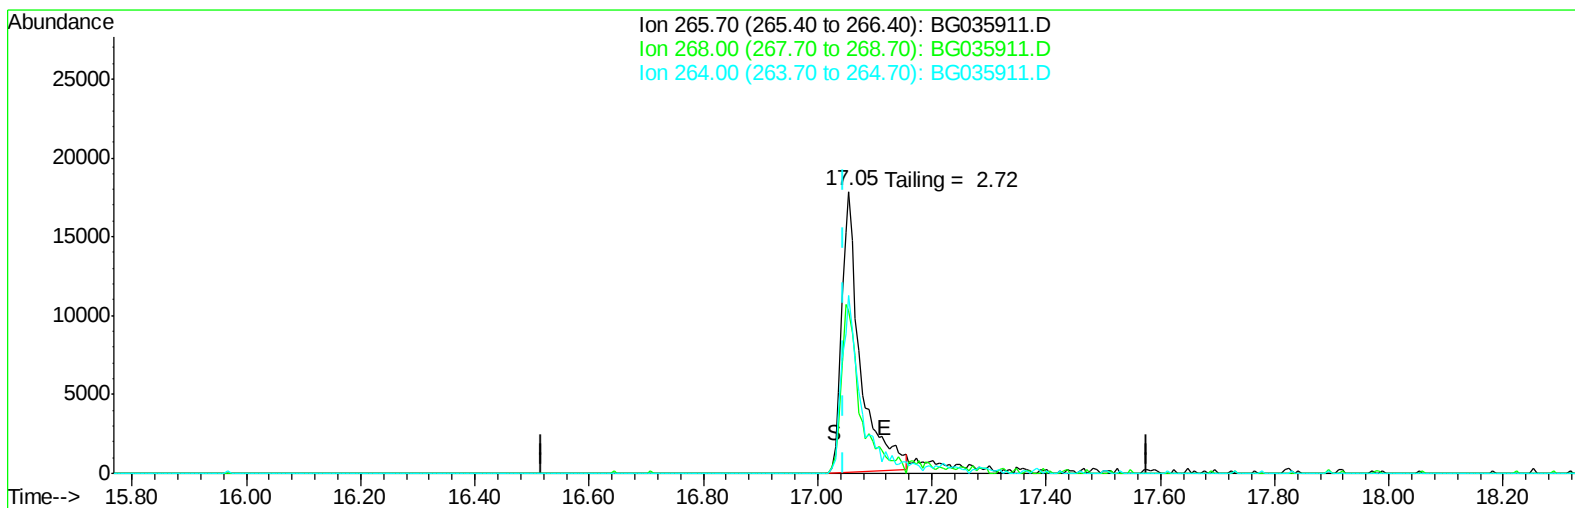

TIC: BG035911.D

(69) Pentachlorophenol (C)

17.054min (+0.007) 77167.43ng

response 40994

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 57.59 |
| 264.00 | 62.00 | 63.19 |
| 0.00   | 0.00  | 0.00  |