
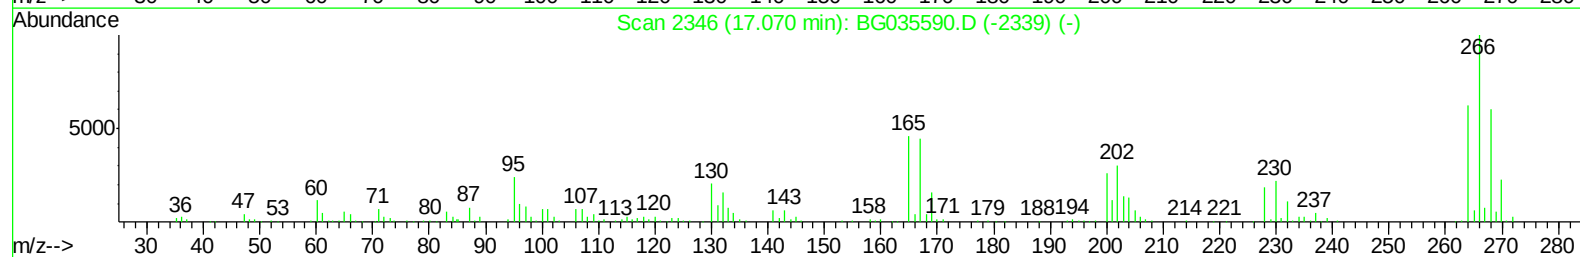
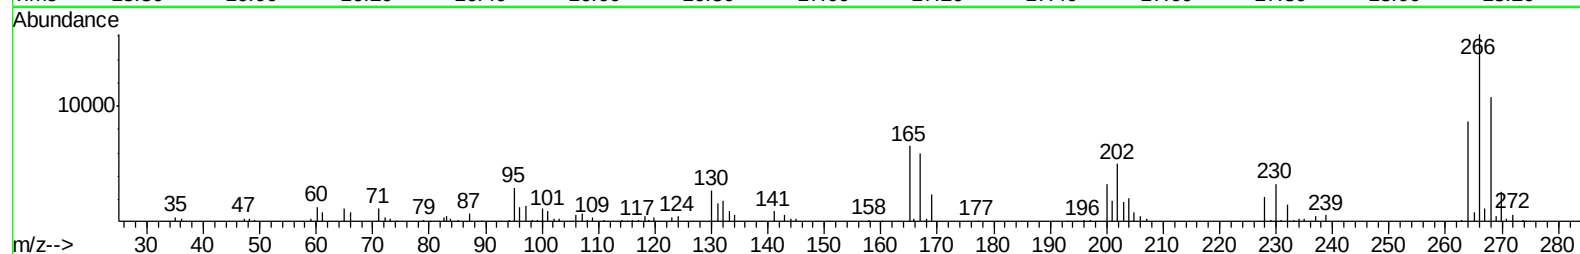


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072718\
Data File : BG035929.D
Acq On : 27 Jul 2018 9:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 05:20:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

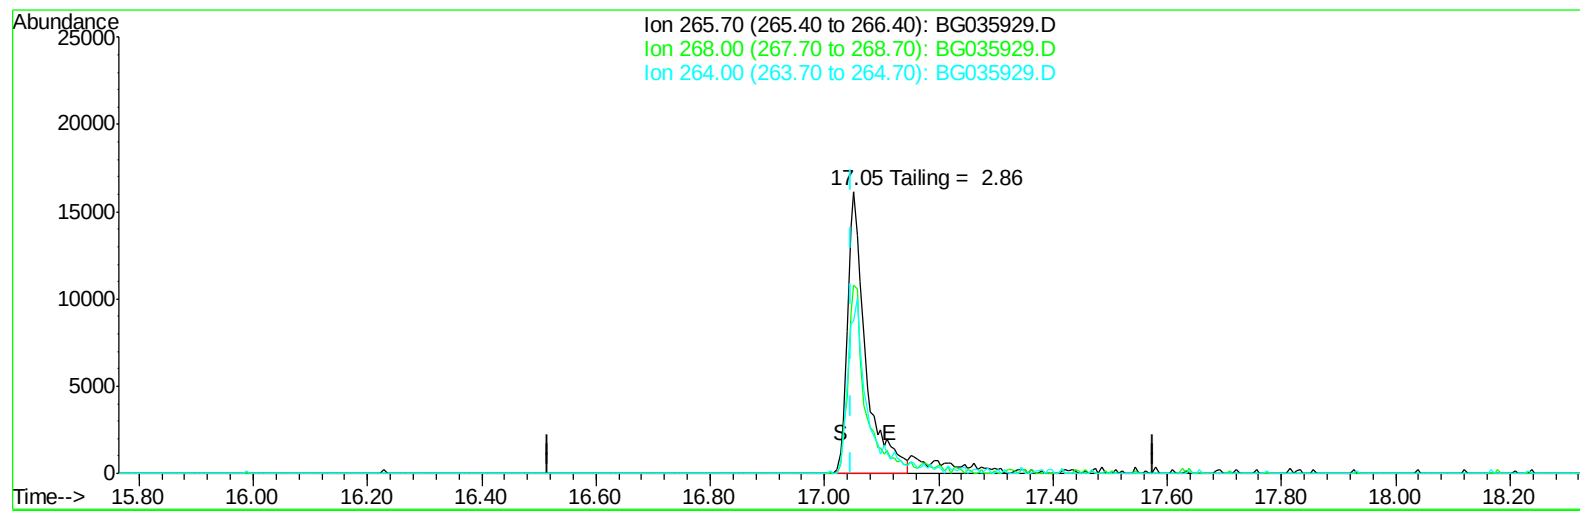

TIC: BG035929.D

(69) Pentachlorophenol (C)




17.051min (+0.004) 88292.10ng

response 35981

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.61
264.00	62.00	54.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072718\
 Data File : BG035929.D
 Acq On : 27 Jul 2018 9:36
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 05:20:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 25 11:04:14 2018
 Response via : Initial Calibration

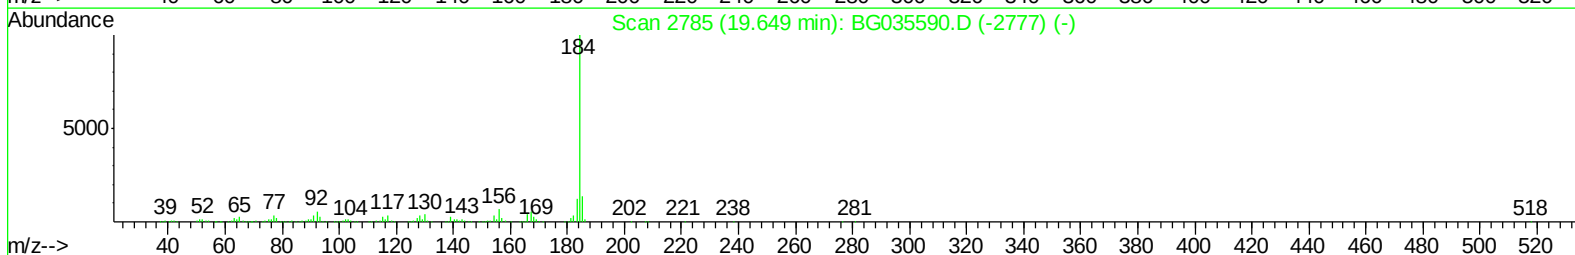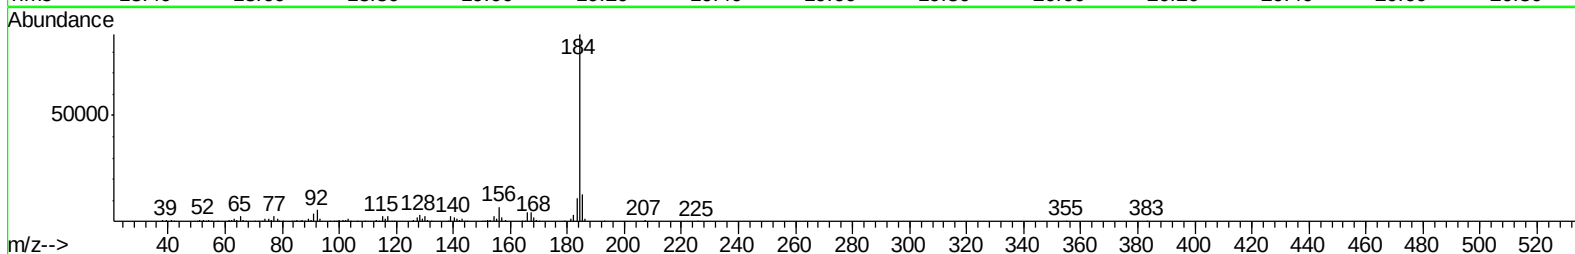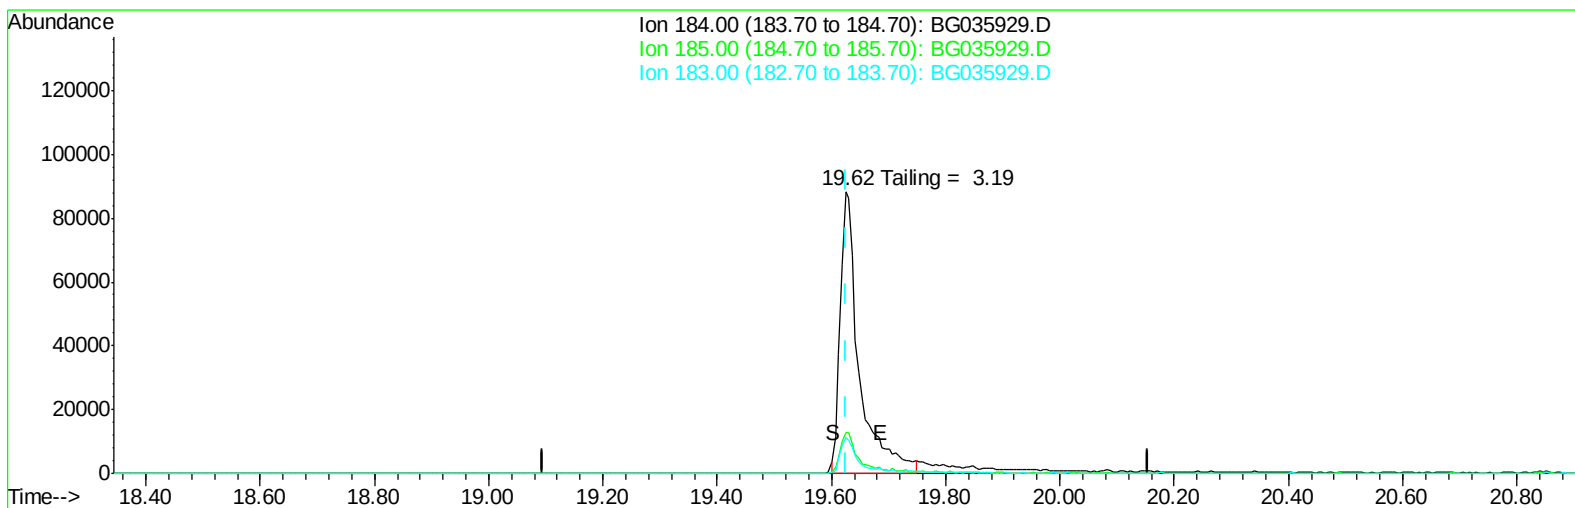

TIC: BG035929.D

(76) Benzidine

19.624min (-0.002) 58323.07ng

response 205466

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.71
183.00	13.30	12.80
0.00	0.00	0.00