
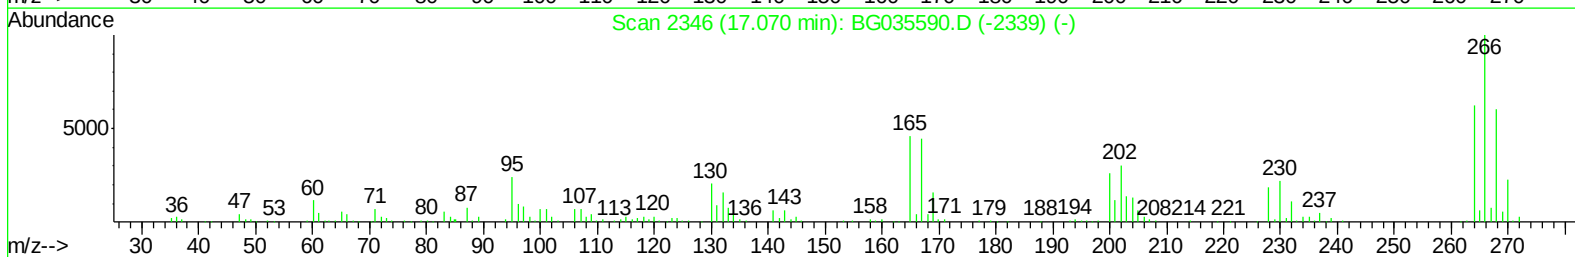
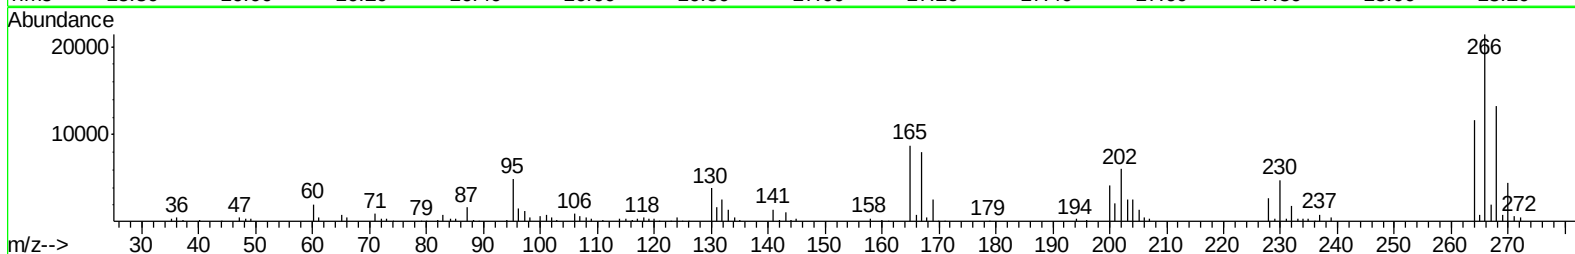


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072718\
Data File : BG035948.D
Acq On : 27 Jul 2018 22:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 05:25:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

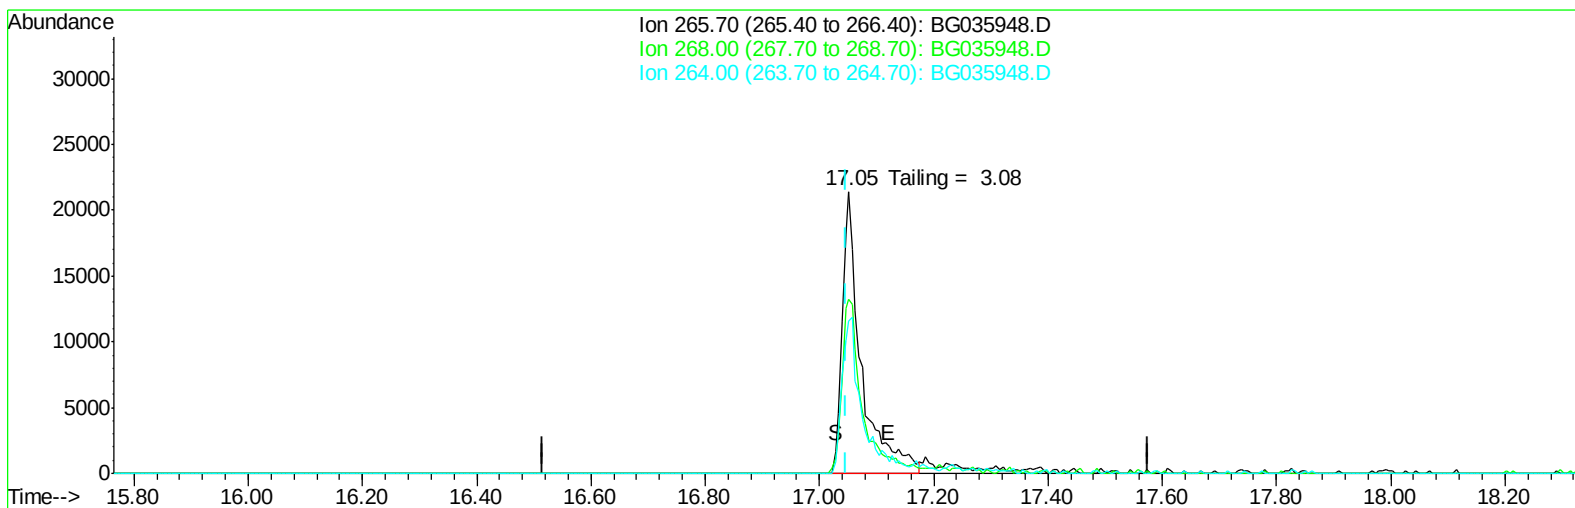

TIC: BG035948.D

(69) Pentachlorophenol (C)




17.051min (+0.004) 92930.72ng

response 49368

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.92
264.00	62.00	54.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072718\
Data File : BG035948.D
Acq On : 27 Jul 2018 22:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 05:25:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

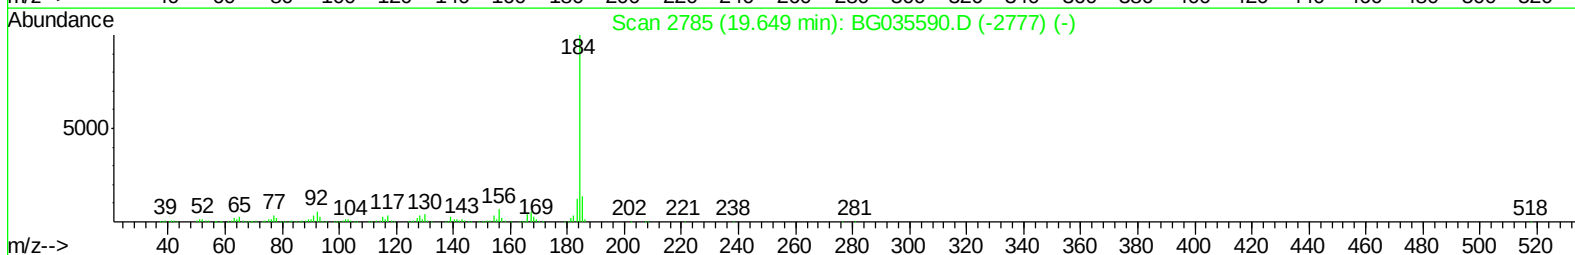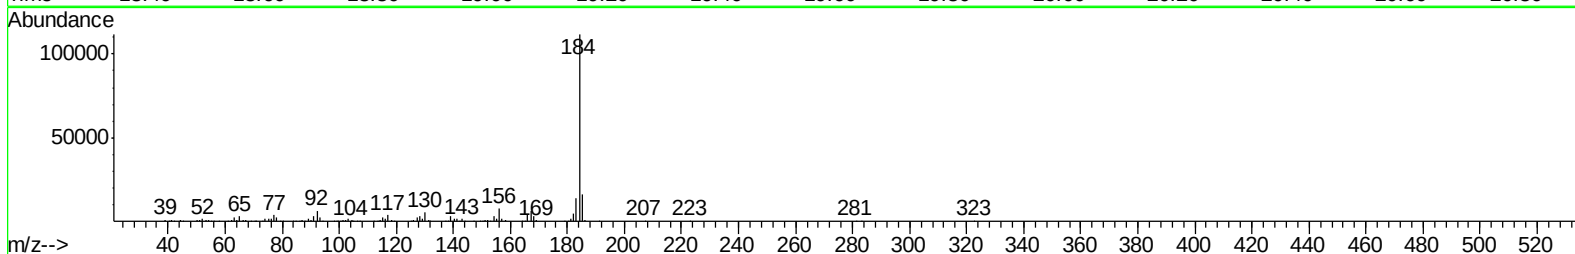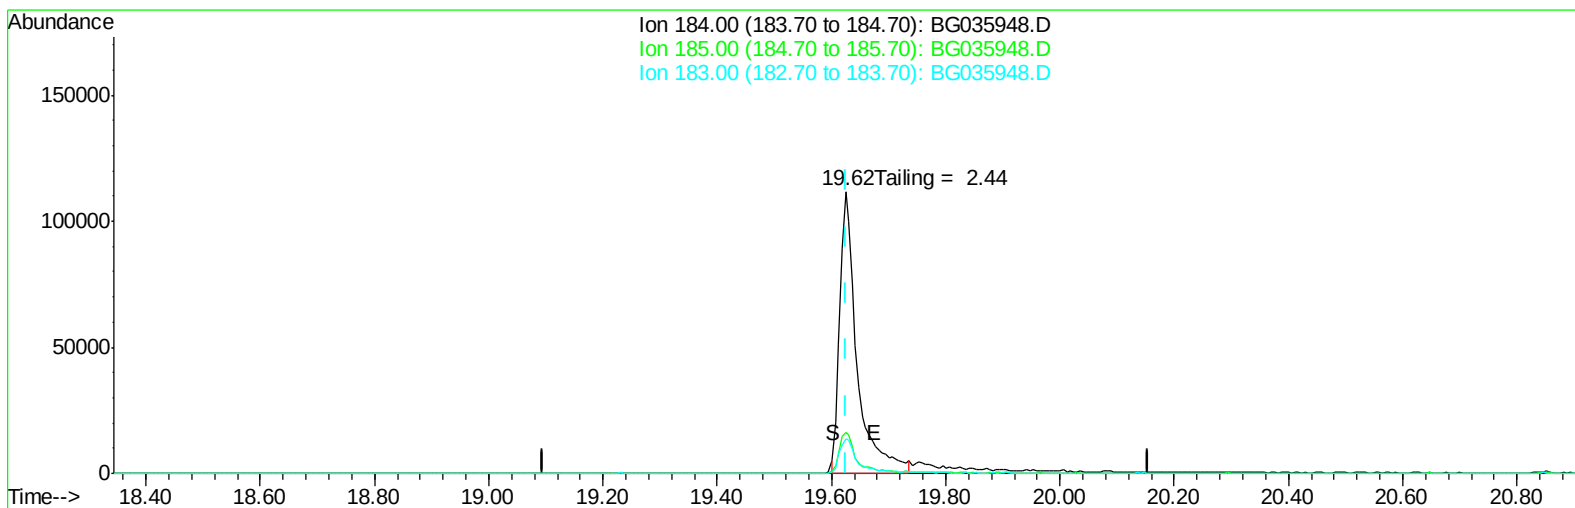

TIC: BG035948.D

(76) Benzidine

19.624min (-0.002) 147713.26ng

response 240772

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.47
183.00	13.30	12.21
0.00	0.00	0.00