


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072718\
Data File : BG035929.D
Acq On : 27 Jul 2018 9:36
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 31 12:30:06 2018

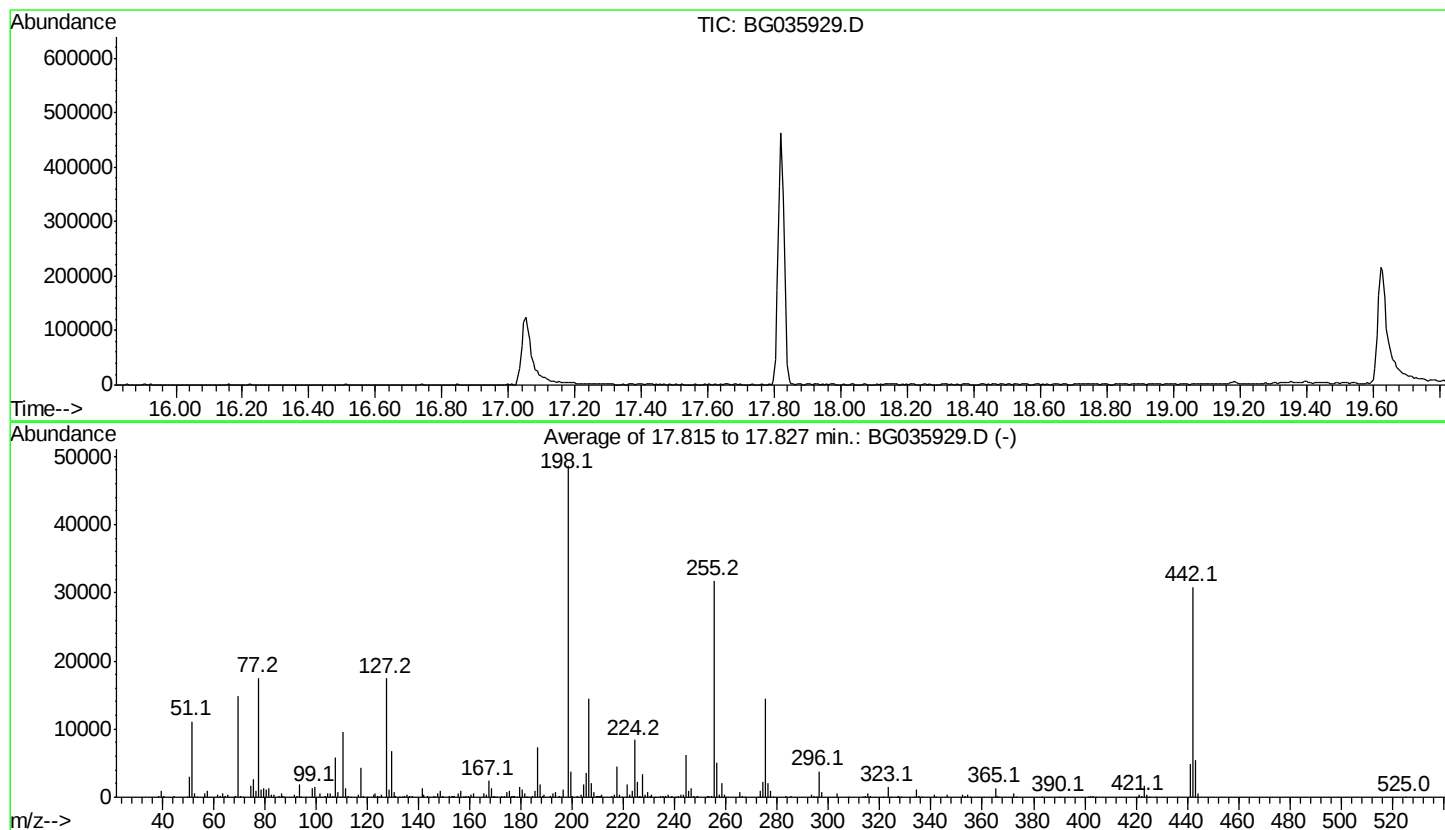

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	11174	PASS
68	69	0.00	2	1.6	243	PASS
69	198	0.00	100	30.4	14801	PASS
70	69	0.00	2	0.9	133	PASS
127	198	10	80	35.9	17444	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48648	PASS
199	198	5	9	7.6	3701	PASS
275	198	10	60	29.7	14435	PASS
365	198	1	100	2.8	1341	PASS
441	198	0.01	100	10.1	4922	PASS
442	198	50	100	63.5	30896	PASS
443	442	15	24	17.6	5431	PASS