


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG072719\
 Data File : BG041774.D
 Acq On : 27 Jul 2019 13:12
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG072719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 29 12:47:21 2019

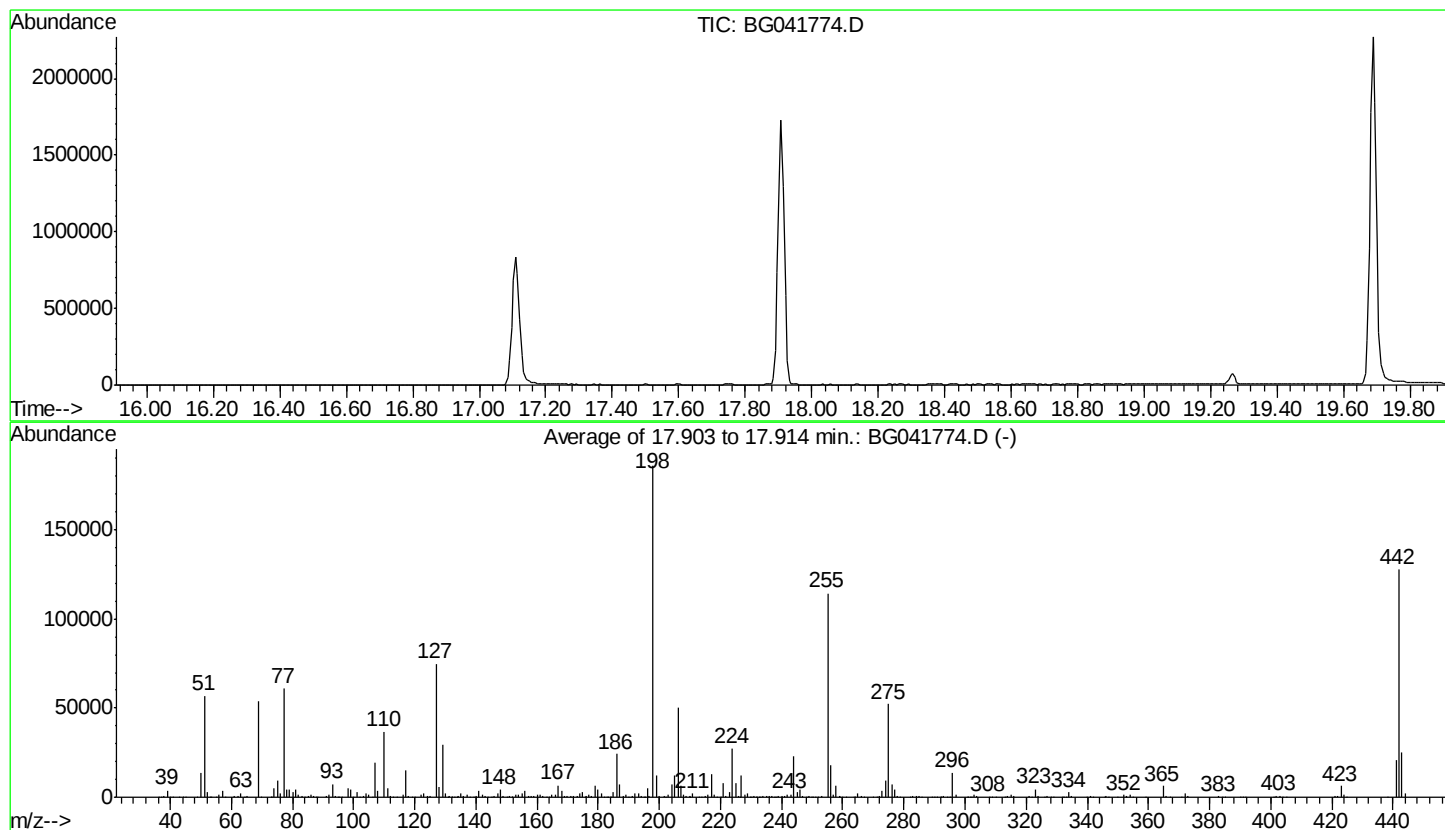

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	56794	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.1	54094	PASS
70	69	0.00	2	0.4	211	PASS
127	198	10	80	40.2	74690	PASS
197	198	0.00	2	0.2	451	PASS
198	198	100	100	100.0	185984	PASS
199	198	5	9	6.7	12544	PASS
275	198	10	60	28.1	52333	PASS
365	198	1	100	3.4	6268	PASS
441	198	0.01	100	11.2	20808	PASS
442	198	50	100	68.6	127645	PASS
443	442	15	24	19.7	25181	PASS