

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
 Data File : BG058497.D
 Acq On : 27 Jul 2023 12:06
 Operator : MA/JU
 Sample : PB154055BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.241	22	26	32	rVB3	15038	21407	1.76%	0.171%
2	3.652	91	96	109	rBV	151079	274027	22.55%	2.185%
3	5.068	336	337	340	rBV2	2027	1279	0.11%	0.010%
4	6.984	656	663	674	rBV	172582	307026	25.27%	2.448%
5	7.142	684	690	703	rVB	138138	238754	19.65%	1.904%
6	7.348	718	725	739	rVB	173384	301584	24.82%	2.405%
7	7.818	798	805	819	rVB	166571	292159	24.05%	2.330%
8	8.529	919	926	938	rBV	184153	358825	29.53%	2.861%
9	8.852	980	981	985	rBV3	1212	1308	0.11%	0.010%
10	8.976	995	1002	1014	rBV	153484	292481	24.07%	2.332%
11	9.222	1041	1044	1046	rVB	1272	1568	0.13%	0.013%
12	9.258	1046	1050	1054	rBV3	1356	2583	0.21%	0.021%
13	9.698	1118	1125	1135	rBV	123133	231946	19.09%	1.850%
14	10.245	1210	1218	1233	rBV	167434	355296	29.24%	2.833%
15	10.615	1273	1281	1293	rBV	240752	447411	36.83%	3.568%
16	10.756	1298	1305	1320	rBV	158211	347399	28.59%	2.770%
17	13.353	1744	1747	1752	rVB2	1688	2379	0.20%	0.019%
18	13.864	1828	1834	1849	rBV	359143	562619	46.31%	4.486%
19	14.158	1876	1884	1903	rBV2	428040	711174	58.53%	5.671%
20	14.463	1929	1936	1948	rVB	409852	638119	52.52%	5.088%
21	14.687	1969	1974	1983	rBV2	24782	71804	5.91%	0.573%
22	14.798	1992	1993	2003	rVB4	3531	5959	0.49%	0.048%
23	14.927	2014	2015	2019	rVB4	1652	1664	0.14%	0.013%
24	15.456	2098	2105	2118	rBV	582403	907651	74.71%	7.238%
25	15.580	2122	2126	2135	rBV	47971	86836	7.15%	0.692%
26	15.697	2142	2146	2149	rVV4	2835	3419	0.28%	0.027%
27	16.014	2194	2200	2204	rBV2	669	1233	0.10%	0.010%
28	17.207	2396	2403	2413	rBV	537708	815273	67.10%	6.501%
29	17.307	2413	2420	2435	rVV	633695	1002975	82.55%	7.998%
30	18.171	2563	2567	2570	rBV2	852	1276	0.11%	0.010%
31	19.164	2732	2736	2741	rBV3	7829	11063	0.91%	0.088%
32	19.234	2743	2748	2752	rBV2	7133	10133	0.83%	0.081%
33	19.522	2795	2797	2799	rBV2	1610	1460	0.12%	0.012%
34	19.598	2804	2810	2823	rBV	804543	1214959	100.00%	9.688%
35	20.022	2880	2882	2885	rBV4	1279	1382	0.11%	0.011%
36	20.051	2885	2887	2890	rVV3	1269	1259	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
 Data File : BG058497.D
 Acq On : 27 Jul 2023 12:06
 Operator : MA/JU
 Sample : PB154055BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK055

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

37	20.127	2898	2900	2903	rVB4	1326	1354	0.11%	0.011%
38	20.210	2912	2914	2915	rBV2	1560	1236	0.10%	0.010%
39	20.327	2928	2934	2938	rBV6	1261	3448	0.28%	0.027%
40	20.486	2959	2961	2964	rBV3	1208	1224	0.10%	0.010%
41	20.515	2964	2966	2971	rVV5	2103	2894	0.24%	0.023%
42	20.550	2971	2972	2973	rVV	2050	1351	0.11%	0.011%
43	20.621	2981	2984	2985	rBV2	1397	1477	0.12%	0.012%
44	20.633	2985	2986	2989	rVB3	2116	1374	0.11%	0.011%
45	20.715	2998	3000	3003	rBV2	1825	1445	0.12%	0.012%
46	20.868	3024	3026	3029	rVB3	2168	2185	0.18%	0.017%
47	20.897	3029	3031	3032	rBV2	1743	1374	0.11%	0.011%
48	21.332	3103	3105	3111	rVB5	3544	4857	0.40%	0.039%
49	21.379	3111	3113	3114	rBV2	2117	1859	0.15%	0.015%
50	21.449	3118	3125	3140	rBV	455517	851338	70.07%	6.789%
51	22.195	3250	3252	3258	rVB6	5687	7870	0.65%	0.063%
52	22.765	3347	3349	3350	rBV2	1929	1324	0.11%	0.011%
53	22.853	3360	3364	3371	rVB7	8740	16315	1.34%	0.130%
54	23.441	3462	3464	3471	rBV6	3323	5442	0.45%	0.043%
55	23.611	3488	3493	3501	rVB3	15331	32138	2.65%	0.256%
56	24.305	3600	3611	3628	rBV2	310129	1084267	89.24%	8.646%
57	24.516	3638	3647	3674	rVB	252233	853712	70.27%	6.808%
58	25.568	3819	3826	3834	rVB4	19002	52585	4.33%	0.419%
59	25.821	3867	3869	3870	rBV2	3235	2291	0.19%	0.018%
60	26.602	4000	4002	4004	rBV2	2821	3043	0.25%	0.024%
61	26.843	4035	4043	4057	rVB5	20625	66130	5.44%	0.527%
62	27.301	4119	4121	4125	rBV5	3232	3433	0.28%	0.027%
63	28.788	4372	4374	4375	rBV2	2531	2033	0.17%	0.016%
64	29.716	4530	4532	4535	rBV4	2850	1866	0.15%	0.015%
65	30.168	4607	4609	4610	rBV2	2903	1537	0.13%	0.012%
66	31.814	4887	4889	4890	rBV2	2584	1445	0.12%	0.012%




Sum of corrected areas: 12540537

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
Data File : BG058497.D
Acq On : 27 Jul 2023 12:06
Operator : MA/JU
Sample : PB154055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

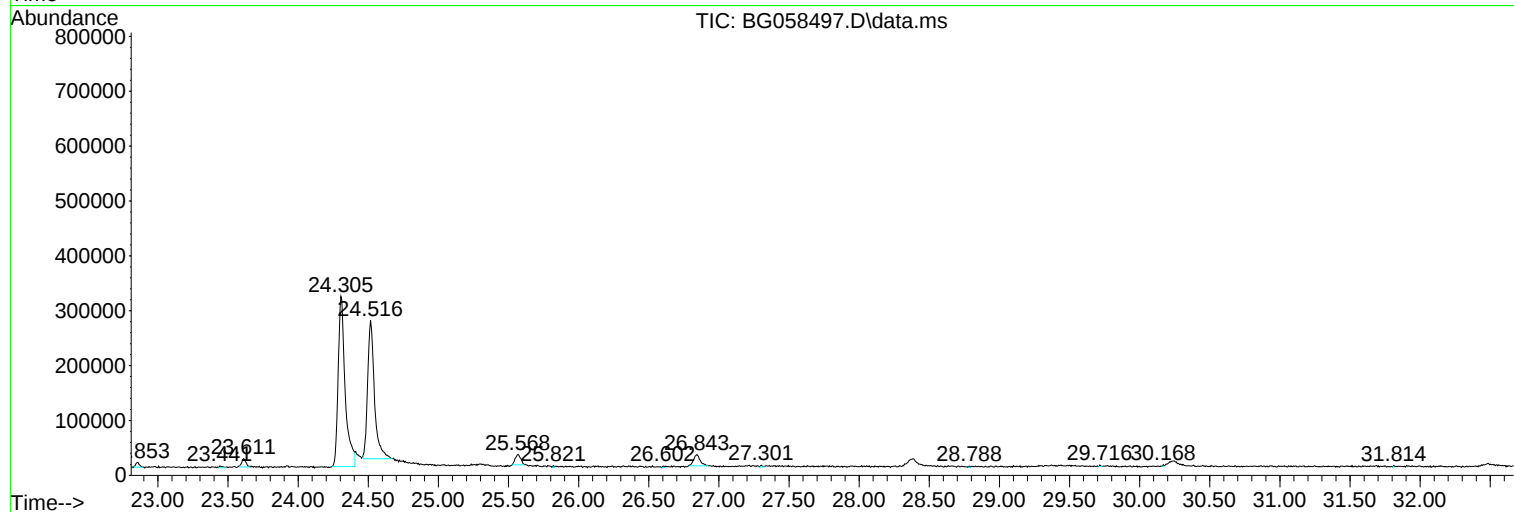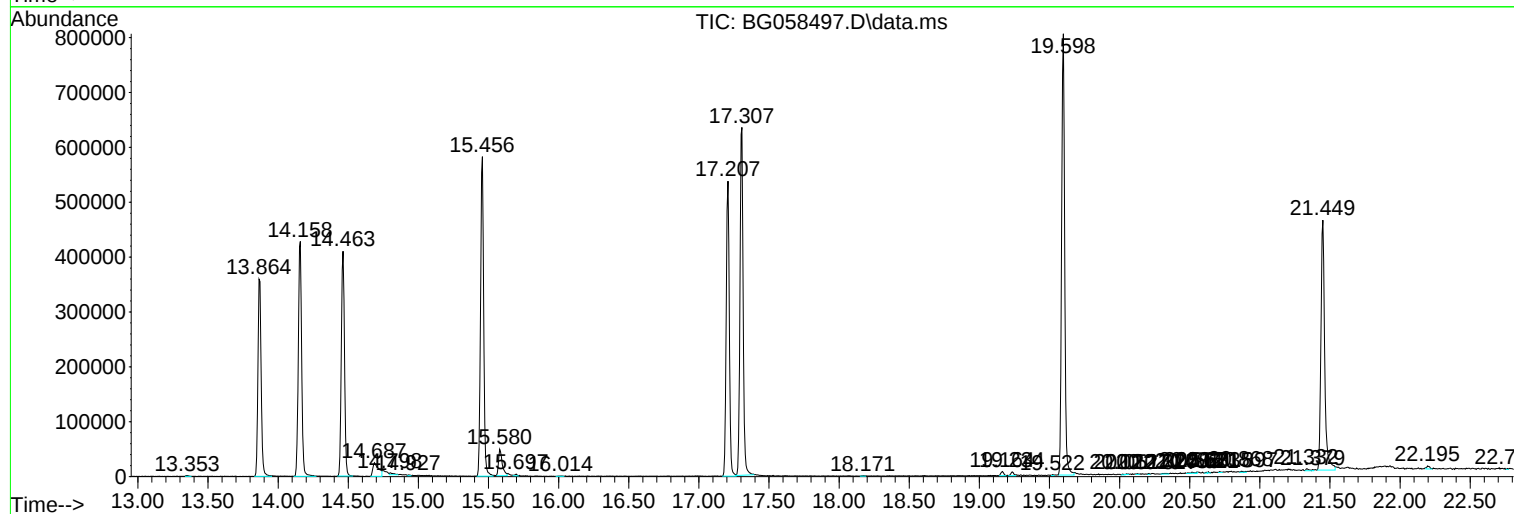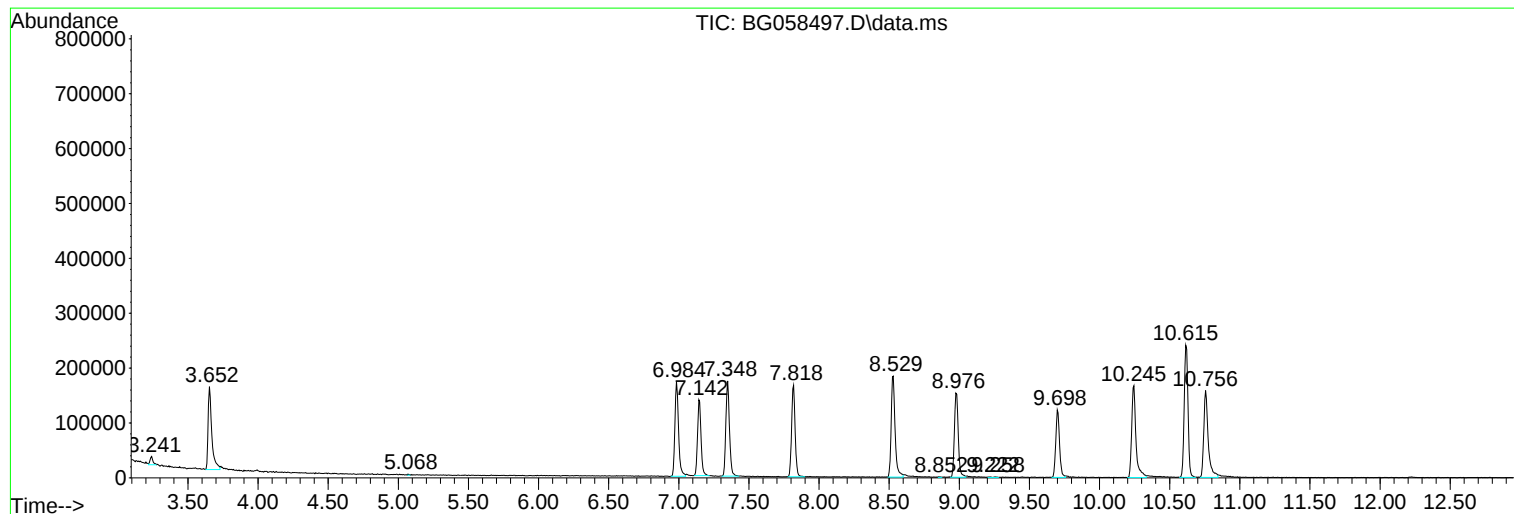

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
Data File : BG058497.D
Acq On : 27 Jul 2023 12:06
Operator : MA/JU
Sample : PB154055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
Data File : BG058497.D
Acq On : 27 Jul 2023 12:06
Operator : MA/JU
Sample : PB154055BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK055

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc