

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
 Data File : BG058499.D
 Acq On : 27 Jul 2023 13:29
 Operator : MA/JU
 Sample : PB154090BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG058499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.235	22	25	36	rVB2	24986	42215	1.88%	0.200%
2	3.652	91	96	117	rBV	278684	514862	22.88%	2.437%
3	3.981	150	152	157	rBV4	3499	5512	0.24%	0.026%
4	6.984	656	663	677	rBV	302337	542374	24.10%	2.567%
5	7.148	684	691	700	rBV	247941	430858	19.14%	2.039%
6	7.348	718	725	739	rBV	307545	548986	24.39%	2.598%
7	7.818	798	805	814	rBV	201509	341742	15.18%	1.617%
8	8.529	918	926	942	rBV	370870	690392	30.68%	3.267%
9	8.981	994	1003	1021	rBV	294903	555611	24.69%	2.630%
10	9.698	1117	1125	1139	rBV	243418	455094	20.22%	2.154%
11	10.239	1208	1217	1238	rBV	347232	686650	30.51%	3.250%
12	10.615	1271	1281	1293	rBV	303074	539652	23.98%	2.554%
13	10.756	1297	1305	1324	rBV	328311	678573	30.15%	3.211%
14	12.219	1550	1554	1560	rBV2	3435	6711	0.30%	0.032%
15	13.353	1743	1747	1752	rBV2	3588	5327	0.24%	0.025%
16	13.870	1828	1835	1851	rBV	743644	1078769	47.93%	5.105%
17	14.157	1877	1884	1895	rBV	841323	1339071	59.50%	6.337%
18	14.463	1928	1936	1946	rBV	497403	782057	34.75%	3.701%
19	14.675	1966	1972	1988	rBV	121435	313728	13.94%	1.485%
20	15.456	2098	2105	2118	rBV	1140986	1692839	75.22%	8.012%
21	15.579	2120	2126	2142	rVV	194059	332799	14.79%	1.575%
22	15.697	2142	2146	2150	rVV6	6980	12379	0.55%	0.059%
23	17.207	2396	2403	2413	rBV	657885	1001523	44.50%	4.740%
24	17.307	2413	2420	2437	rVV	1213624	1875736	83.35%	8.877%
25	19.163	2731	2736	2742	rBV2	15153	20948	0.93%	0.099%
26	19.234	2742	2748	2756	rBV	12903	19822	0.88%	0.094%
27	19.528	2794	2798	2804	rBV4	3693	6417	0.29%	0.030%
28	19.598	2804	2810	2824	rBV	1539539	2250549	100.00%	10.651%
29	20.562	2971	2974	2979	rBV7	6273	8926	0.40%	0.042%
30	20.620	2982	2984	2989	rVB3	2069	2637	0.12%	0.012%
31	20.885	3027	3029	3033	rVB4	2499	2328	0.10%	0.011%
32	20.920	3033	3035	3038	rBV3	2414	2663	0.12%	0.013%
33	21.331	3101	3105	3111	rBV5	7200	13119	0.58%	0.062%
34	21.449	3118	3125	3139	rBV	566796	1047827	46.56%	4.959%
35	22.201	3250	3253	3260	rVB7	4940	8439	0.37%	0.040%
36	22.589	3317	3319	3324	rVB6	2763	4713	0.21%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
 Data File : BG058499.D
 Acq On : 27 Jul 2023 13:29
 Operator : MA/JU
 Sample : PB154090BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M

Title : SVOA CALIBRATION

37	22.859	3360	3365	3371	rBV5	8490	17542	0.78%	0.083%
38	23.611	3489	3493	3500	rVB3	10586	18116	0.80%	0.086%
39	24.310	3601	3612	3638	rBV2	601810	2148523	95.47%	10.168%
40	24.516	3638	3647	3670	rVB2	294248	1033733	45.93%	4.892%
41	25.579	3819	3828	3834	rBV6	12559	36282	1.61%	0.172%
42	28.206	4273	4275	4281	rVB7	3091	2874	0.13%	0.014%
43	28.341	4296	4298	4299	rBV2	4128	3132	0.14%	0.015%
44	28.358	4299	4301	4302	rBV2	3670	2642	0.12%	0.013%
45	31.784	4882	4884	4885	rBV2	2475	2309	0.10%	0.011%
46	32.612	5023	5025	5028	rBV4	2808	2751	0.12%	0.013%




Sum of corrected areas: 21129752

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
Data File : BG058499.D
Acq On : 27 Jul 2023 13:29
Operator : MA/JU
Sample : PB154090BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

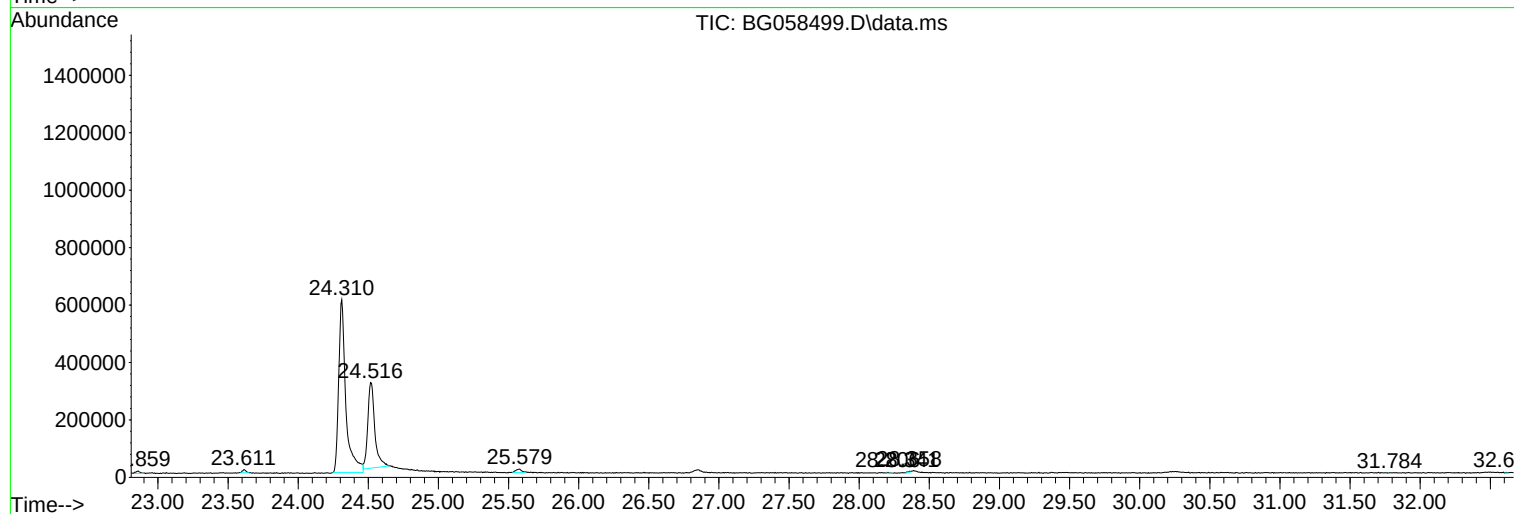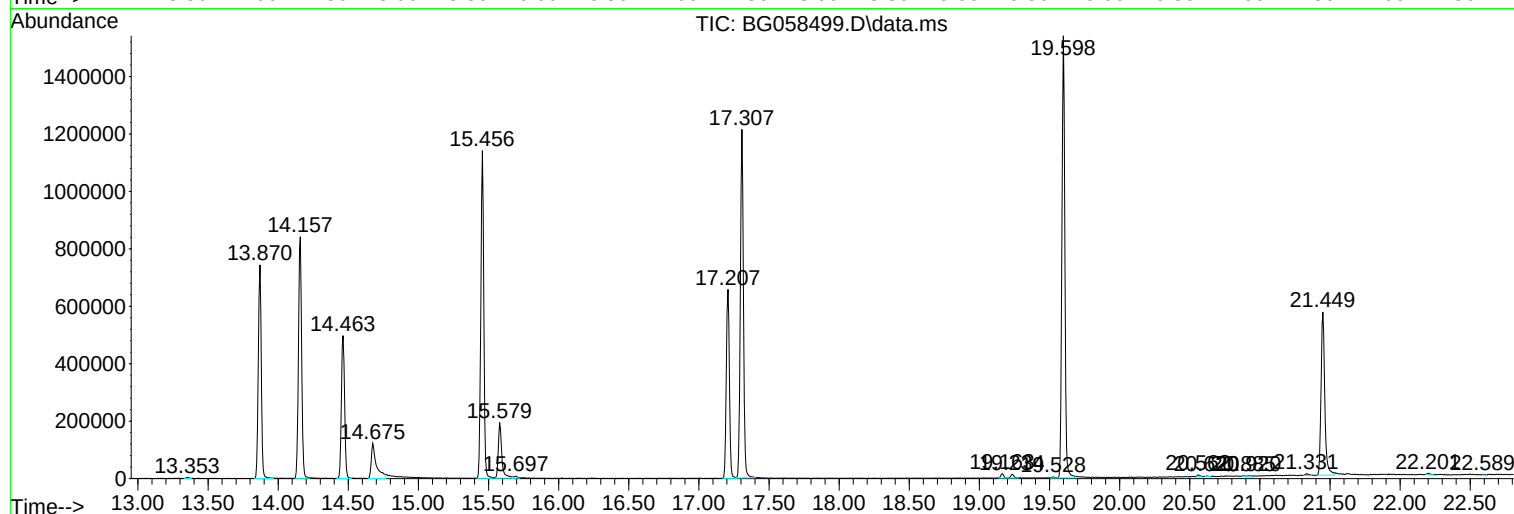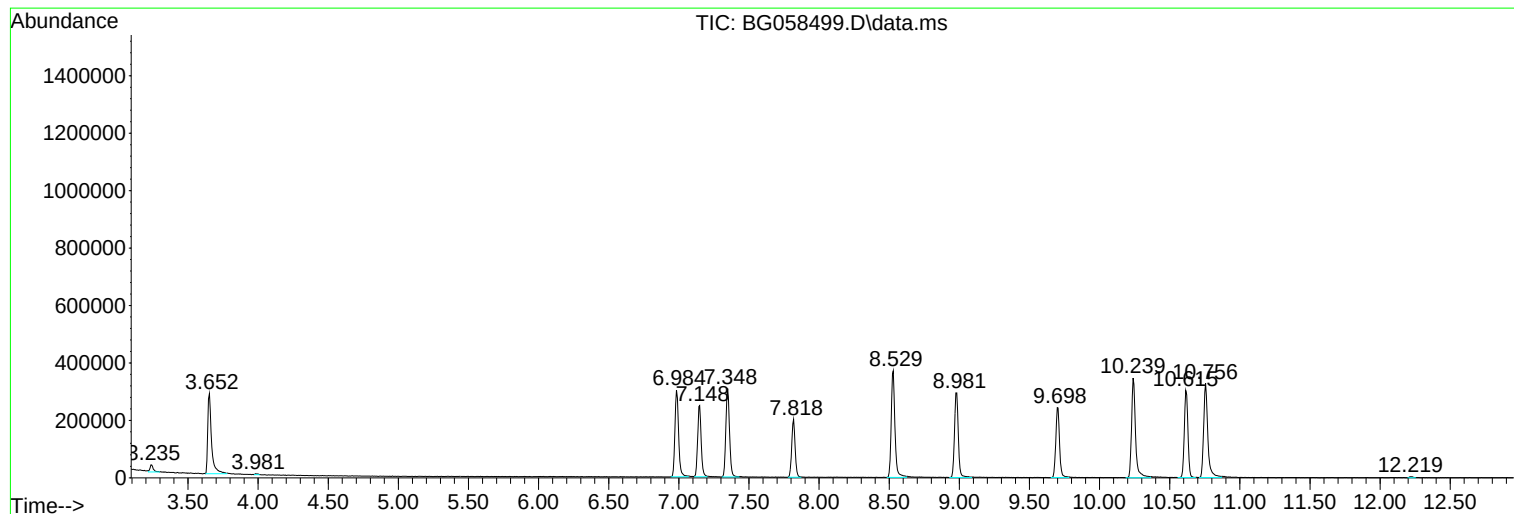

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
Data File : BG058499.D
Acq On : 27 Jul 2023 13:29
Operator : MA/JU
Sample : PB154090BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072723\
Data File : BG058499.D
Acq On : 27 Jul 2023 13:29
Operator : MA/JU
Sample : PB154090BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc