
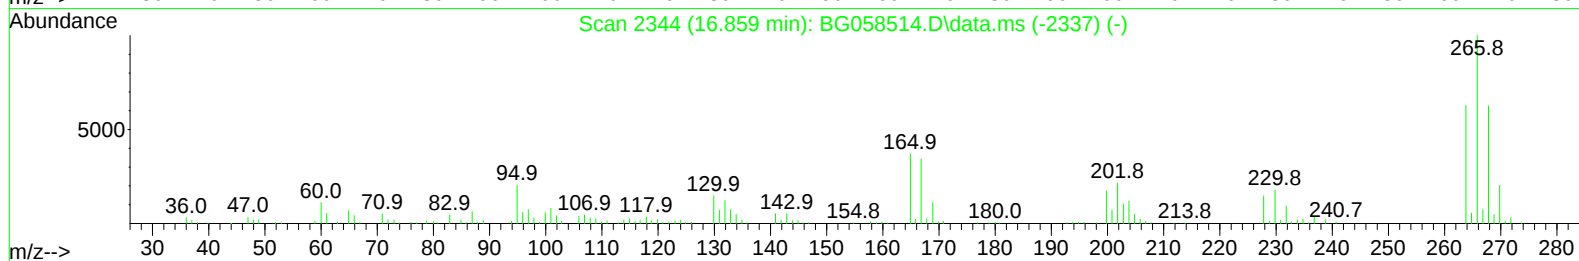
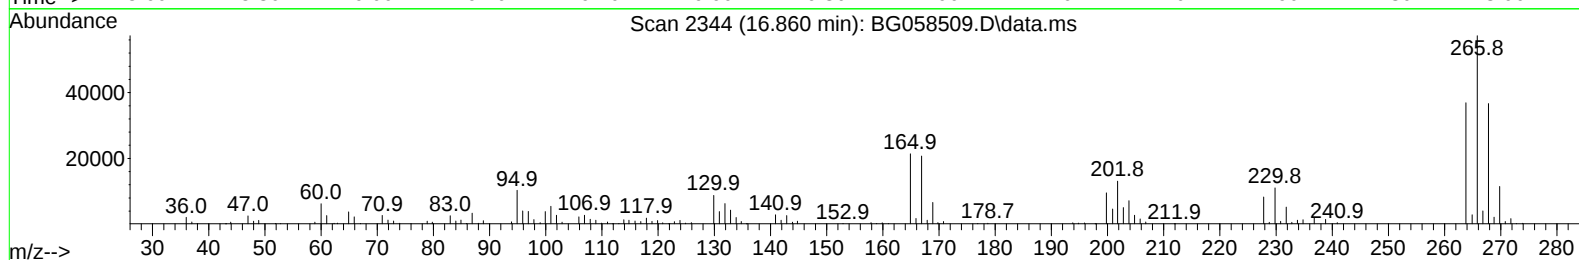


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058509.D
Acq On : 28 Jul 2023 8:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 15:27:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 14:44:42 2023
Response via : Initial Calibration

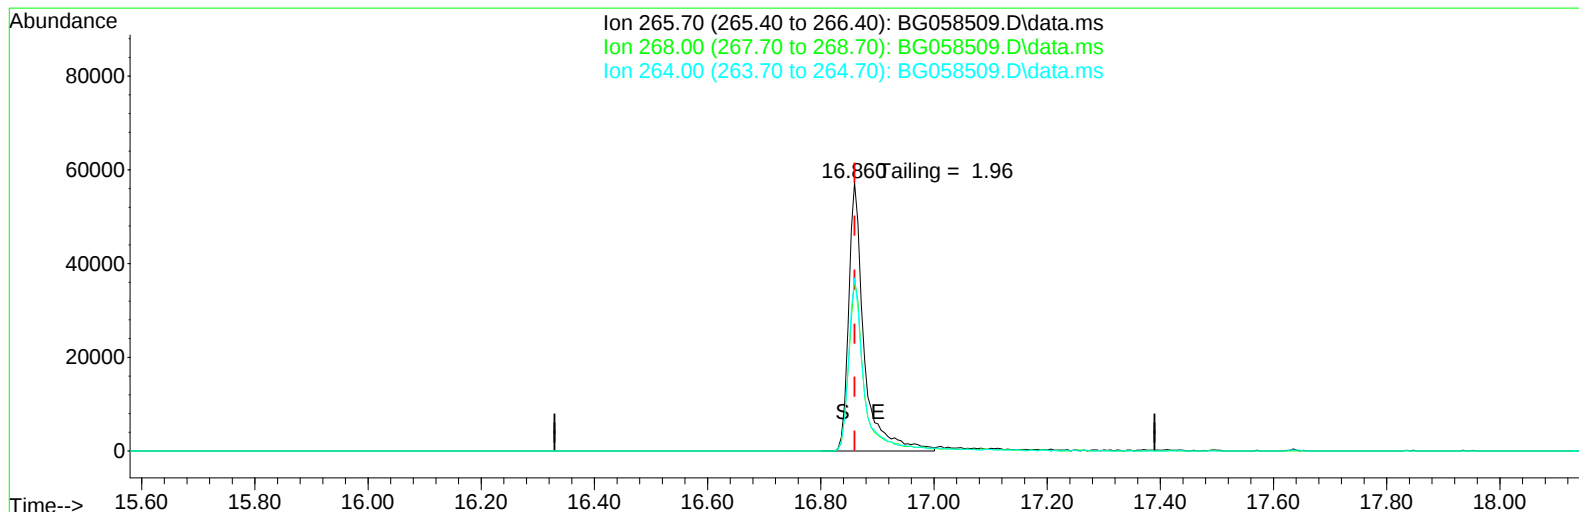

TIC: BG058509.D\data.ms

(70) Pentachlorophenol (C)




16.860min (+ 0.000) 26830.98 ng

response 109111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	63.99
264.00	63.60	64.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058509.D
Acq On : 28 Jul 2023 8:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 15:27:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 14:44:42 2023
Response via : Initial Calibration

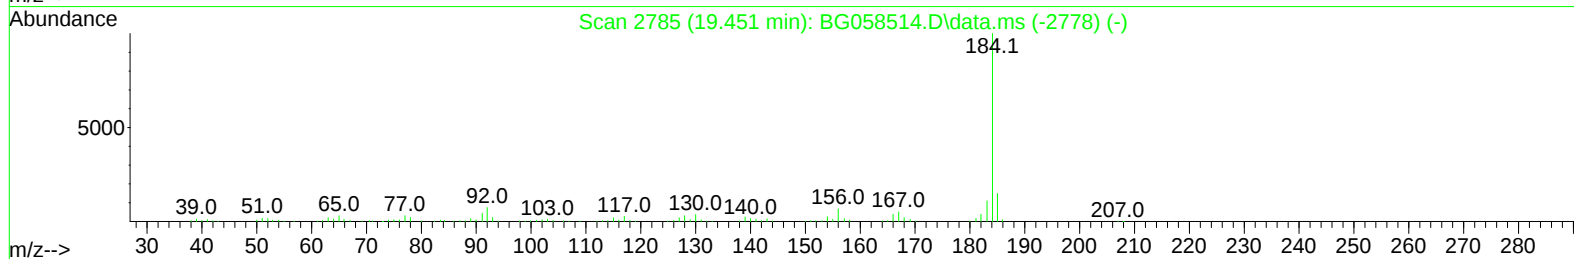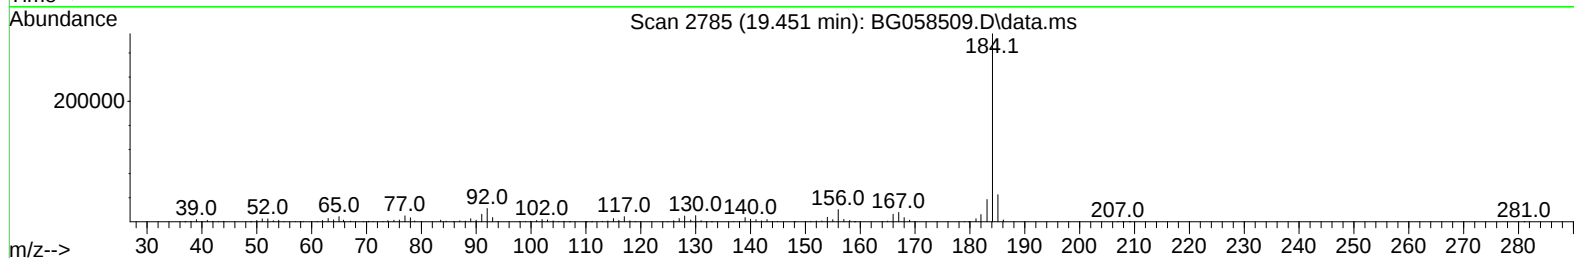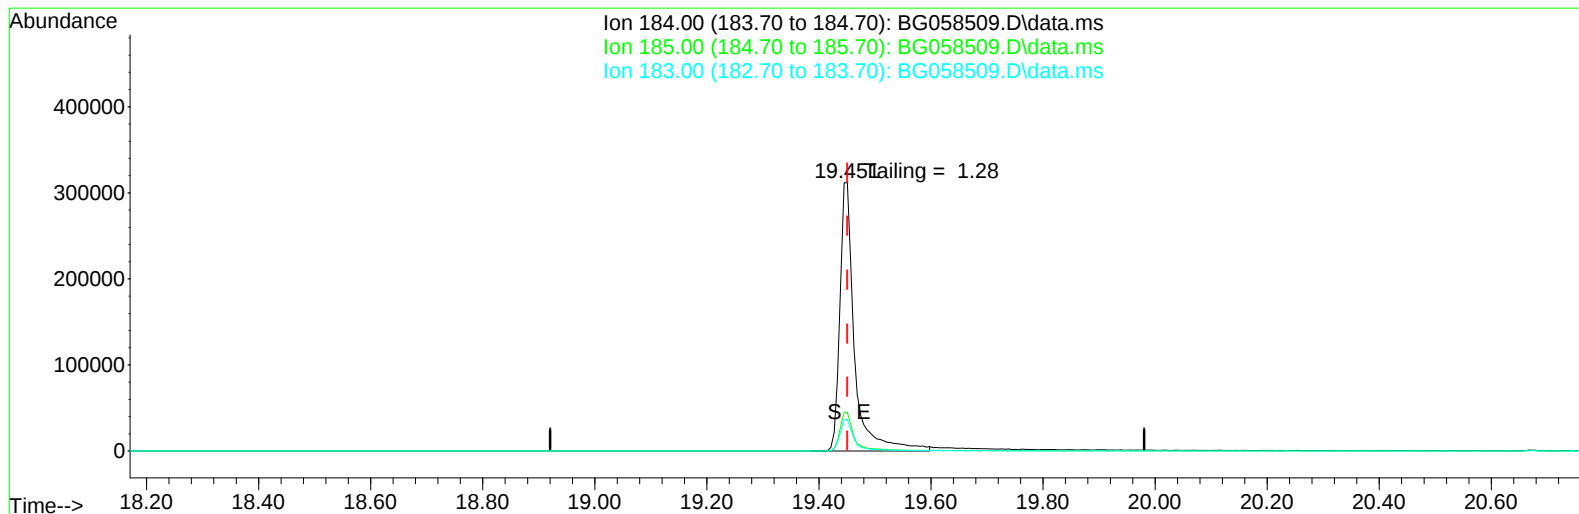

TIC: BG058509.D\data.ms

(77) Benzidine**19.451min (+ 0.000) 689236.40 ng****response 595742**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.46
183.00	11.20	11.87
0.00	0.00	0.00