
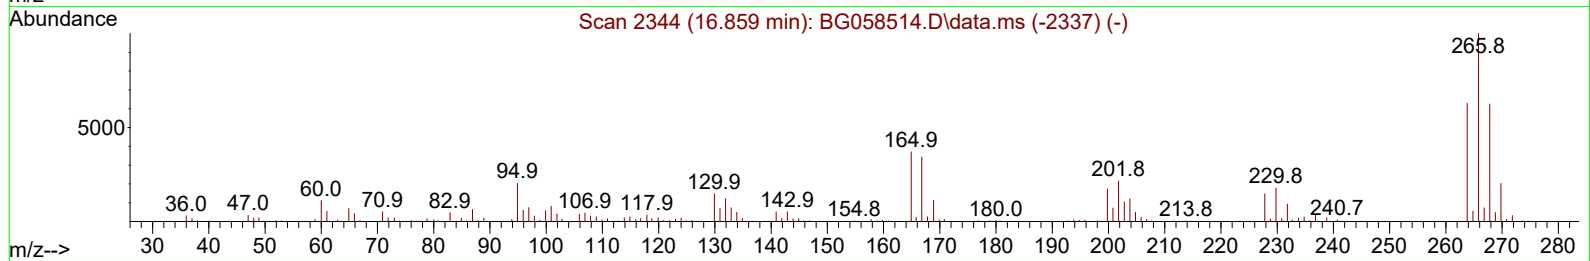
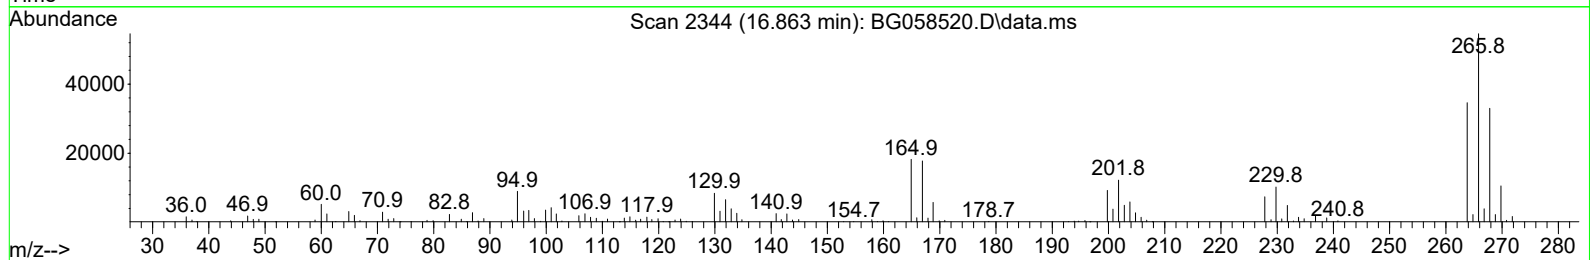


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058520.D
Acq On : 28 Jul 2023 16:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 04:24:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

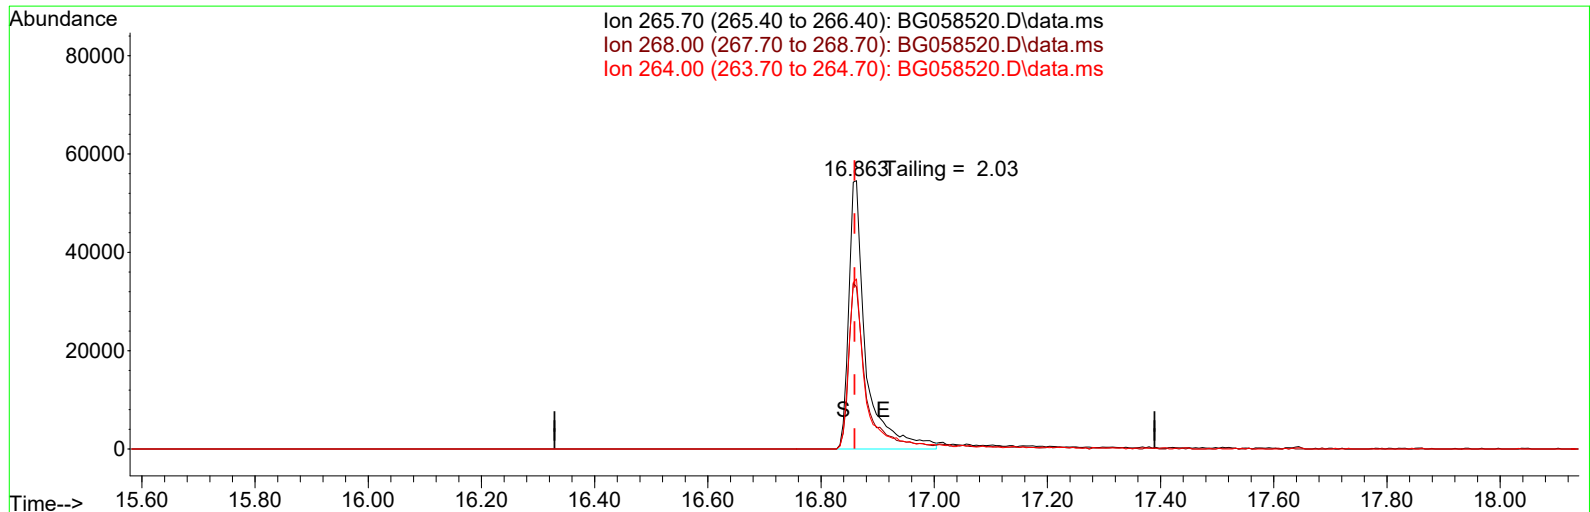

TIC: BG058520.D\data.ms

(70) Pentachlorophenol (C)




16.863min (+ 0.004) 25228.78 ng

response 116359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	60.44
264.00	62.80	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058520.D
Acq On : 28 Jul 2023 16:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 04:24:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

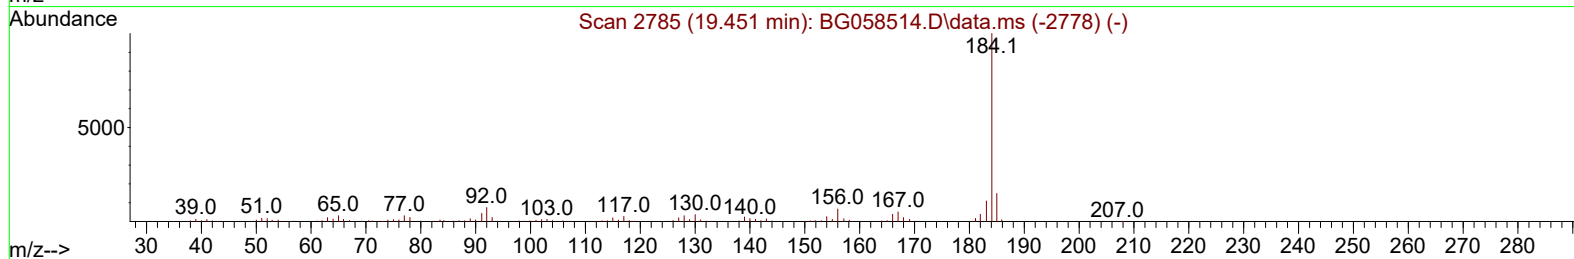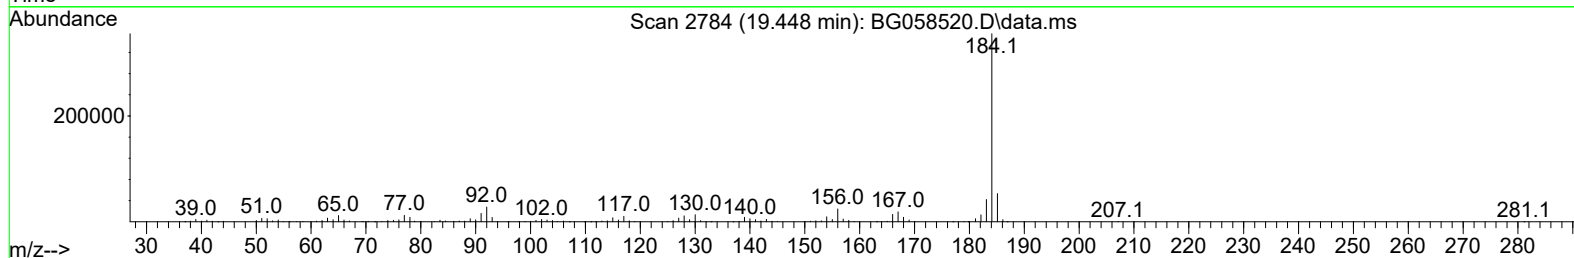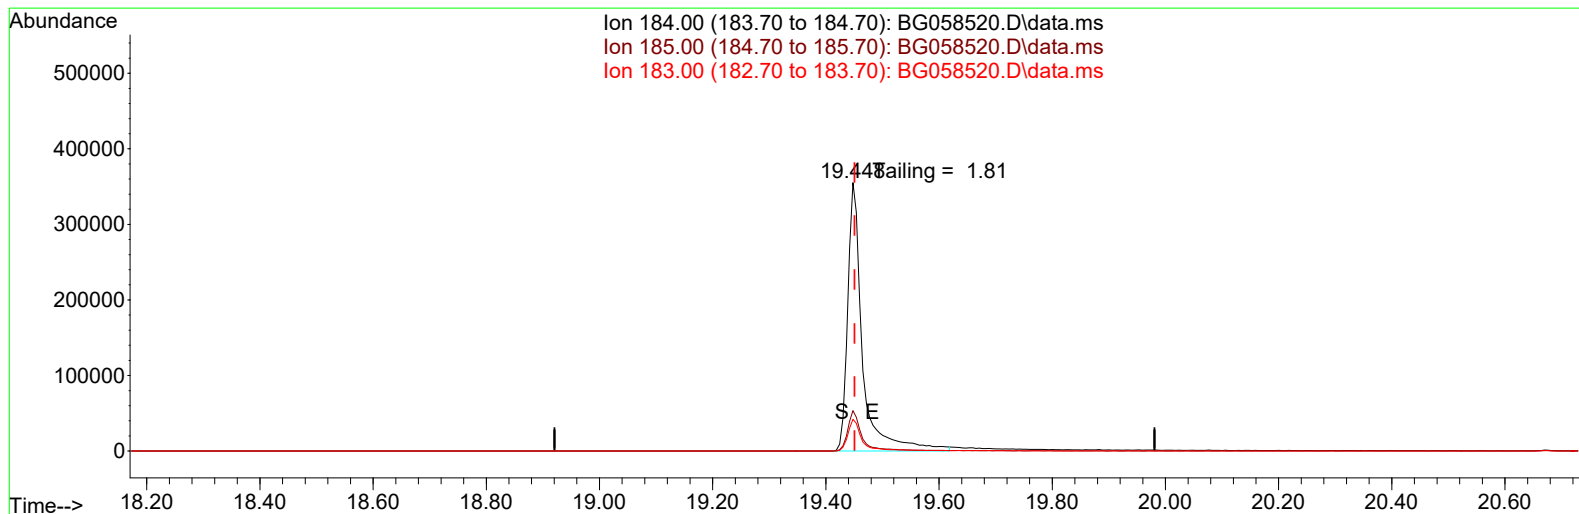

TIC: BG058520.D\data.ms

(77) Benzidine

19.448min (-0.003) 0.00 ng

response 642024

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.02
183.00	10.90	11.85
0.00	0.00	0.00