

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
 Data File : BG058519.D
 Acq On : 28 Jul 2023 15:32
 Operator : MA/JU
 Sample : PB154316BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB154316BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG058519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.909	305	310	317	rBV	29553	43944	1.04%	0.260%
2	5.385	384	391	404	rBV	1009428	1589767	37.78%	9.399%
3	6.989	656	664	682	rBV	910473	1589187	37.77%	9.396%
4	7.811	798	804	815	rVB	164570	277288	6.59%	1.639%
5	8.974	992	1002	1020	rBV	525019	980757	23.31%	5.799%
6	10.614	1274	1281	1298	rBV	204789	397552	9.45%	2.351%
7	13.081	1694	1701	1716	rBV	1392984	2250813	53.49%	13.308%
8	14.462	1929	1936	1954	rBV	374049	592752	14.09%	3.505%
9	15.949	2183	2189	2214	rBV	1241351	2108434	50.11%	12.466%
10	17.206	2396	2403	2418	rBV	537521	865969	20.58%	5.120%
11	19.826	2843	2849	2864	rBV	3127440	4207670	100.00%	24.878%
12	21.448	3118	3125	3137	rBV	536259	937192	22.27%	5.541%
13	24.515	3636	3647	3667	rBV	354099	1072136	25.48%	6.339%




Sum of corrected areas: 16913461

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058519.D
Acq On : 28 Jul 2023 15:32
Operator : MA/JU
Sample : PB154316BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154316BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

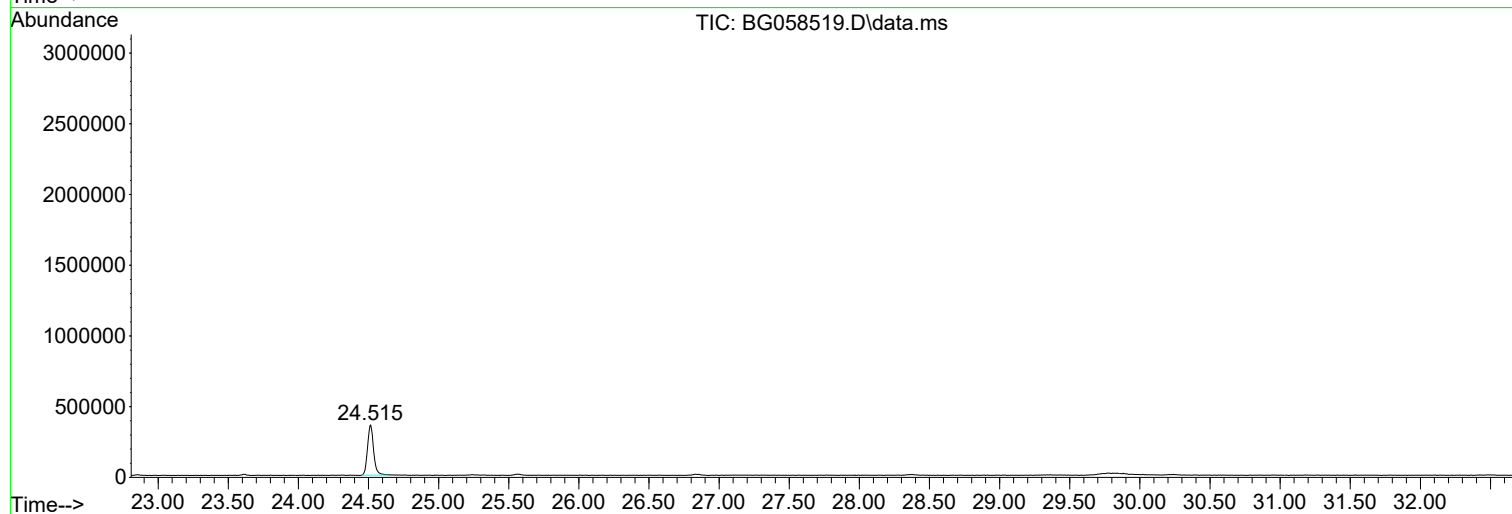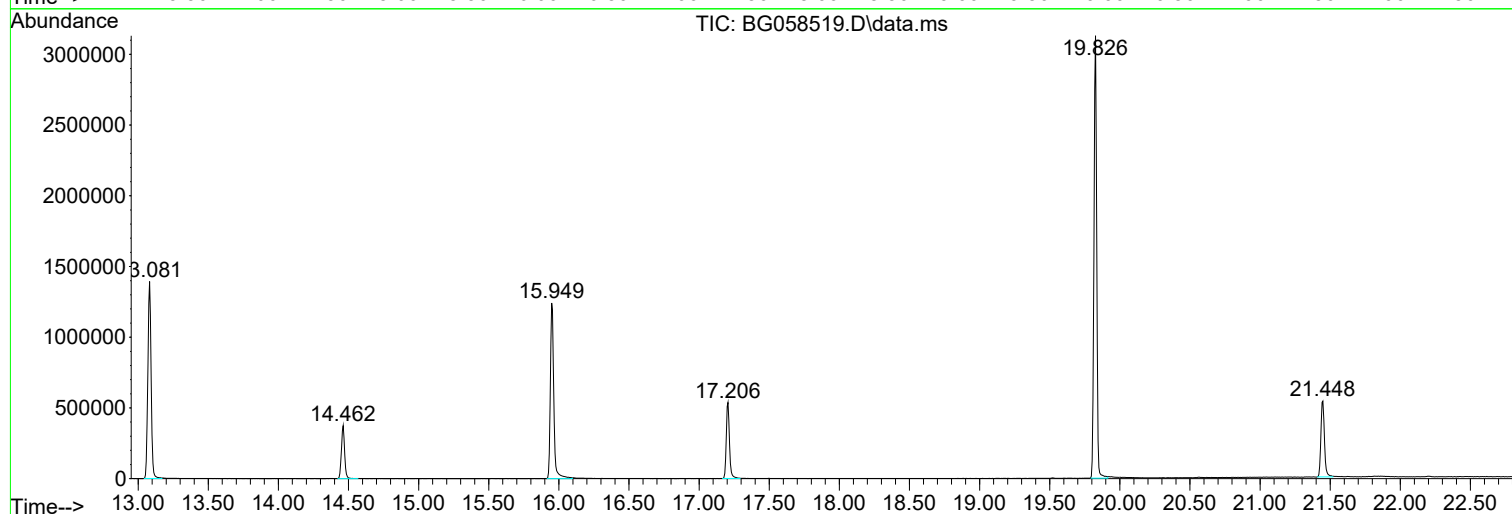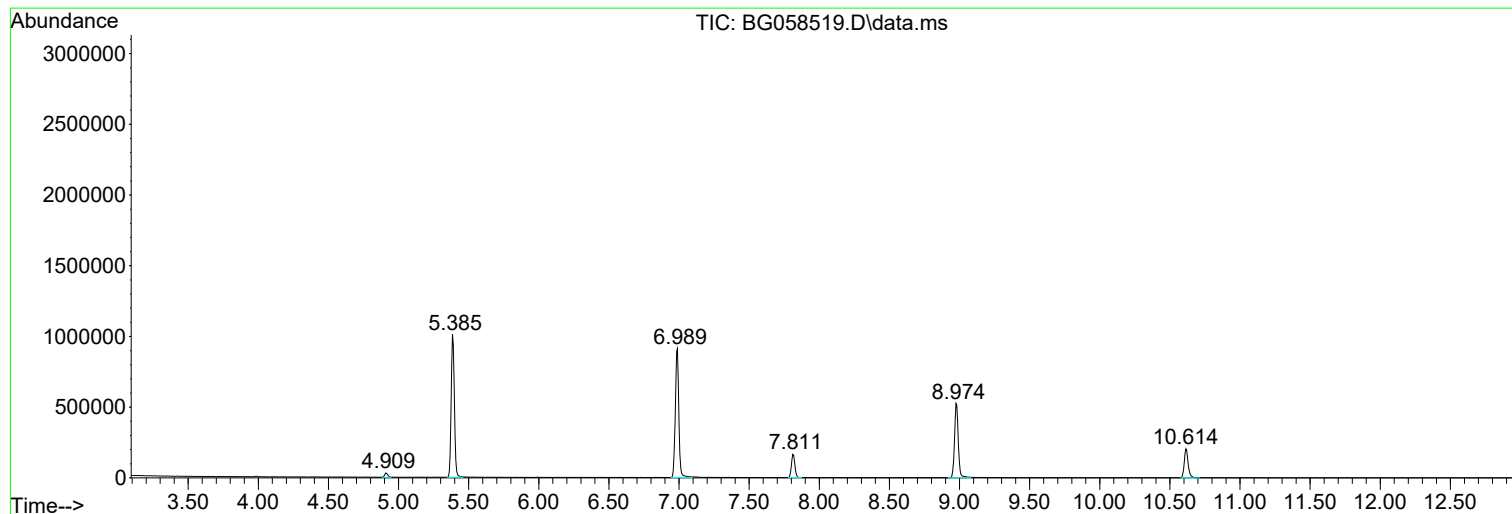

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058519.D
Acq On : 28 Jul 2023 15:32
Operator : MA/JU
Sample : PB154316BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154316BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.909	3.17 ng	43944	1,4-Dichlorobenzene-d4	7.811

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50	
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16	
3	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	
4	4-Penten-2-one, 4-methyl-	98	C6H10O	003744-02-3	9	
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9	

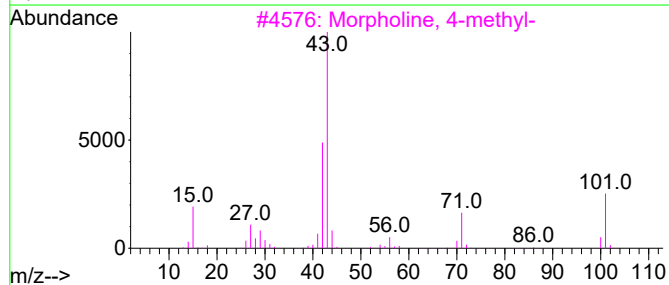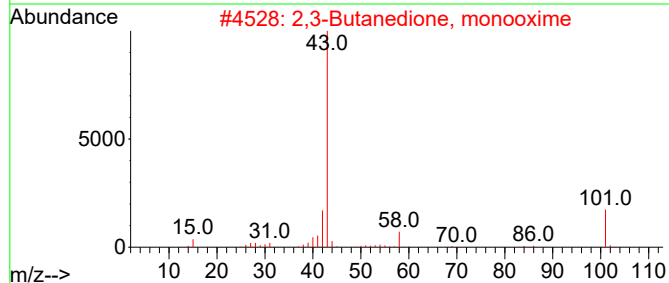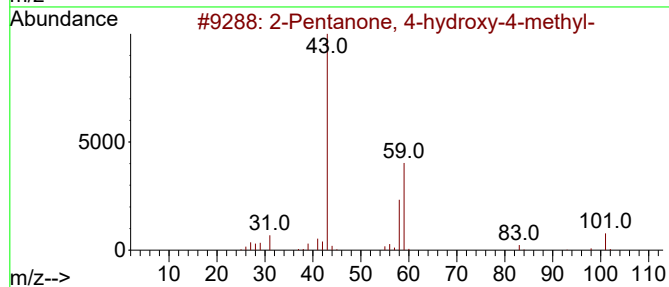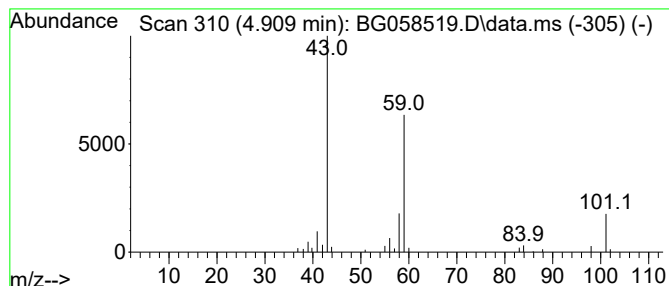

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058519.D
Acq On : 28 Jul 2023 15:32
Operator : MA/JU
Sample : PB154316BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB154316BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.909	3.2	ng	43944	1	7.811	277288	20.0