


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058520.D
Acq On : 28 Jul 2023 16:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

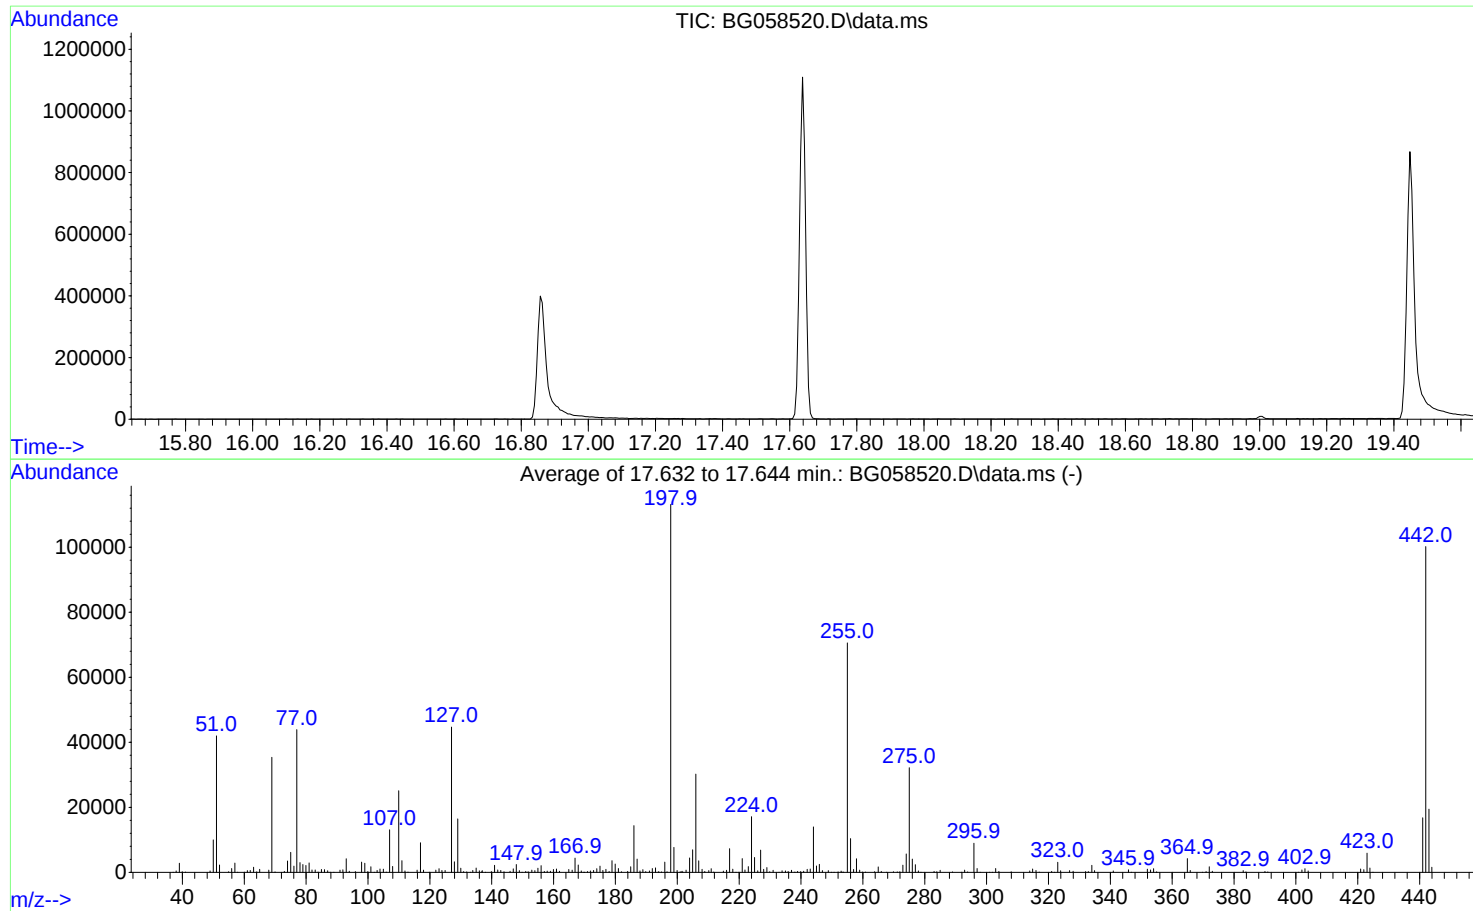




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	41992	PASS
68	69	0.00	2	1.9	688	PASS
69	198	0.00	100	31.3	35400	PASS
70	69	0.00	2	0.4	134	PASS
127	198	10	80	39.5	44693	PASS
197	198	0.00	2	0.2	219	PASS
198	198	100	100	100.0	113139	PASS
199	198	5	9	6.8	7673	PASS
275	198	10	60	28.5	32195	PASS
365	198	1	100	3.7	4212	PASS
441	198	0.01	100	14.8	16792	PASS
442	442	50	100	100.0	100192	PASS
443	442	15	24	19.4	19433	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058520.D
Acq On : 28 Jul 2023 16:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 29 04:24:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

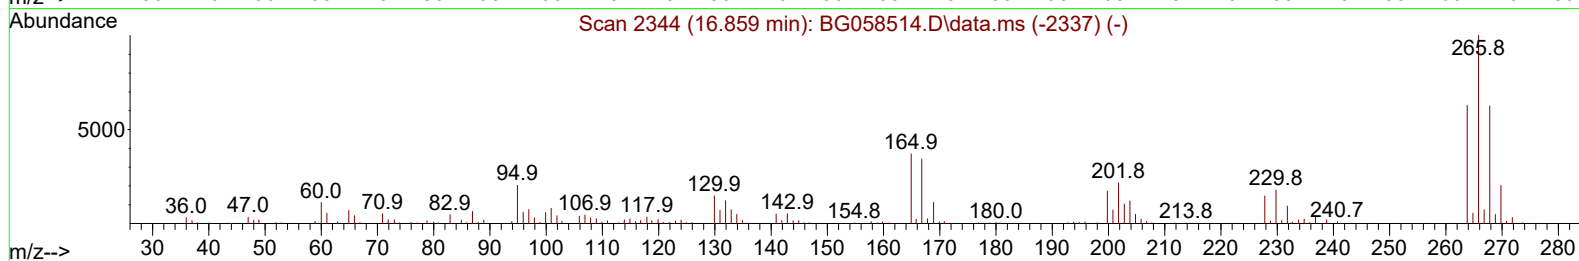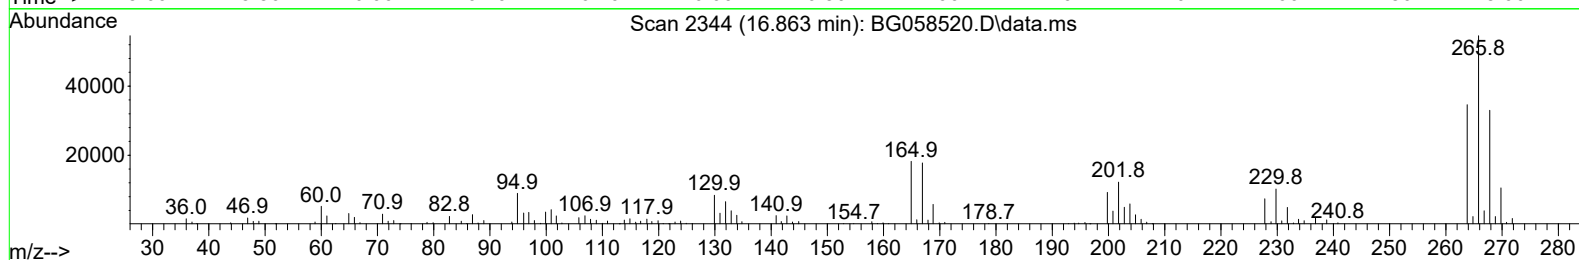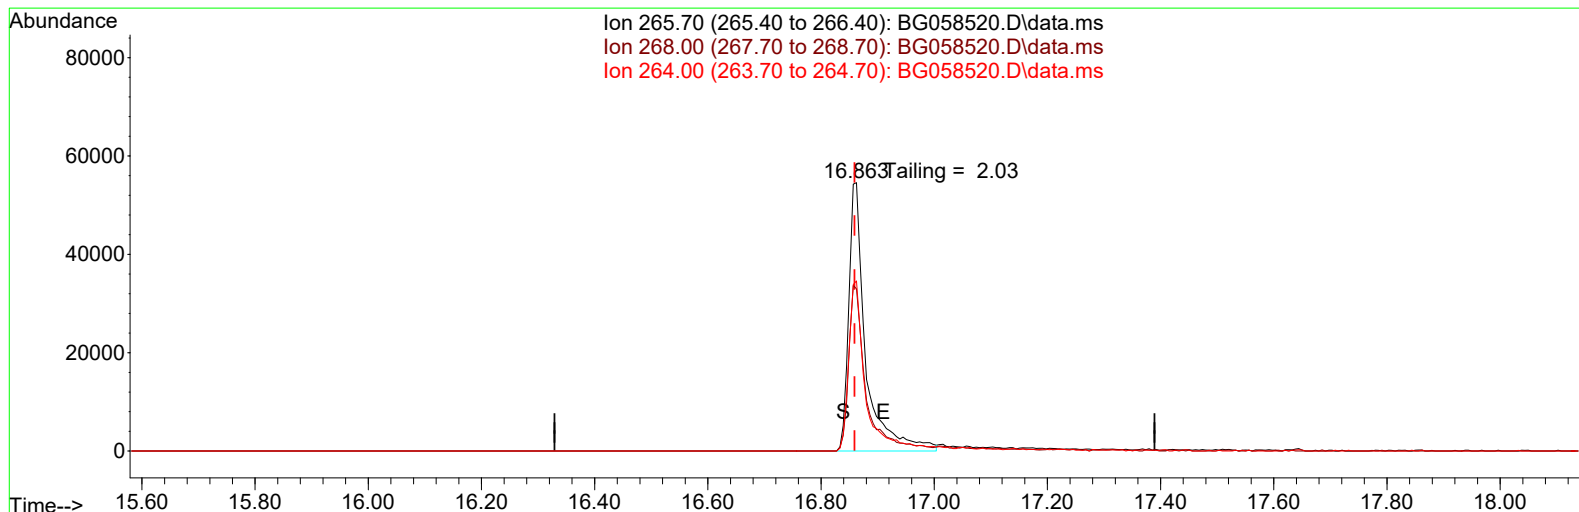

TIC: BG058520.D\data.ms

(70) Pentachlorophenol (C)

16.863min (+ 0.004) 25228.78 ng




response 116359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	60.44
264.00	62.80	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058520.D
Acq On : 28 Jul 2023 16:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 29 04:24:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

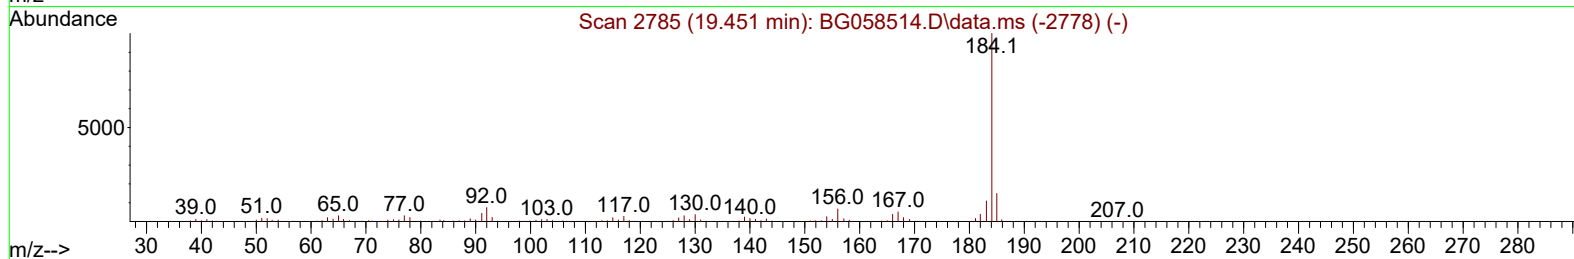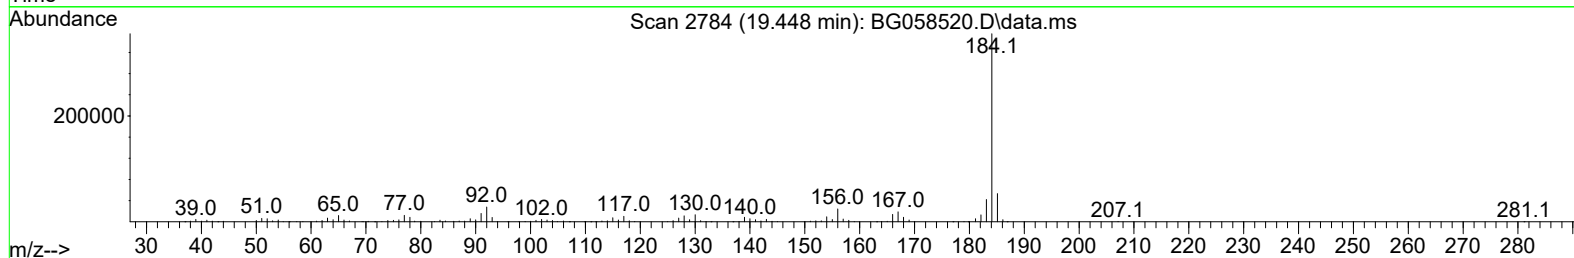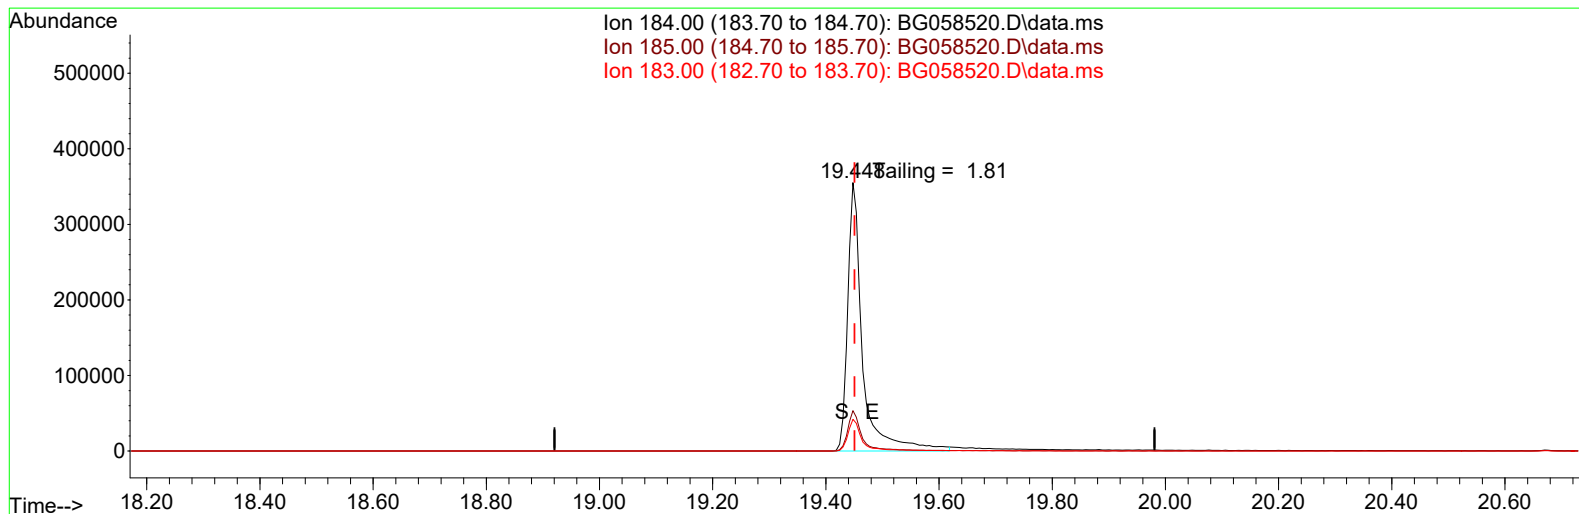

TIC: BG058520.D\data.ms

(77) Benzidine

19.448min (-0.003) 0.00 ng

response 642024

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.02
183.00	10.90	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/28/2023	BNA_G	<u>BG058520.D</u>
Compound Name	Response	Retention Time
DDT	326596	20.676
DDD	37523	20.235
DDE	675	19.73
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38198	364794	10.47

Instrument :
BNA_G
ClientSampleId :
DFTPP