
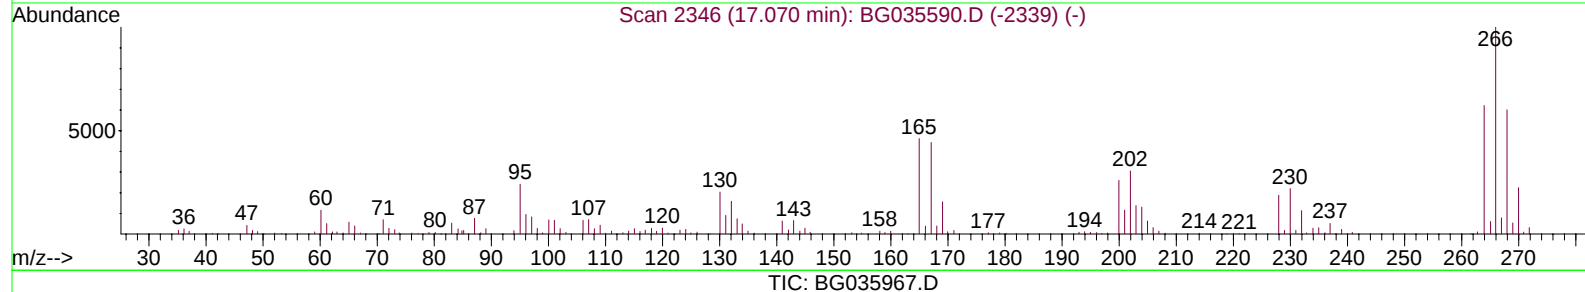
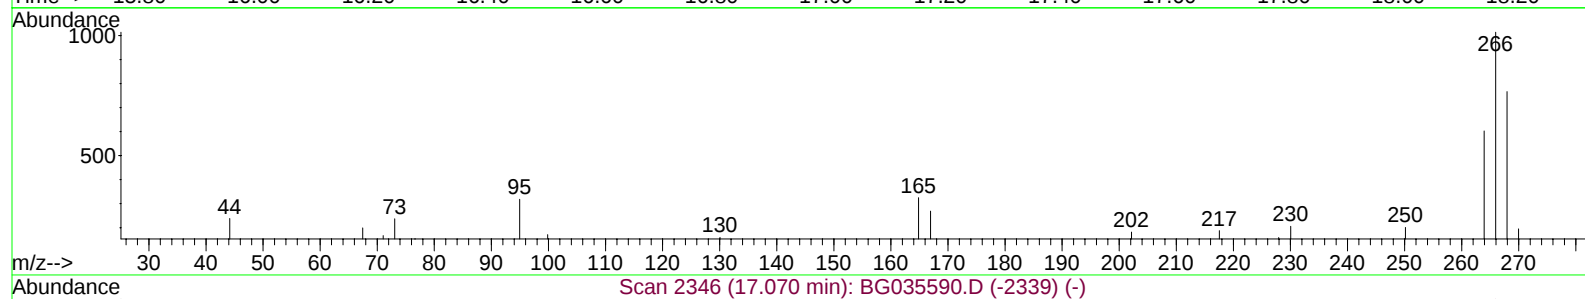


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073018\
Data File : BG035967.D
Acq On : 30 Jul 2018 9:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 14:23:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

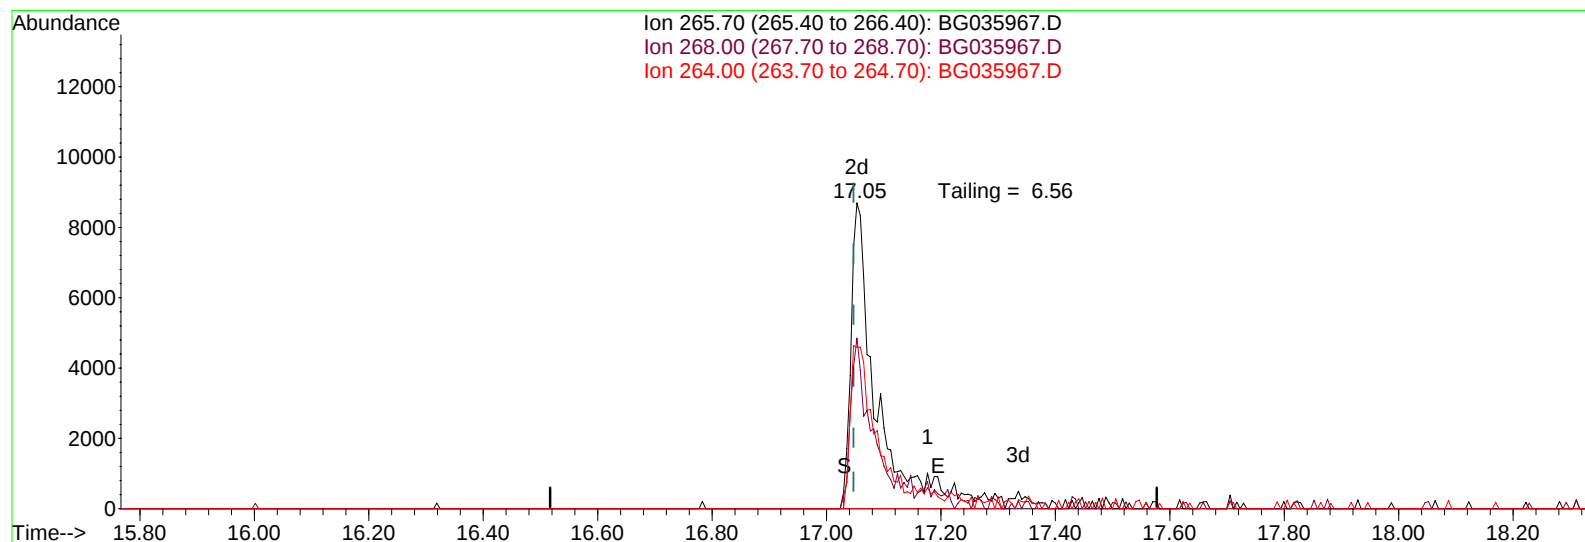

(69) Pentachlorophenol (C)




17.177min (+0.129) 251.04ng

response 844

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	75.64
264.00	62.00	59.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG073018\
Data File : BG035967.D
Acq On : 30 Jul 2018 9:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 14:23:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 25 11:04:14 2018
Response via : Initial Calibration

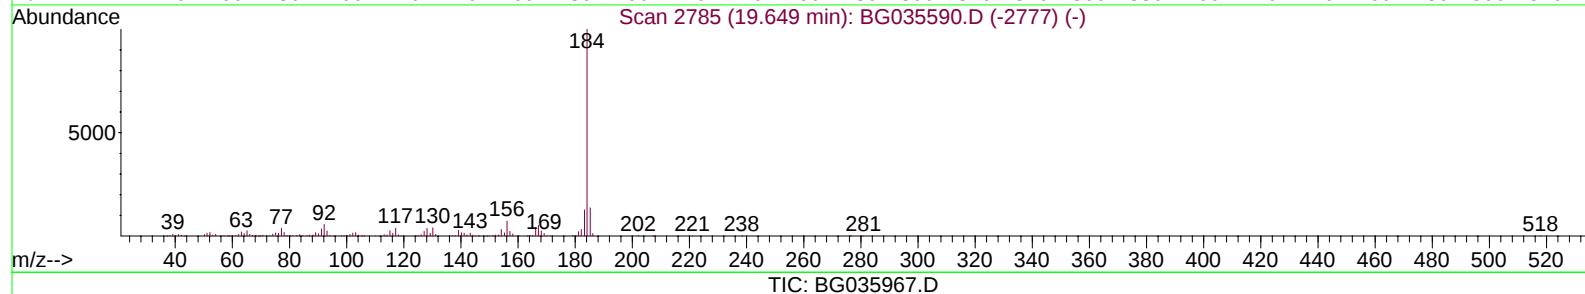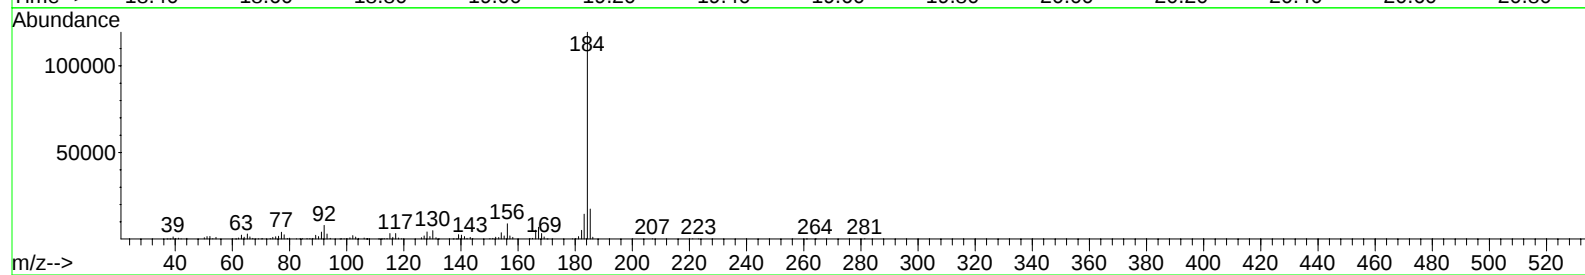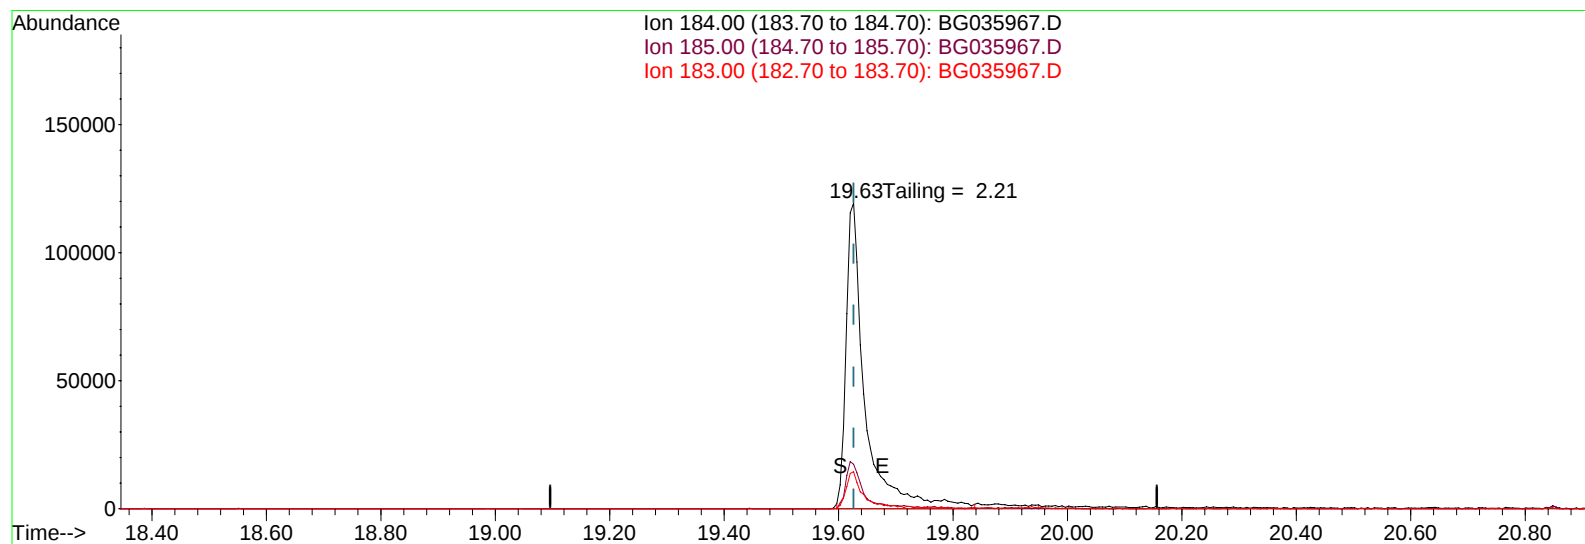

(76) Benzidine

19.626min (-0.000) 0.00ng

response 264079

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.56
183.00	13.30	12.10
0.00	0.00	0.00